

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061021\
 Data File : BM030367.D
 Acq On : 10 Jun 2021 10:29
 Operator : CG/JU
 Sample : PB136969BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB136969BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM030367.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.428	391	398	413	rBV	4534615	6539251	32.89%	8.867%
2	7.010	659	667	677	rBV	4475389	6874278	34.57%	9.321%
3	7.845	802	809	816	rBV	768559	1222936	6.15%	1.658%
4	8.998	997	1005	1020	rBV	2460571	4003622	20.13%	5.429%
5	10.633	1275	1283	1293	rBV	1017669	1710608	8.60%	2.320%
6	13.092	1692	1701	1711	rBV	7305941	10442706	52.52%	14.160%
7	14.468	1928	1935	1942	rBV	1766156	2508388	12.62%	3.401%
8	15.951	2180	2187	2209	rBV	6303461	8643754	43.47%	11.721%
9	17.204	2393	2400	2413	rBV	2389832	3273492	16.46%	4.439%
10	19.821	2838	2845	2850	rBV	15664795	19884090	100.00%	26.962%
11	21.362	3102	3107	3116	rBV	3175503	4249378	21.37%	5.762%
12	23.644	3489	3495	3505	rVB2	2317327	4396330	22.11%	5.961%




Sum of corrected areas: 73748833

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061021\
Data File : BM030367.D
Acq On : 10 Jun 2021 10:29
Operator : CG/JU
Sample : PB136969BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB136969BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

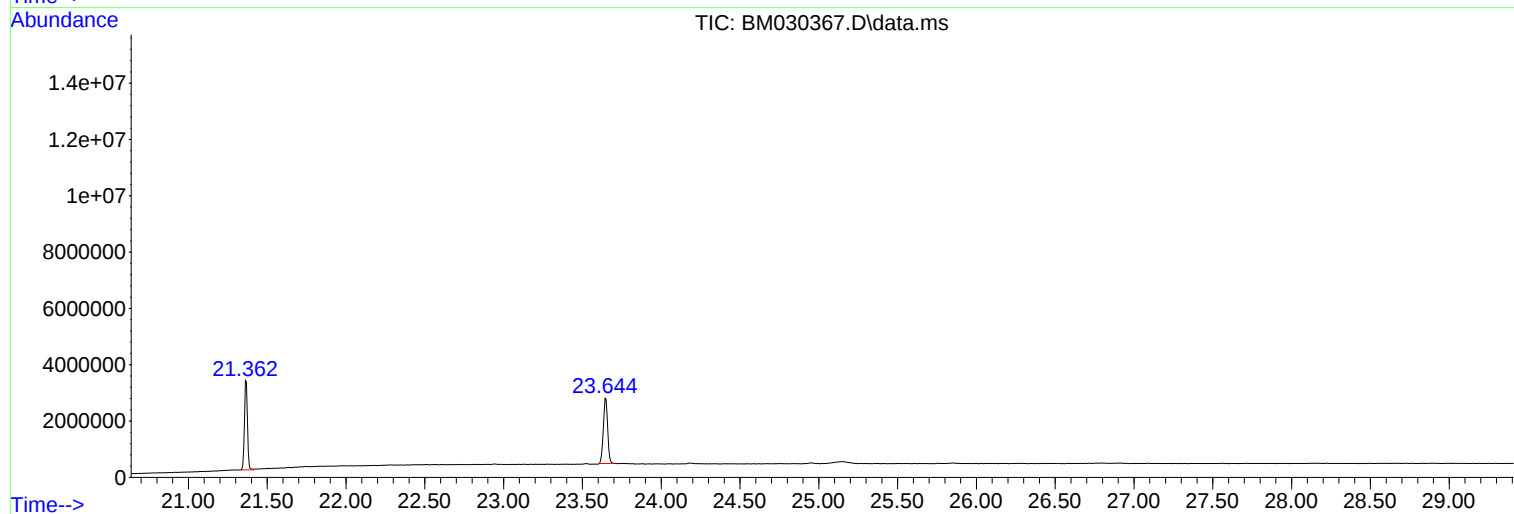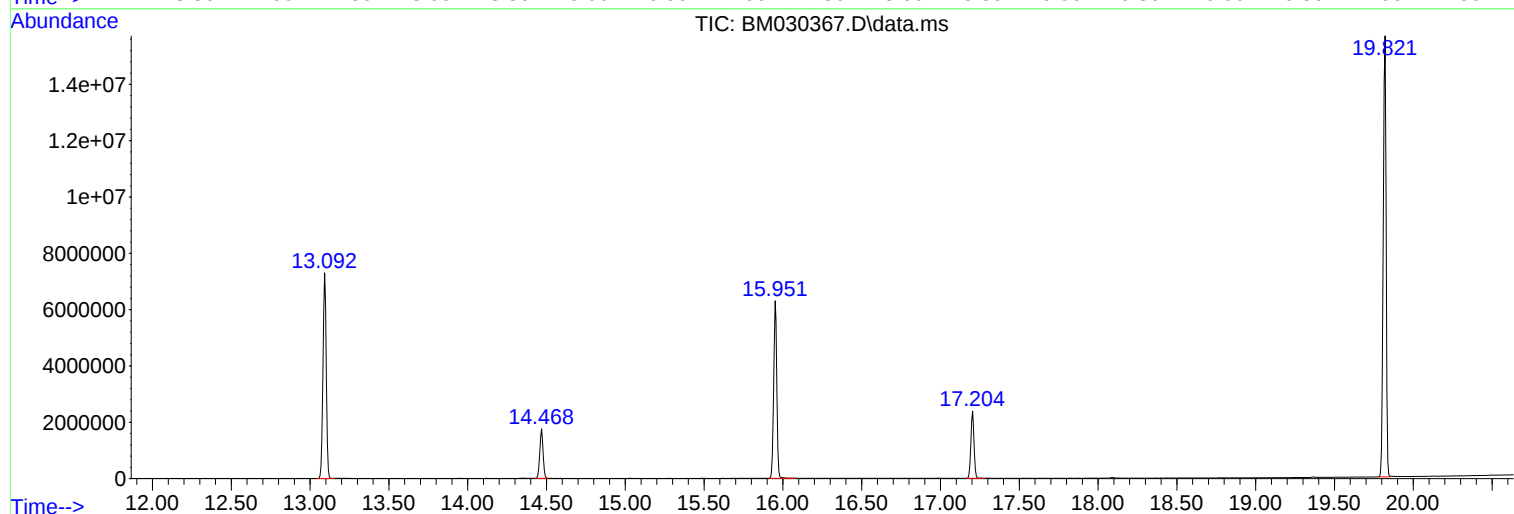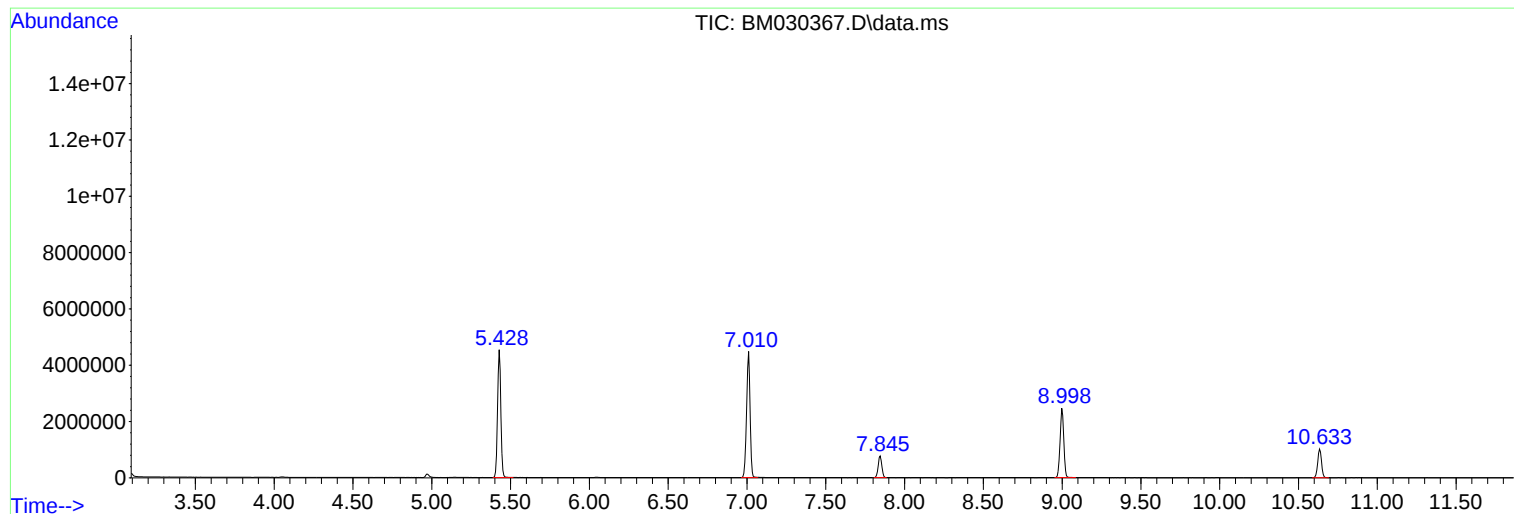

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061021\
Data File : BM030367.D
Acq On : 10 Jun 2021 10:29
Operator : CG/JU
Sample : PB136969BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB136969BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061021\
Data File : BM030367.D
Acq On : 10 Jun 2021 10:29
Operator : CG/JU
Sample : PB136969BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB136969BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------