
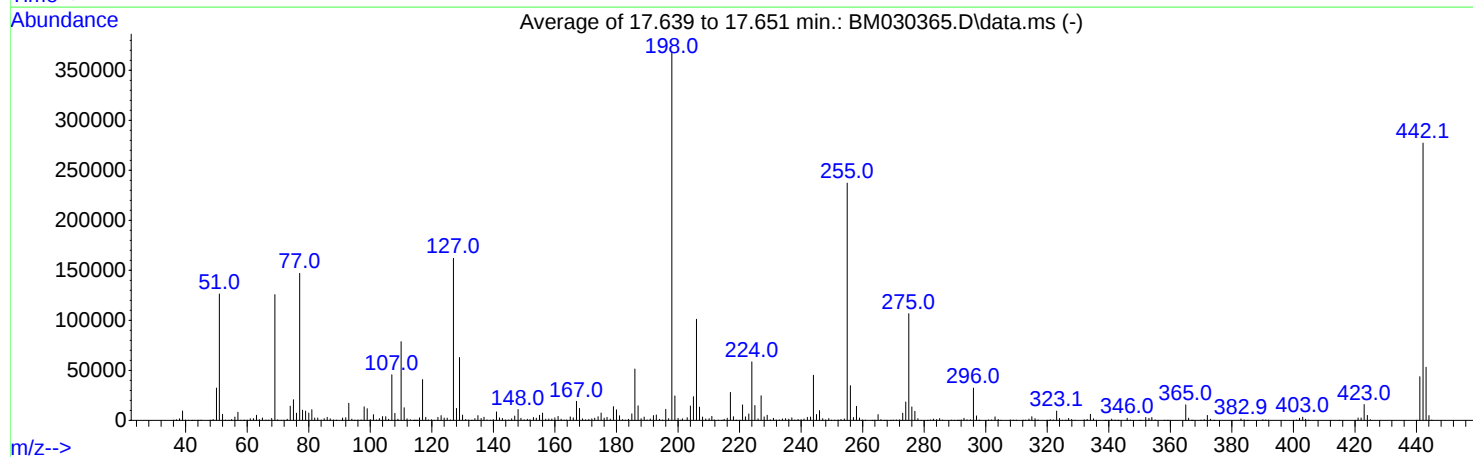


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061021\
 Data File : BM030365.D
 Acq On : 10 Jun 2021 08:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 11 14:10:50 2021

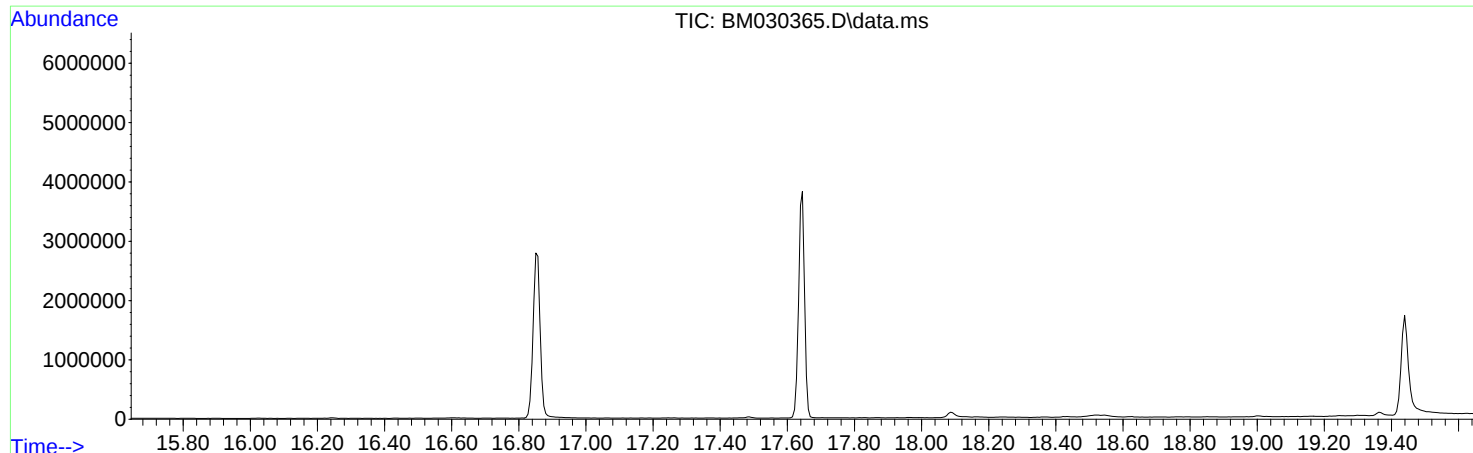




AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2467

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.4	126472	PASS
68	69	0.00	2	1.6	1974	PASS
69	198	0.00	100	34.2	125759	PASS
70	69	0.00	2	0.5	636	PASS
127	198	10	80	44.1	162093	PASS
197	198	0.00	2	0.5	1825	PASS
198	198	100	100	100.0	367829	PASS
199	198	5	9	6.7	24539	PASS
275	198	10	60	29.0	106797	PASS
365	198	1	100	4.2	15522	PASS
441	198	0.01	100	11.9	43635	PASS
442	442	50	100	100.0	277333	PASS
443	442	15	24	19.2	53136	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061021\
Data File : BM030365.D
Acq On : 10 Jun 2021 08:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jun 10 10:33:33 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 08 20:51:08 2021
Response via : Initial Calibration

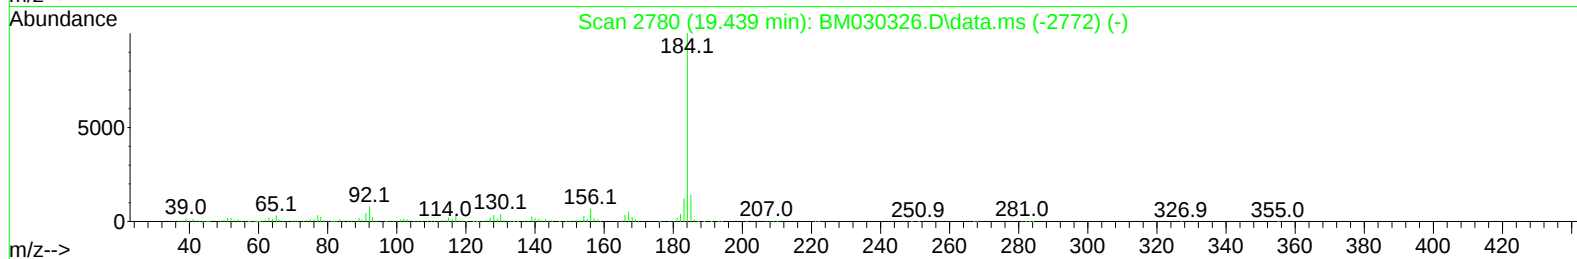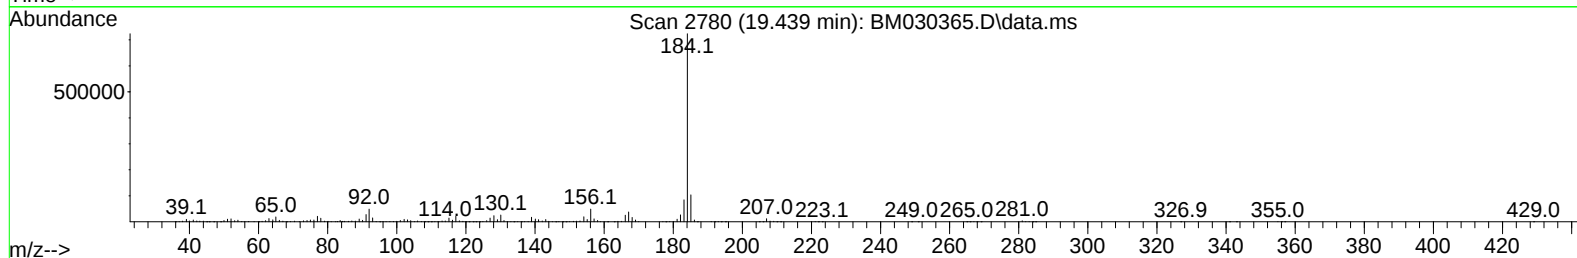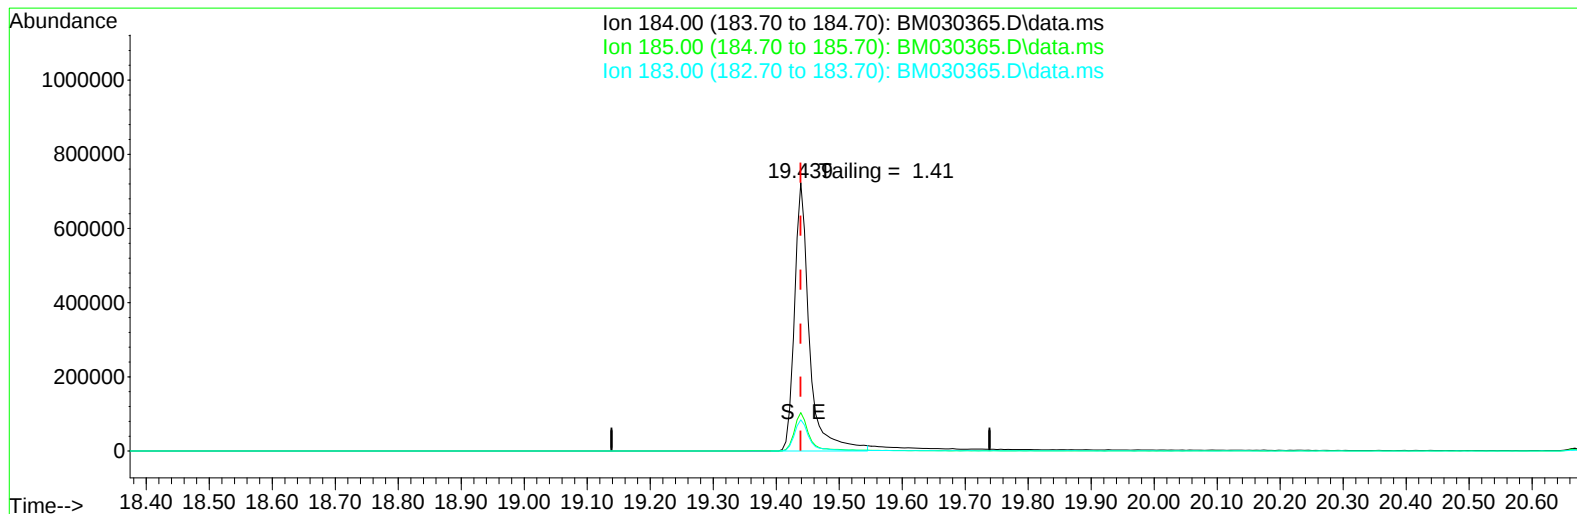

TIC: BM030365.D\data.ms

(77) Benzidine

19.439min (+ 0.000) 1295701.43 ng




response 1260904

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	14.35
183.00	12.30	11.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061021\
 Data File : BM030365.D
 Acq On : 10 Jun 2021 08:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Jun 10 10:33:33 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 08 20:51:08 2021
 Response via : Initial Calibration

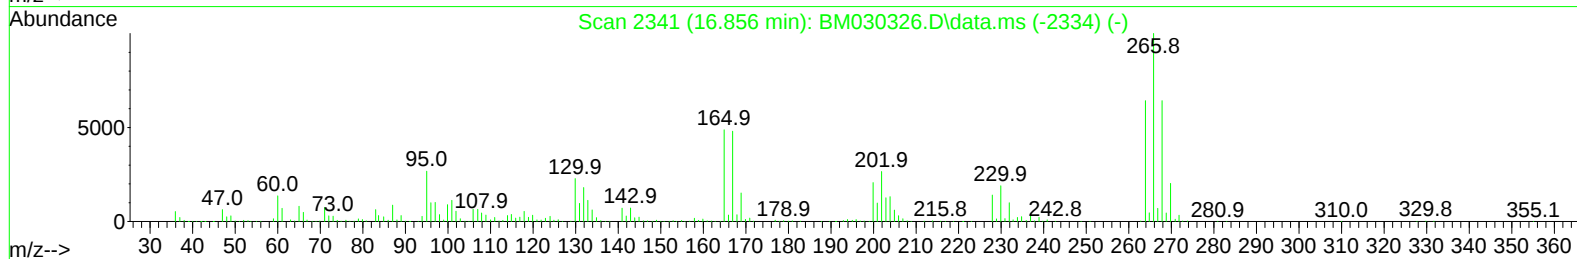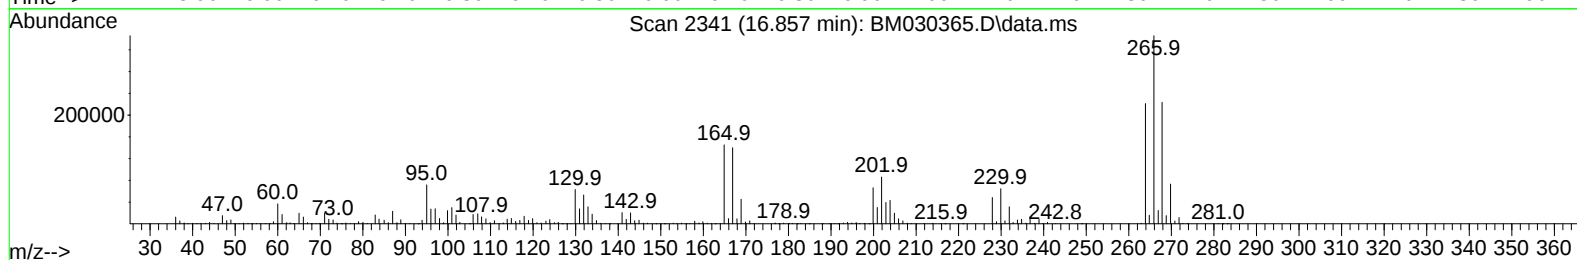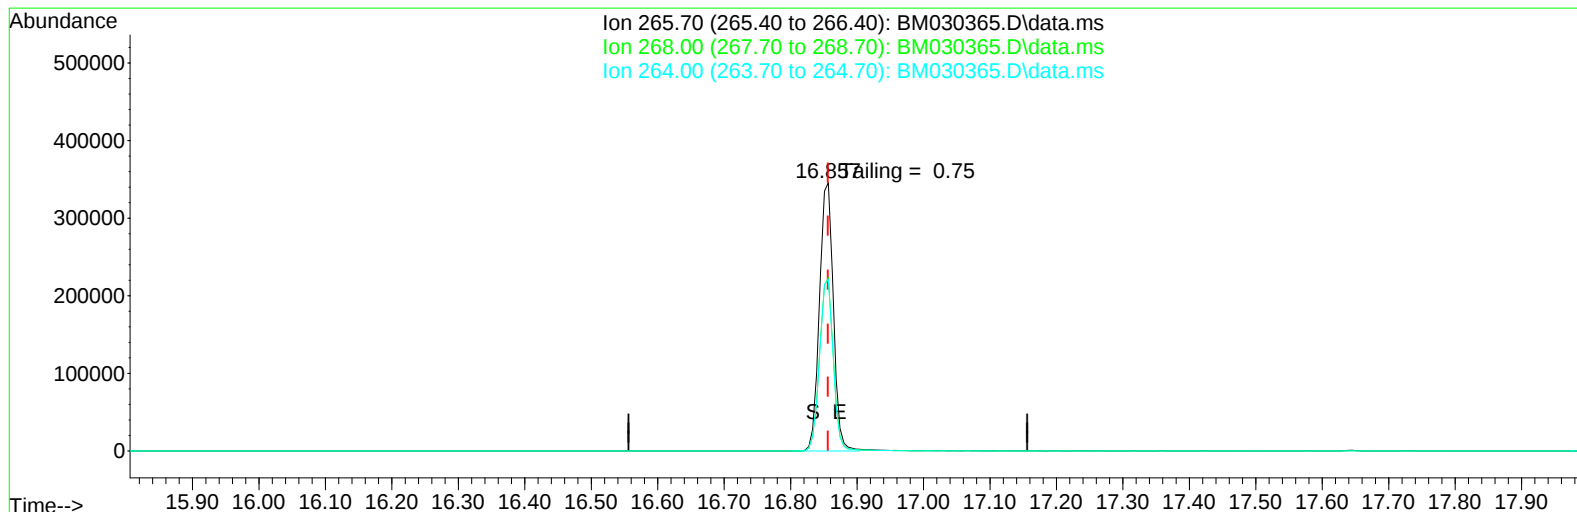

TIC: BM030365.D\data.ms

(70) Pentachlorophenol (C)

16.857min (+ 0.001) 850138.18 ng

response 506267

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.00	64.60
264.00	64.90	63.92
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/10/2021	BNA_M	<u>BM030365.D</u>
Compound Name	Response	Retention Time
DDT	1566694	20.66
DDD	15086	20.22
DDE	2026	19.72
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17112	1583806	1.08

Instrument :
BNA_M
ClientSampleId :
DFTPP