


Benzoic acid

Response Ratio

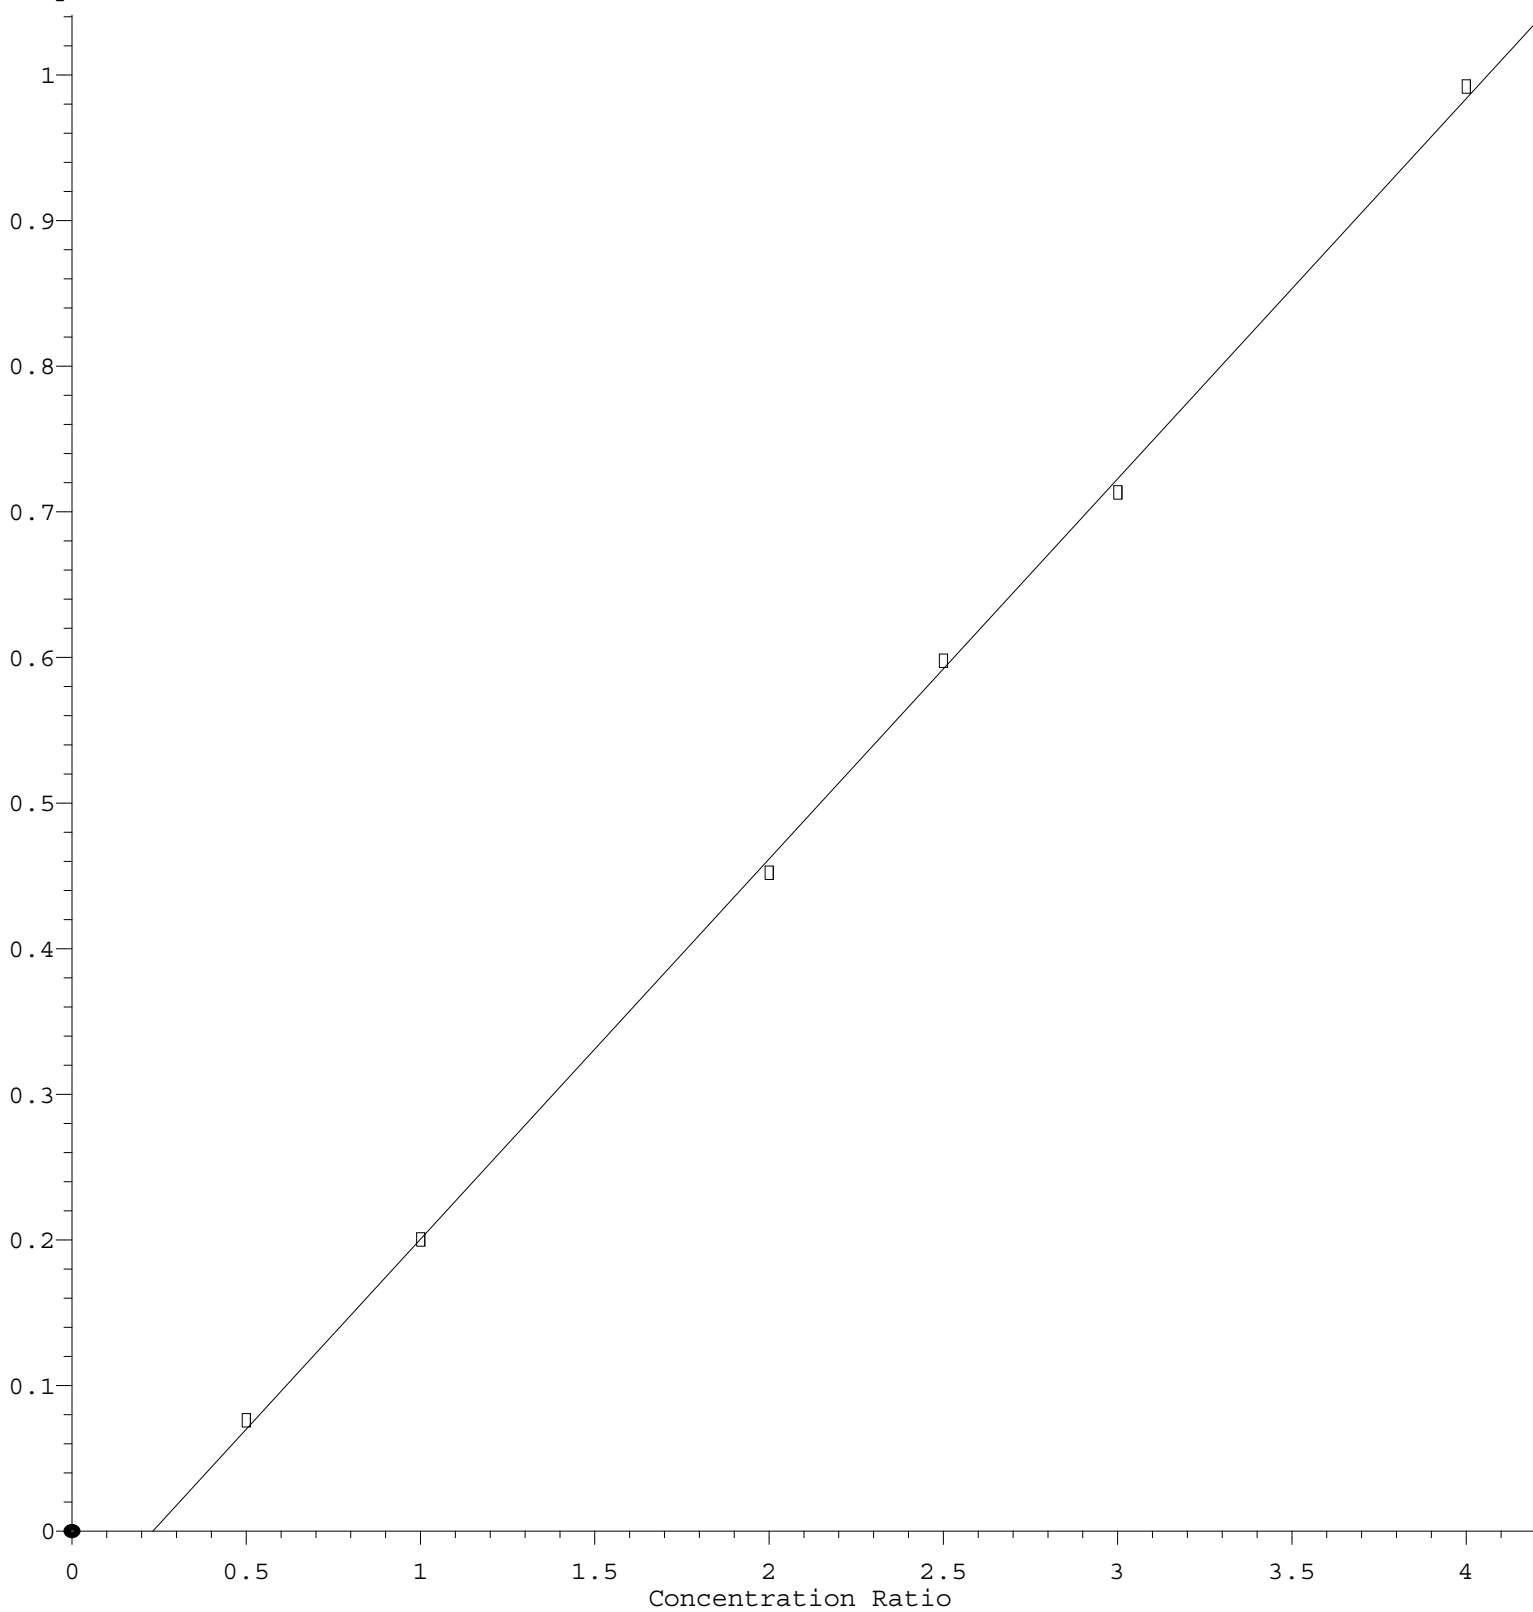

$$\text{Response} = 2.612\text{e-}001 * \text{Amt} - 6.062\text{e-}002$$


Coef of Det (r^2) = 0.999446 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA M\Methods\8270-BM061022.M

Calibration Table Last Updated: Fri Jun 10 16:05:33 2022

Hexachlorocyclopentadiene

Response Ratio

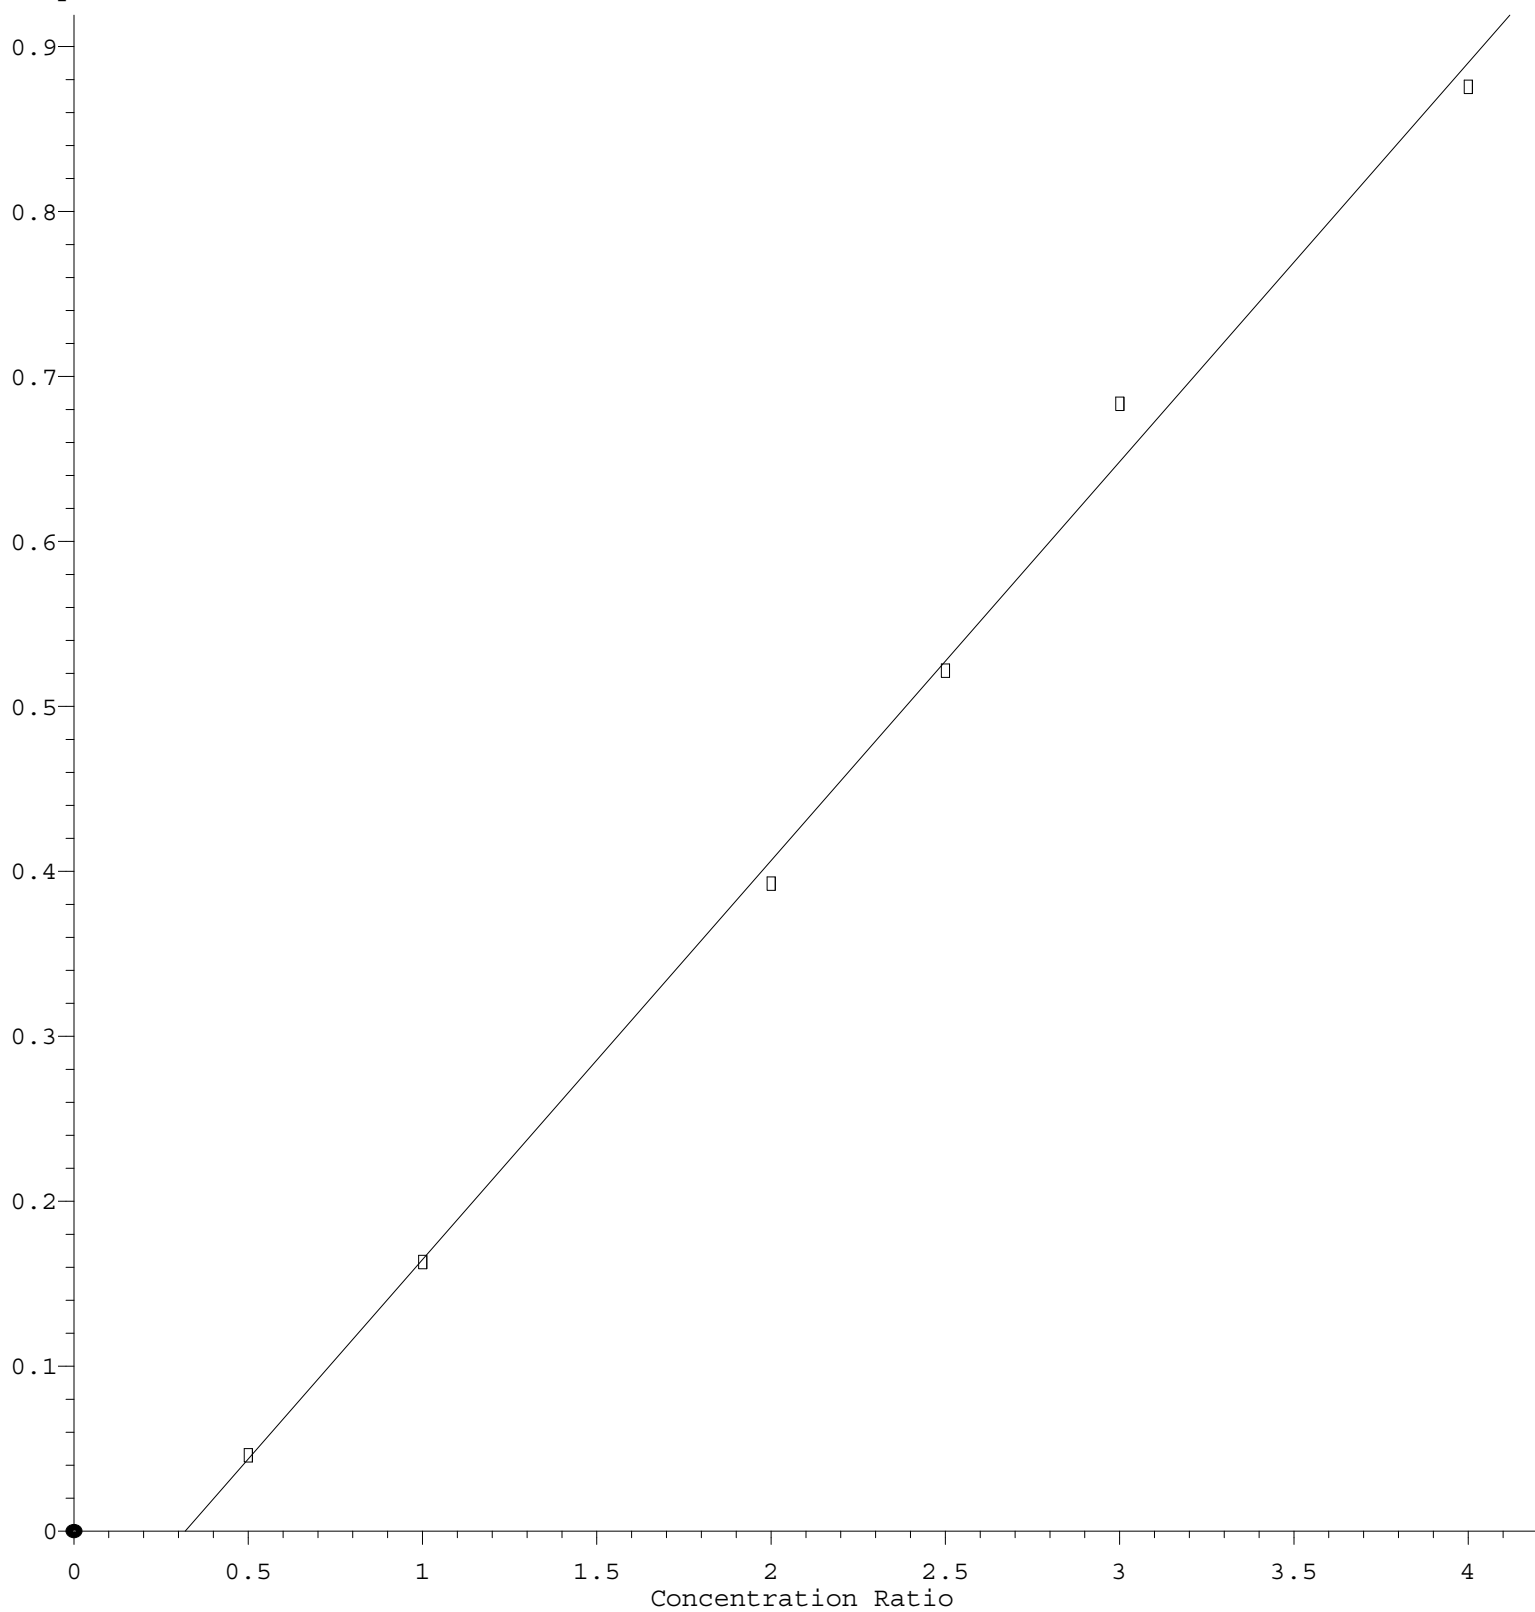


$$\text{Response} = 2.420\text{e-}001 * \text{Amt} - 7.720\text{e-}002$$

Coef of Det (r^2) = 0.996573 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA M\Methods\8270-BM061022.M

Calibration Table Last Updated: Fri Jun 10 16:05:33 2022


2,4-Dinitrophenol

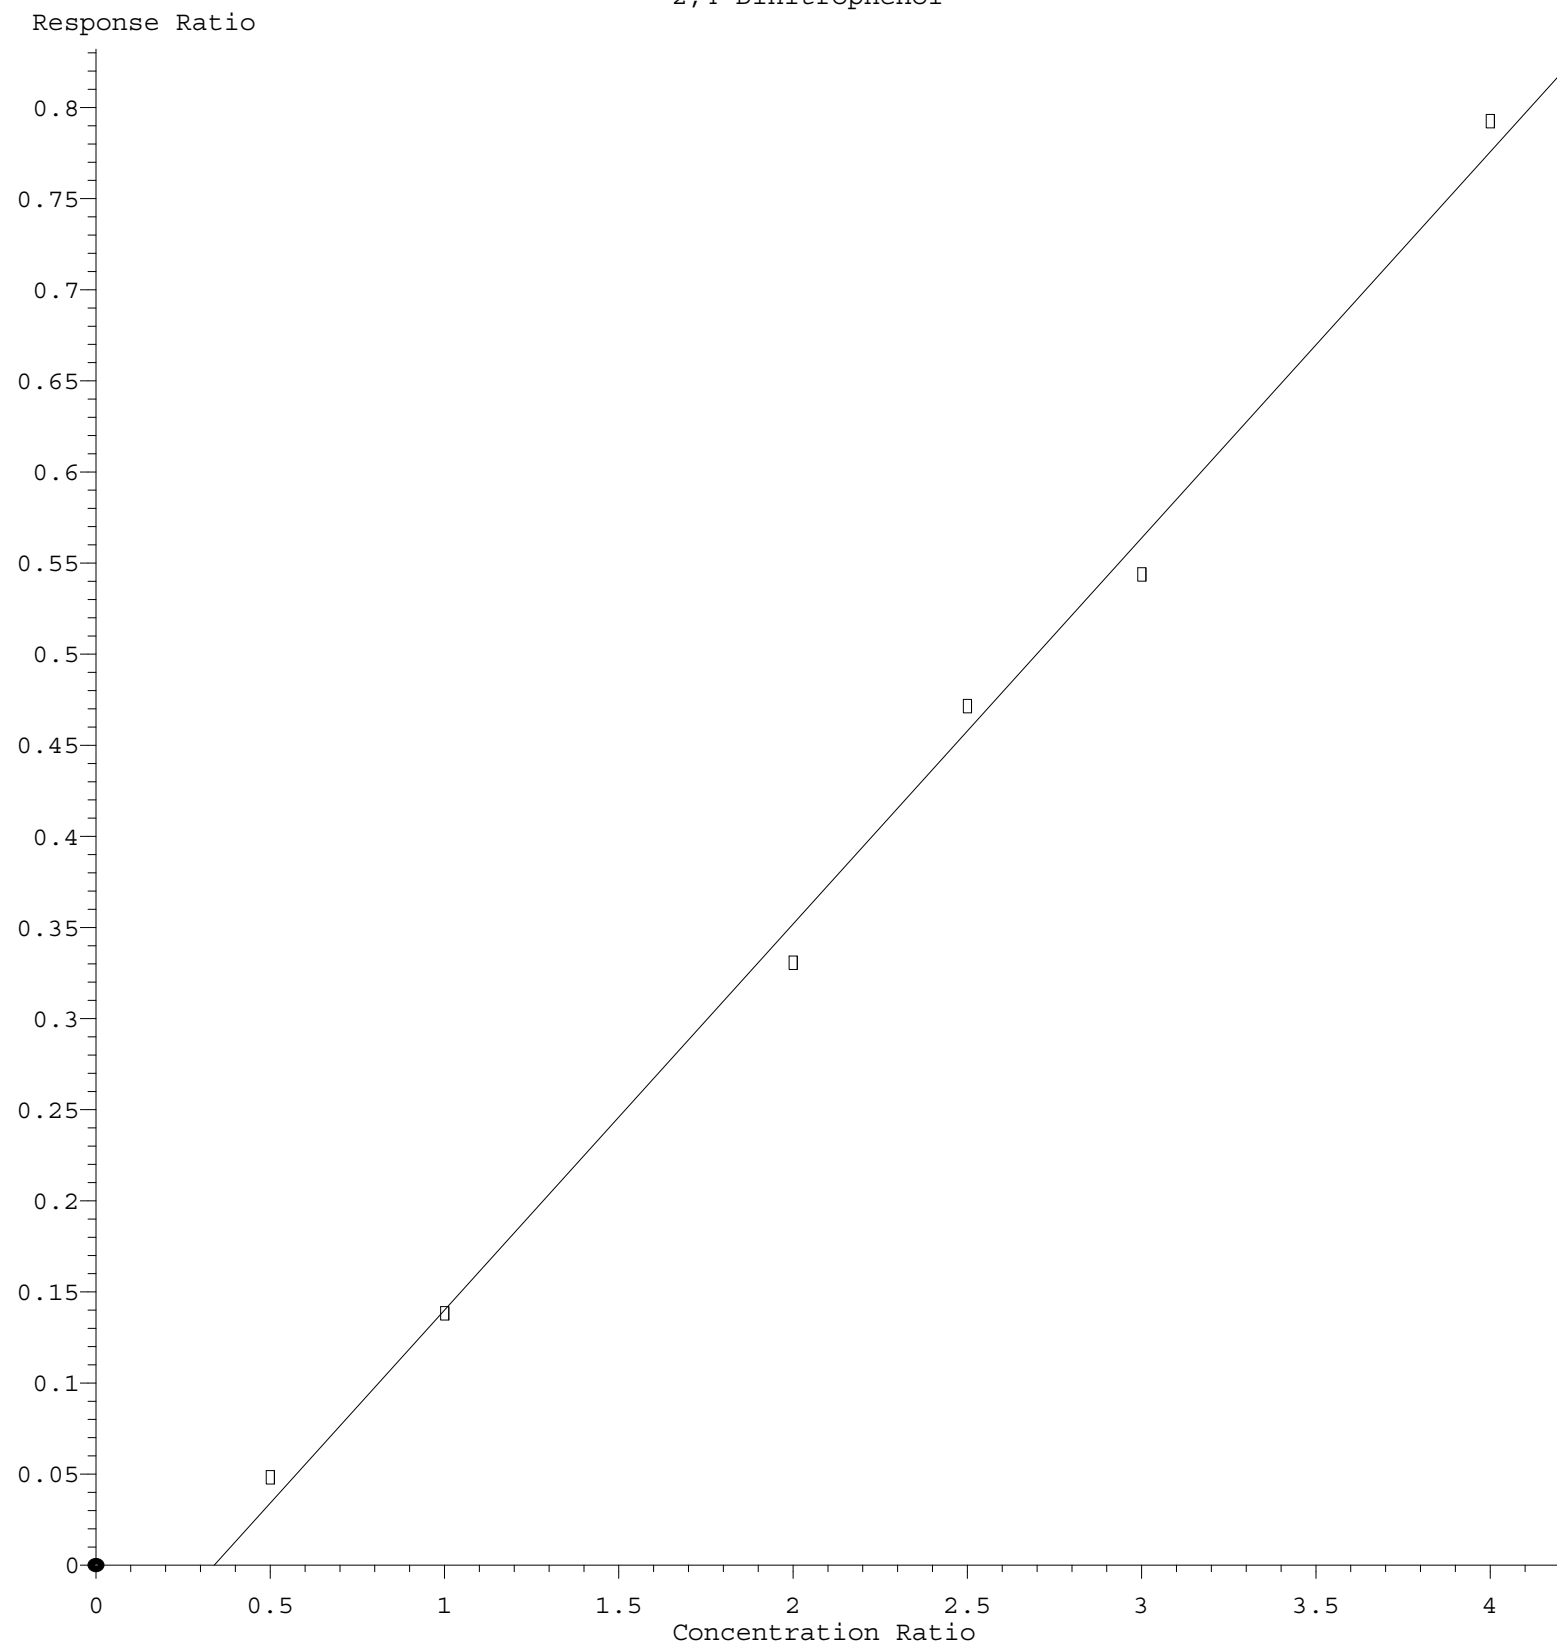

Response = $2.120 \times 10^{-1} \times \text{Amt} - 7.185 \times 10^{-2}$
Coef of Det (r^2) = 0.995936 Curve Fit: Linear
Method Name: Z:\svoasrv\HPCHEM1\BNA M\Methods\8270-BM061022.M
Calibration Table Last Updated: Fri Jun 10 16:05:33 2022

4-Nitrophenol

Response Ratio

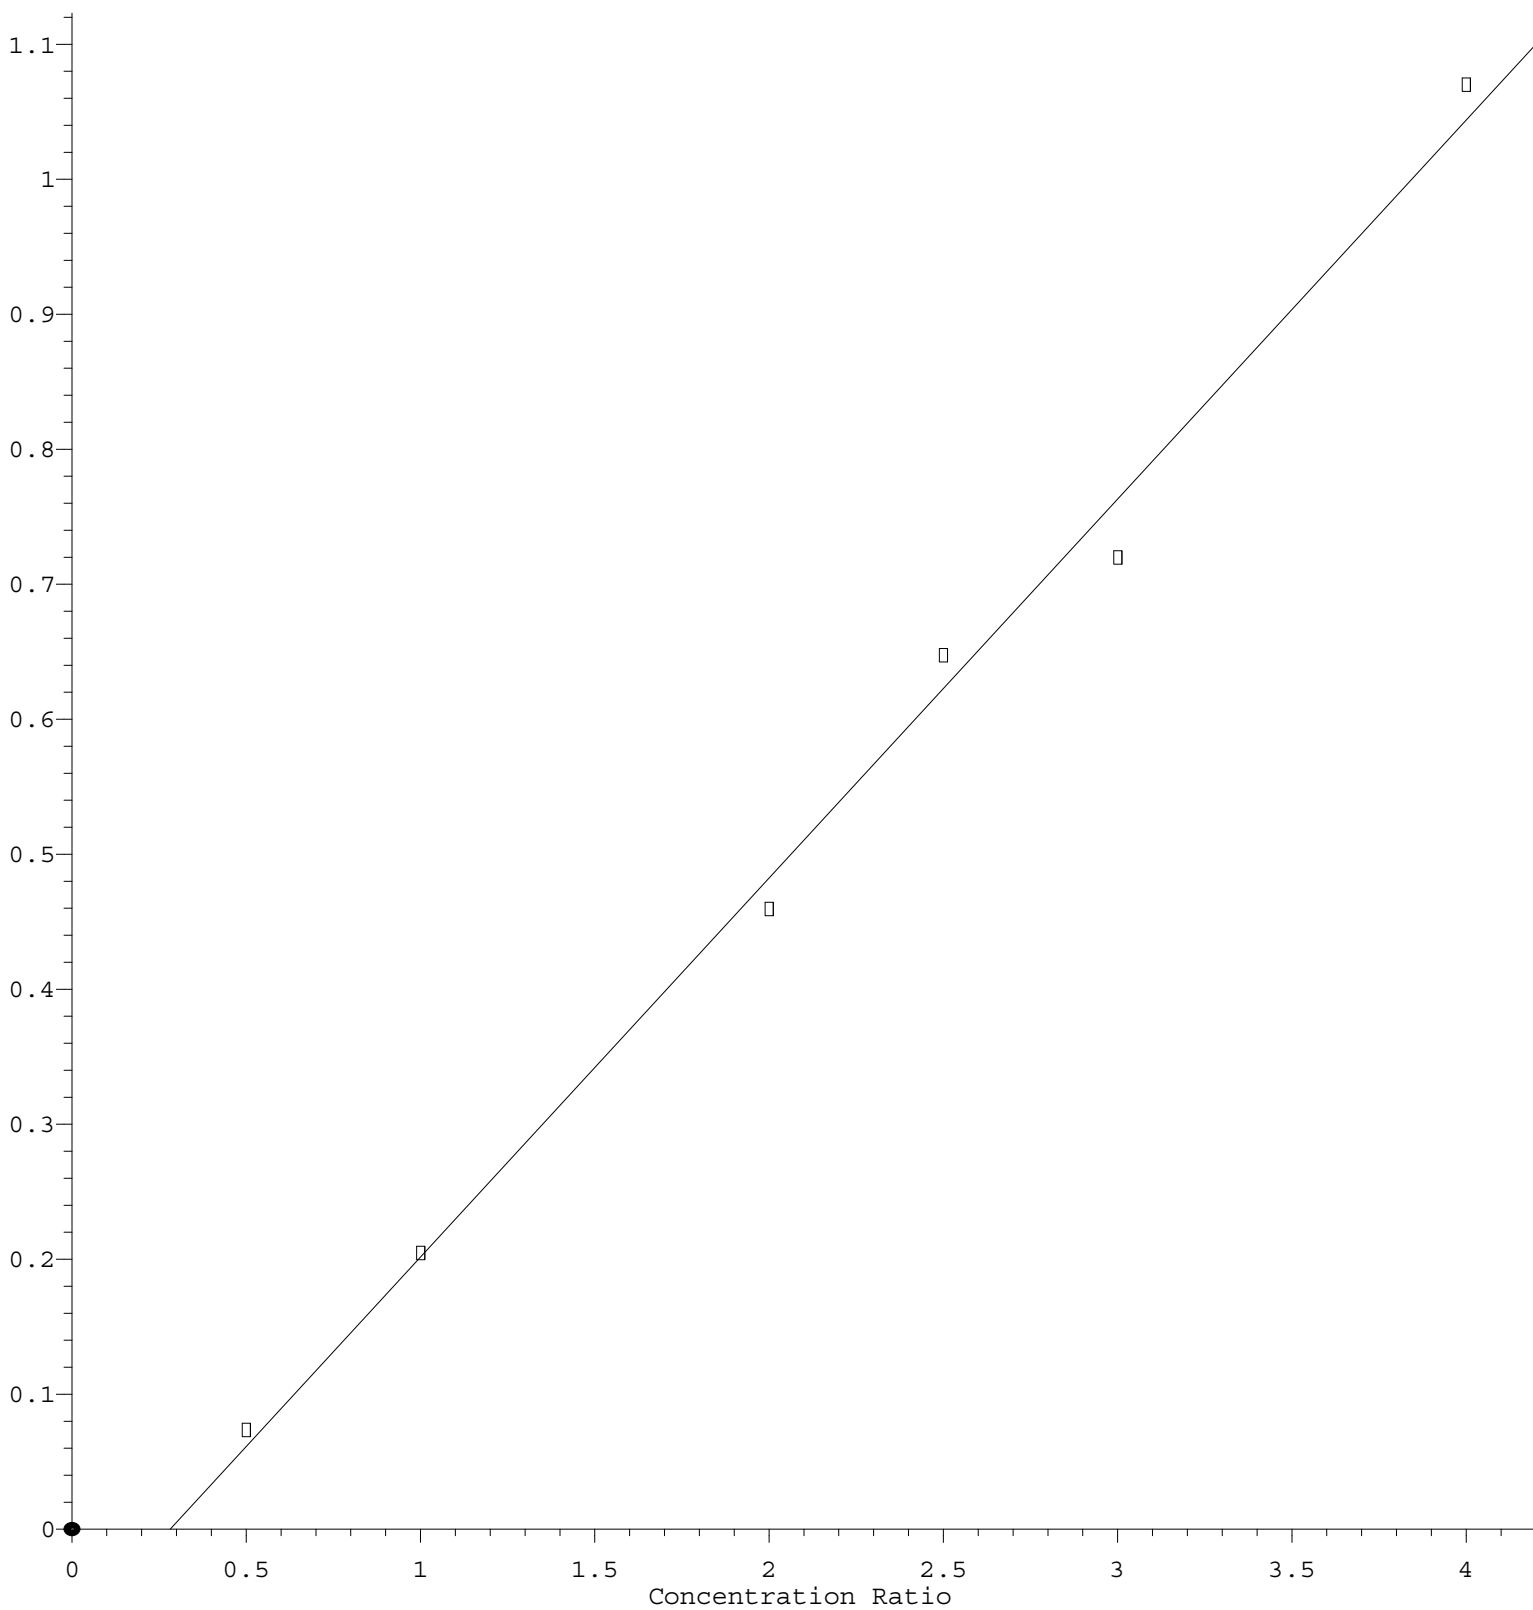

$$\text{Response} = 2.808\text{e-}001 * \text{Amt} - 7.921\text{e-}002$$

Coef of Det (r^2) = 0.994158 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA M\Methods\8270-BM061022.M

Calibration Table Last Updated: Fri Jun 10 16:05:33 2022