
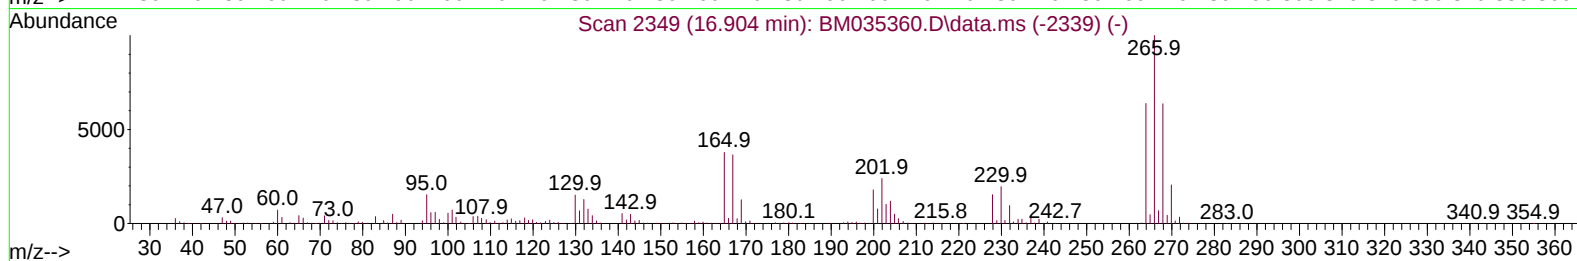
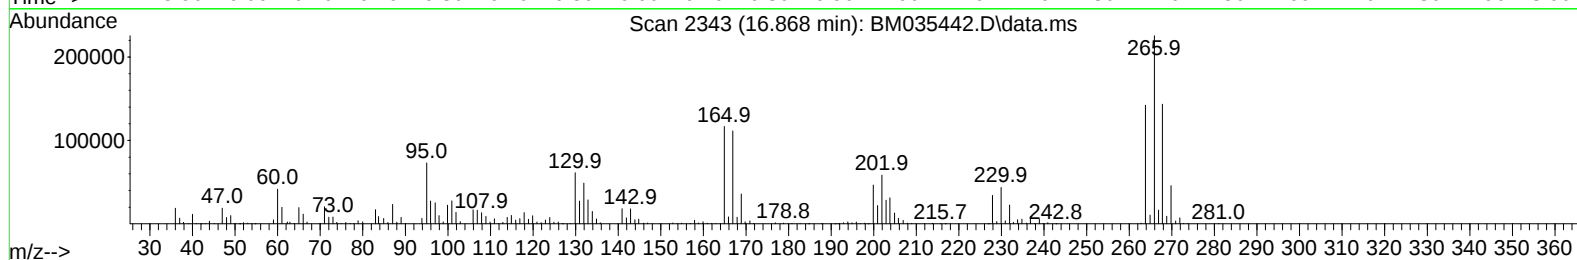


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061022\
 Data File : BM035442.D
 Acq On : 10 Jun 2022 10:49
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 10 13:18:26 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 10 13:12:23 2022
 Response via : Initial Calibration

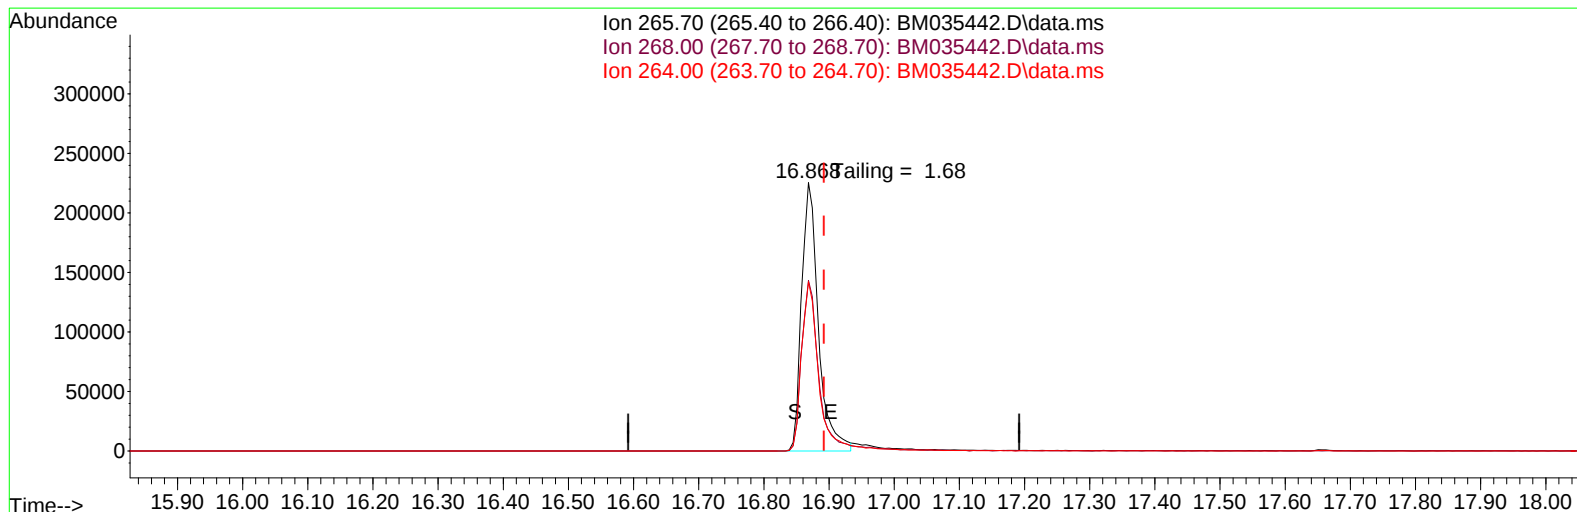

TIC: BM035442.D\data.ms

(70) Pentachlorophenol (C)




16.868min (-0.024) 0.00 ng

response 423589

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	63.58
264.00	63.30	63.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061022\
Data File : BM035442.D
Acq On : 10 Jun 2022 10:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 10 13:18:26 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 10 13:12:23 2022
Response via : Initial Calibration

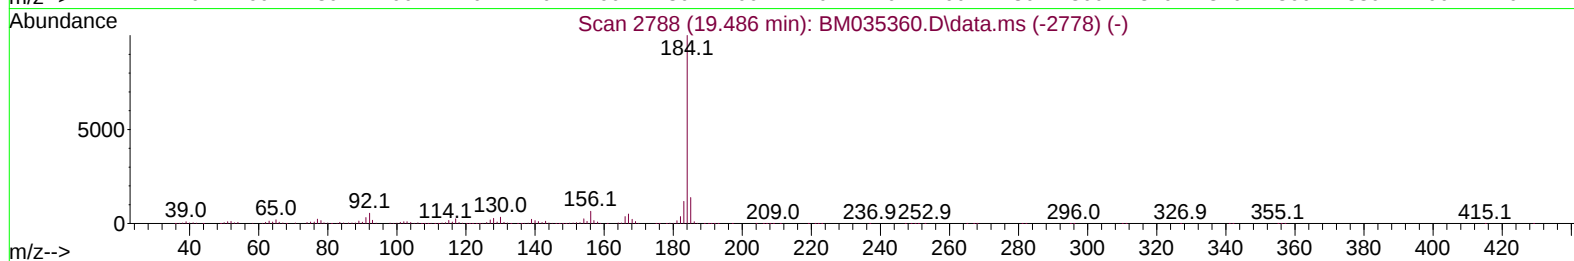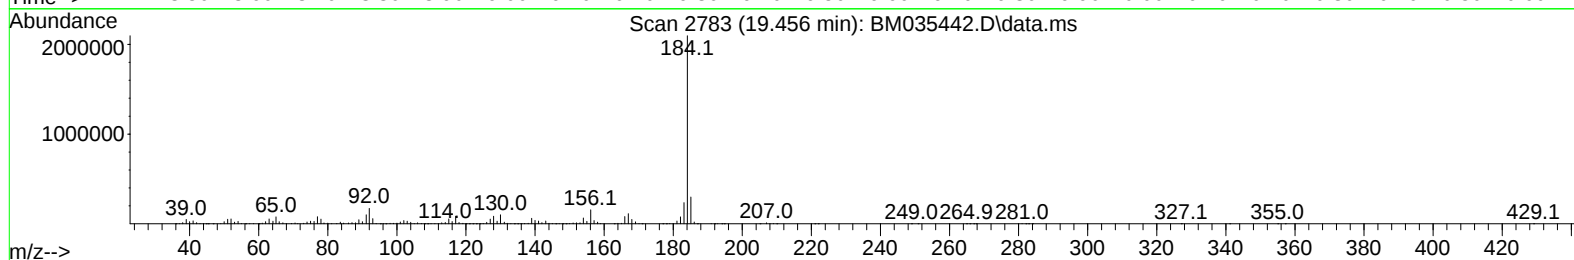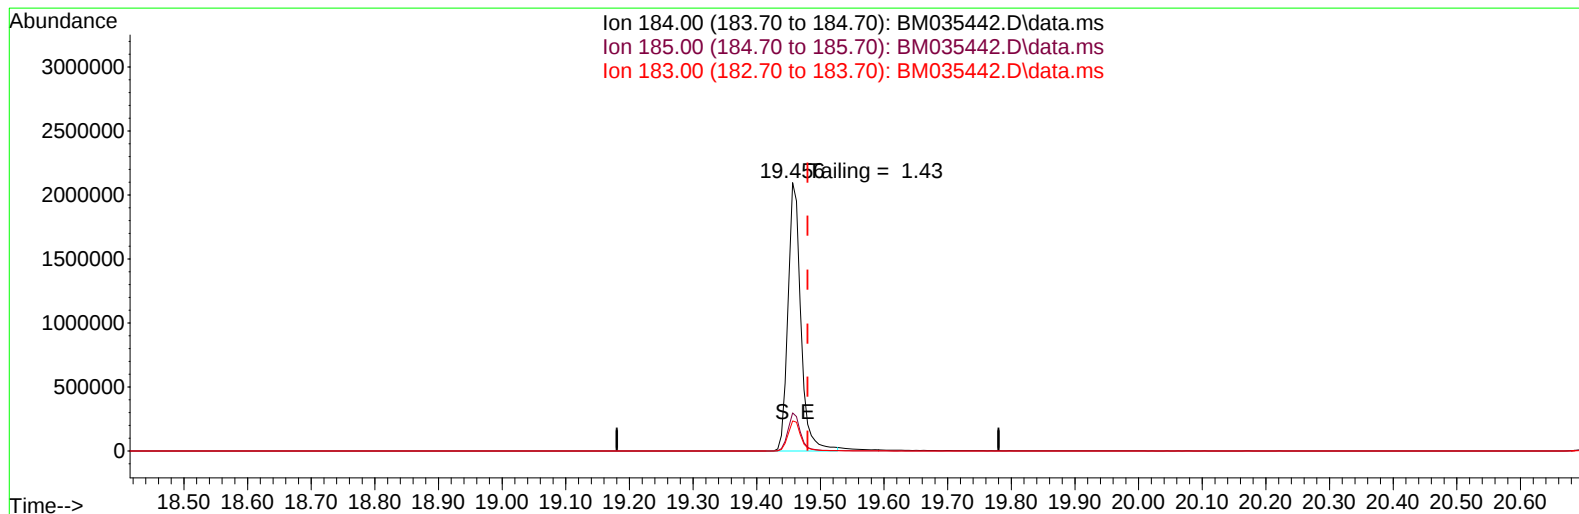

TIC: BM035442.D\data.ms

(77) Benzidine

19.456min (-0.024) 0.00 ng

response 3022270

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.20
183.00	11.90	11.20
0.00	0.00	0.00