

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061022\
 Data File : BM035451.D
 Acq On : 10 Jun 2022 16:18
 Operator : CG/JU
 Sample : PB145400TB
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB145400TB

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061022.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035451.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.404	388	394	413	rBV	5582050	8749797	51.19%	10.734%
2	7.004	659	666	697	rBV	5468774	9173001	53.67%	11.253%
3	7.822	798	805	820	rBV	1037963	1754487	10.27%	2.152%
4	8.981	995	1002	1015	rBV	3188956	5741050	33.59%	7.043%
5	10.622	1273	1281	1307	rBV	1272522	2549503	14.92%	3.128%
6	13.086	1693	1700	1723	rBV	8893535	13203296	77.25%	16.198%
7	14.463	1928	1934	1950	rBV	2134955	3364181	19.68%	4.127%
8	15.957	2181	2188	2212	rBV	5842540	9170527	53.65%	11.250%
9	17.210	2395	2401	2419	rBV	2507923	3857484	22.57%	4.732%
10	19.839	2842	2848	2861	rBV	13811140	17091753	100.00%	20.968%
11	21.398	3108	3113	3126	rBV	2650189	3721206	21.77%	4.565%
12	23.744	3505	3512	3528	rVB2	1424941	3137198	18.36%	3.849%




Sum of corrected areas: 81513483

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061022\
Data File : BM035451.D
Acq On : 10 Jun 2022 16:18
Operator : CG/JU
Sample : PB145400TB
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145400TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

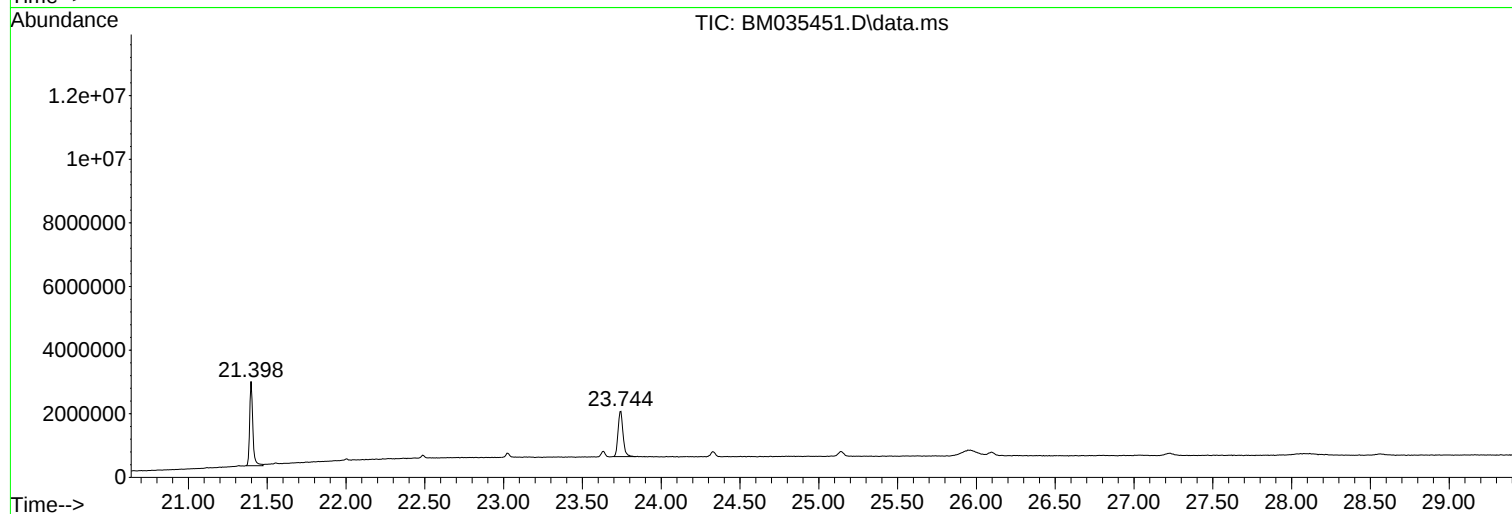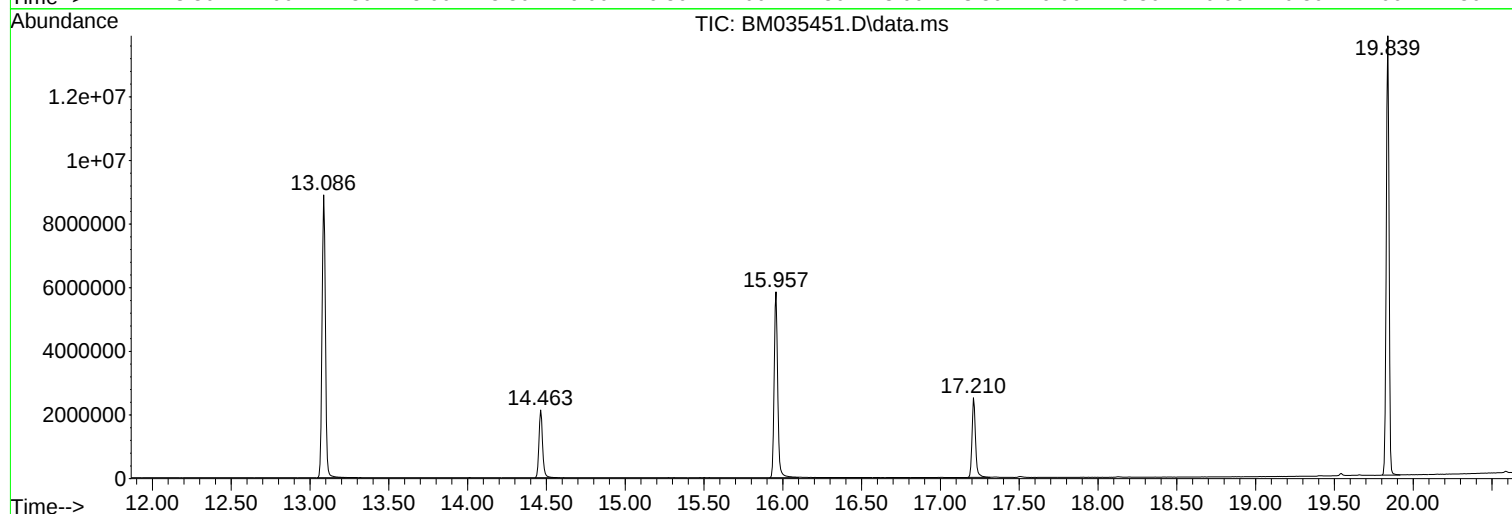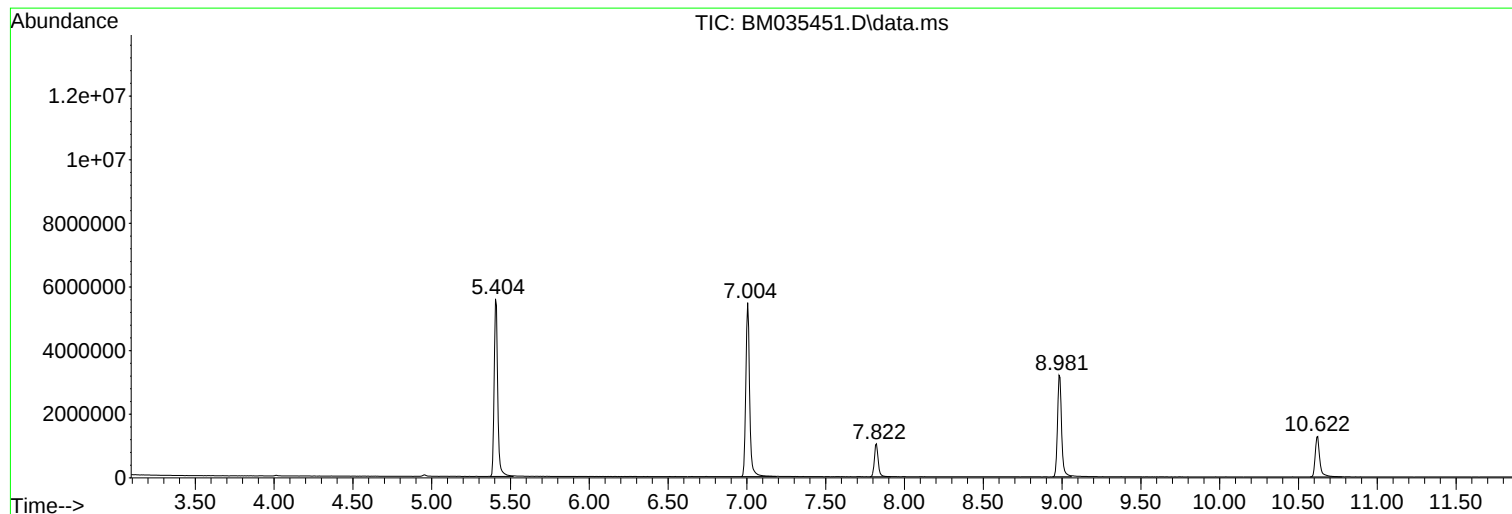

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061022\
Data File : BM035451.D
Acq On : 10 Jun 2022 16:18
Operator : CG/JU
Sample : PB145400TB
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145400TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061022\
Data File : BM035451.D
Acq On : 10 Jun 2022 16:18
Operator : CG/JU
Sample : PB145400TB
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145400TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------