


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061022\
Data File : BM035442.D
Acq On : 10 Jun 2022 10:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061022.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jun 10 16:05:33 2022

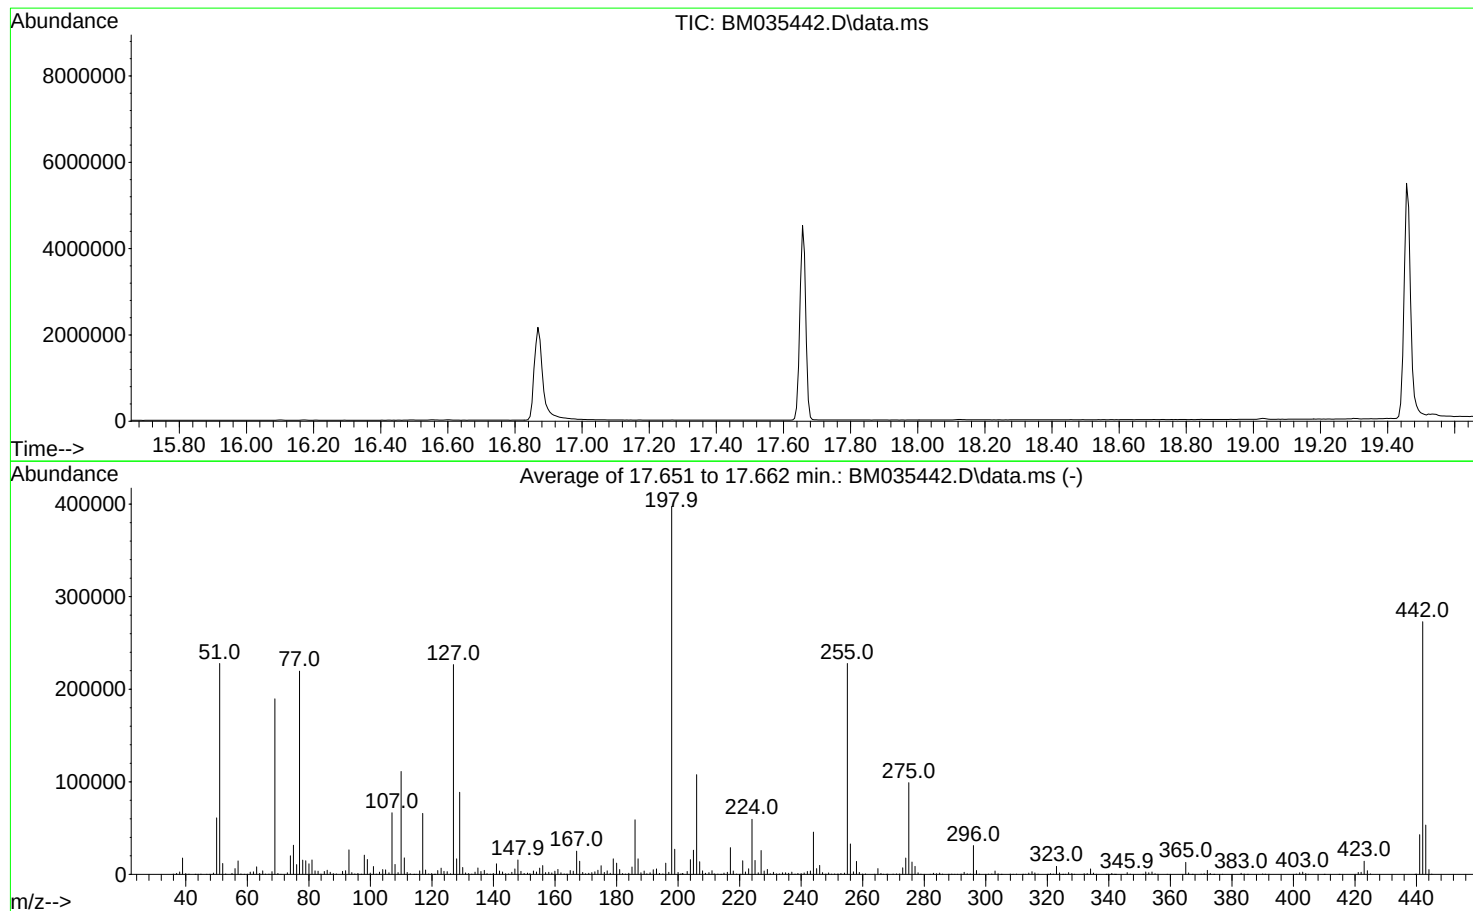




AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.3	227906	PASS
68	69	0.00	2	1.5	2889	PASS
69	198	0.00	100	47.7	189642	PASS
70	69	0.00	2	0.5	1041	PASS
127	198	10	80	57.0	226688	PASS
197	198	0.00	2	0.6	2304	PASS
198	198	100	100	100.0	397397	PASS
199	198	5	9	6.8	27112	PASS
275	198	10	60	24.9	99048	PASS
365	198	1	100	3.3	12978	PASS
441	198	0.01	100	10.8	42827	PASS
442	442	50	100	100.0	272939	PASS
443	442	15	24	19.5	53229	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061022\
 Data File : BM035442.D
 Acq On : 10 Jun 2022 10:49
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Jun 10 13:18:26 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 10 13:12:23 2022
 Response via : Initial Calibration

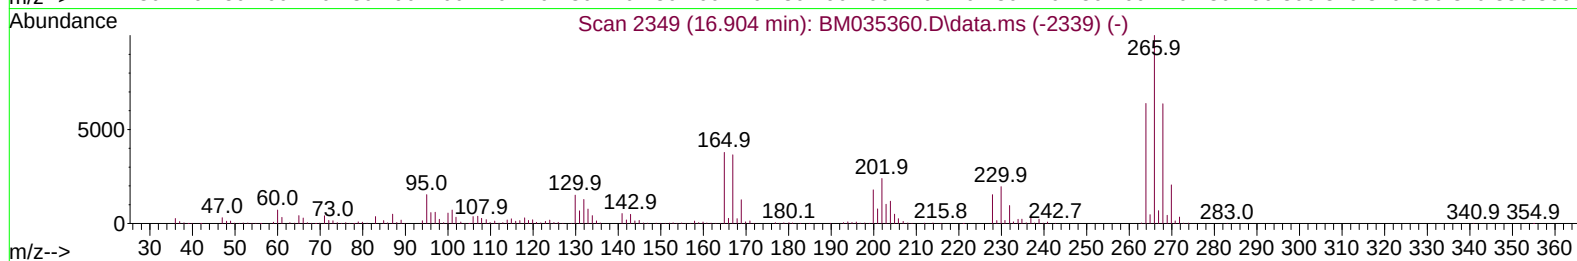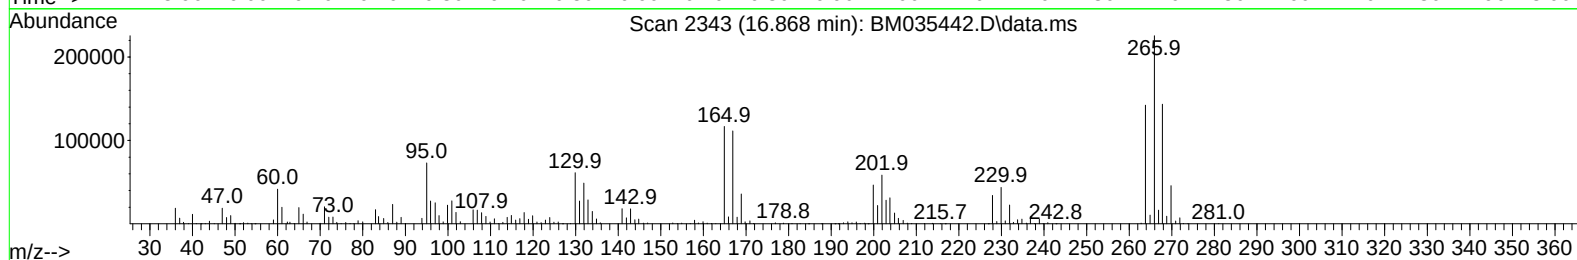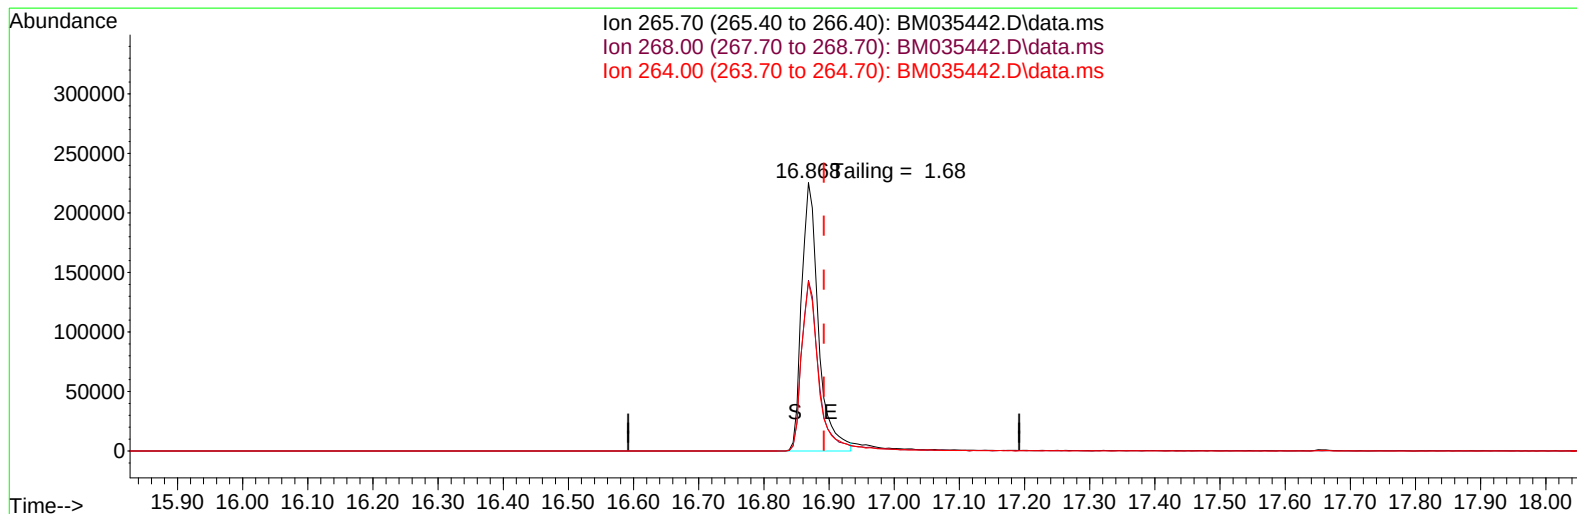

TIC: BM035442.D\data.ms

(70) Pentachlorophenol (C)

16.868min (-0.024) 0.00 ng




response 423589

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	63.58
264.00	63.30	63.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061022\
 Data File : BM035442.D
 Acq On : 10 Jun 2022 10:49
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Jun 10 13:18:26 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 10 13:12:23 2022
 Response via : Initial Calibration

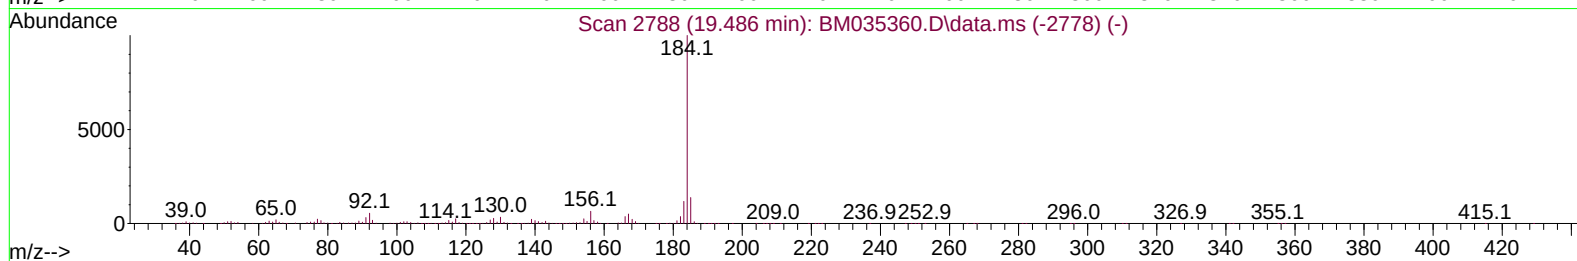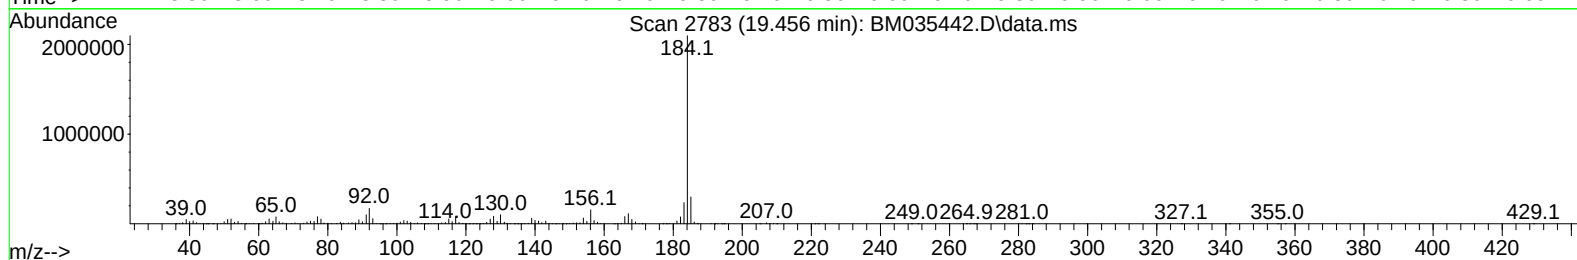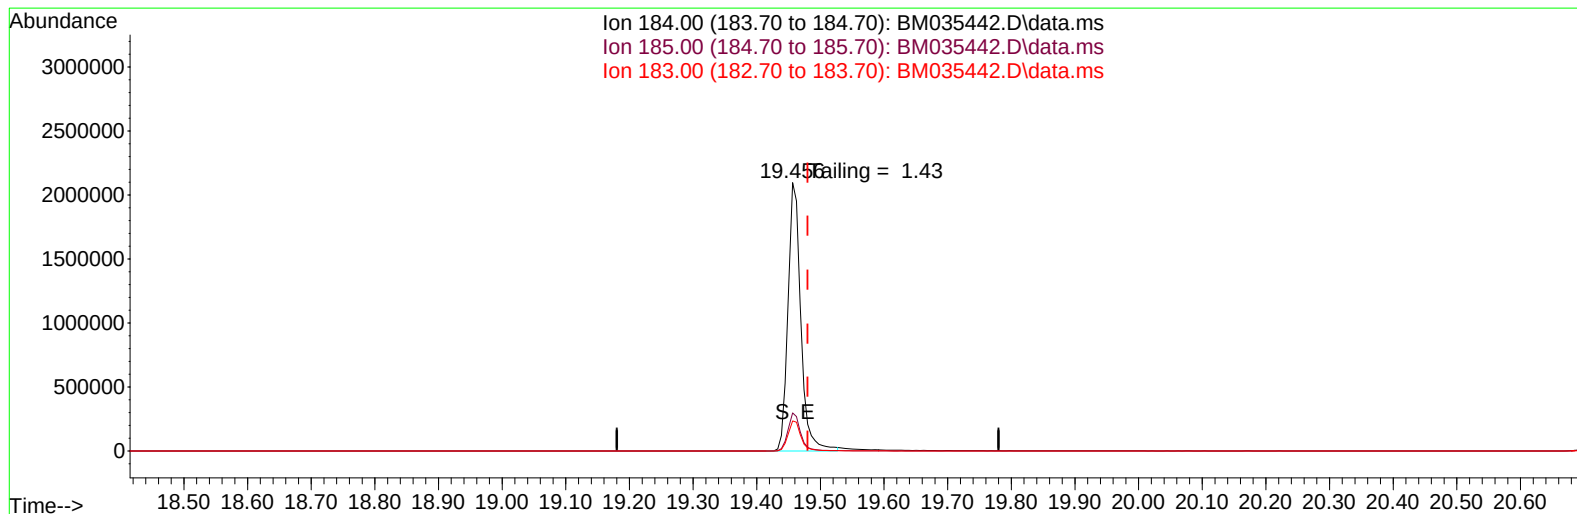

TIC: BM035442.D\data.ms

(77) Benzidine

19.456min (-0.024) 0.00 ng

response 3022270

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.20
183.00	11.90	11.20
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/10/2022	BNA_M	<u>BM035442.D</u>
Compound Name	Response	Retention Time
DDT	1883071	20.69
DDD	10125	20.25
DDE	5535	19.75
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15660	1898731	0.82

Instrument :
BNA_M
ClientSampleId :
DFTPP