


Data Path : S:\HPCHEM1\BNA_M\DATA\BM061115\
 Data File : BM001635.D
 Acq On : 10 Jun 2015 19:43
 Operator : TP/IZ
 Sample : DFTPP57
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP57

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-SIM-BM061115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 11 07:52:35 2015

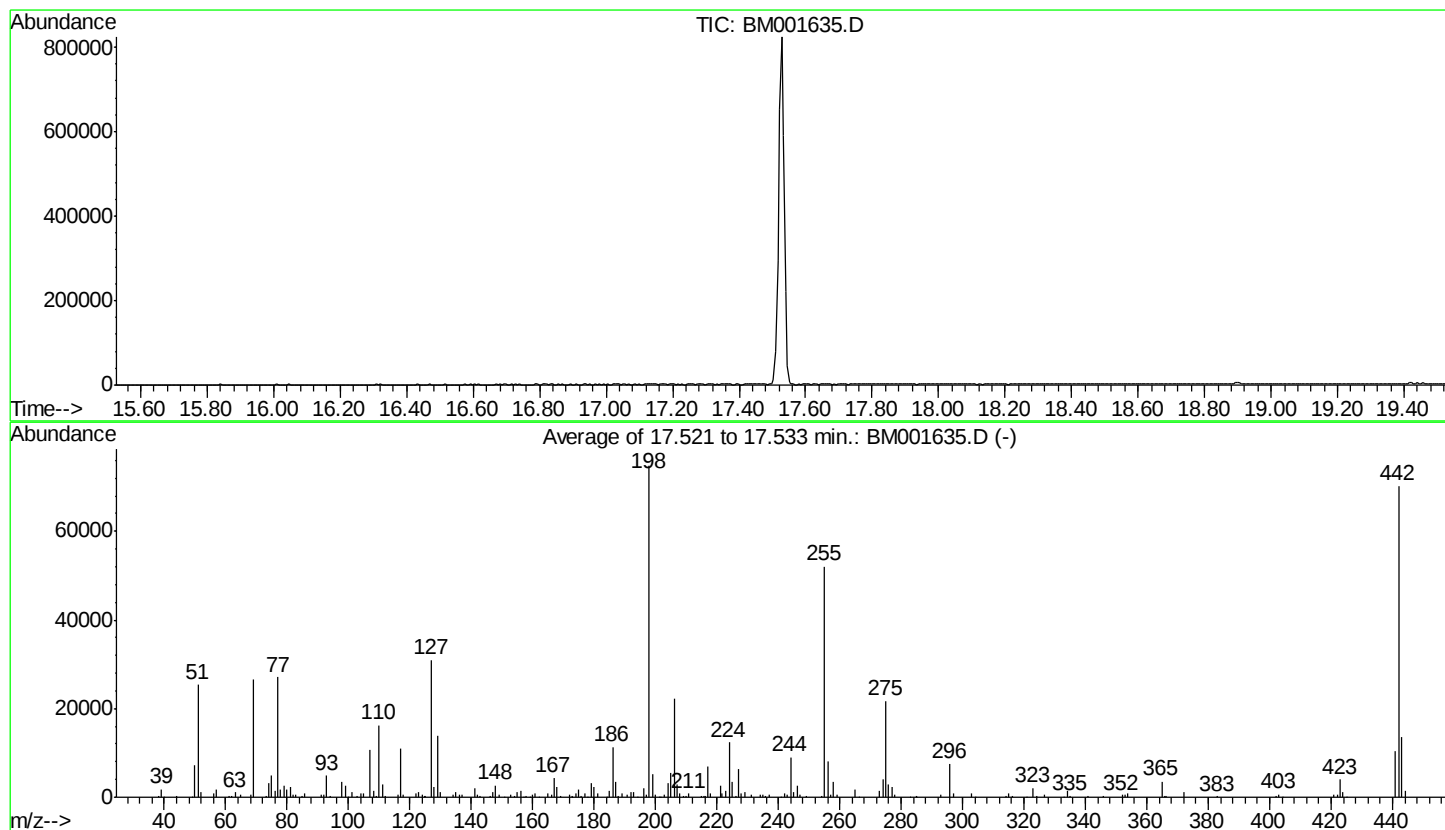

AutoFind: Scans 2522, 2523, 2524; Background Corrected with Scan 2516

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.9	25402	PASS
68	69	0.00	2	2.0	522	PASS
69	198	0.00	100	35.5	26581	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.4	30960	PASS
197	198	0.00	1	0.7	490	PASS
198	198	100	100	100.0	74840	PASS
199	198	5	9	7.0	5239	PASS
275	198	10	60	29.0	21730	PASS
365	198	1	100	4.7	3522	PASS
441	443	0.01	100	76.7	10402	PASS
442	198	50	100	93.9	70277	PASS
443	442	15	24	19.3	13561	PASS

m/z	Abundance
38.00	302.0
39.10	1912.0
39.90	368.0
44.00	871.0
50.10	7781.0
51.10	28472.0
52.10	1242.0
55.90	737.0
57.00	1871.0
61.00	372.0
62.00	481.0
63.10	1159.0
65.00	589.0
68.00	585.0
69.00	28528.0
73.00	453.0
74.10	3349.0
75.00	5413.0
76.00	1757.0
77.10	28376.0
78.00	2120.0
79.00	2554.0
80.00	1968.0
81.00	2449.0
82.00	676.0
82.90	578.0
84.90	431.0
85.90	970.0
91.00	708.0
92.00	902.0
93.00	5238.0
93.90	327.0
98.00	3812.0
99.00	2934.0
100.00	314.0
100.90	1161.0
102.90	473.0
103.90	916.0
105.00	1019.0
107.00	10865.0
108.00	1543.0
109.00	415.0
110.00	16456.0
111.00	3146.0
111.90	301.0
116.00	590.0
117.00	11215.0
117.90	640.0
122.00	807.0
123.00	1326.0
124.00	430.0
124.80	477.0
127.00	31176.0
128.00	2463.0
129.00	13514.0
130.00	1298.0
133.90	321.0
134.90	1084.0
135.90	550.0
137.00	542.0
141.00	2160.0
142.00	595.0
143.00	417.0
145.90	396.0
147.00	1151.0
148.00	2787.0
149.00	542.0
153.00	664.0
154.00	360.0
154.90	1065.0
156.00	1446.0
158.00	389.0
159.90	677.0
160.90	1002.0
162.00	339.0
165.00	737.0
166.00	551.0
167.00	3998.0
168.00	2581.0
168.90	418.0
171.90	509.0
172.80	444.0
174.00	947.0
175.00	1597.0
176.10	347.0
176.90	1004.0
179.00	3097.0
180.00	2548.0
181.00	1019.0
185.00	1309.0
186.00	10749.0

Instrument :
BNA_M
ClientSampleId :
DFTPP57

187.00	3576.0
189.00	717.0
191.00	463.0
192.00	1199.0
193.00	1422.0
196.00	1919.0
197.00	541.0
198.00	71928.0
199.00	5367.0
200.10	406.0
203.10	525.0
204.00	2895.0
205.00	5231.0
206.00	20304.0
207.00	3086.0
207.90	1047.0
209.00	383.0
211.00	691.0
215.90	490.0
217.00	6597.0
217.90	826.0
221.00	1905.0
221.80	746.0
223.00	1420.0
224.00	11487.0
225.00	3032.0
227.00	6374.0
227.90	757.0
229.00	1311.0
231.00	550.0
234.00	432.0
235.00	397.0
235.90	358.0
237.00	802.0
241.90	628.0
243.00	743.0
244.10	8118.0
245.00	1121.0
246.00	2223.0
247.00	592.0
249.00	395.0
254.10	335.0
255.00	47576.0
256.00	7671.0
257.00	501.0
258.00	2944.0
259.00	386.0
265.00	1470.0
273.00	1303.0
274.00	3446.0
275.00	18968.0
276.00	2401.0
277.00	1992.0
277.90	321.0
284.90	385.0
293.00	551.0
296.00	6543.0
296.90	991.0
303.00	869.0
315.00	793.0
316.10	368.0
323.00	1677.0
323.90	329.0
326.90	436.0
334.00	1398.0
335.00	301.0
345.90	548.0
352.00	540.0
353.00	622.0
353.90	603.0
365.00	2646.0
365.90	376.0
372.10	840.0
403.10	617.0
420.90	441.0
422.00	444.0
423.10	3174.0
424.00	809.0
425.00	329.0
441.00	8085.0
442.10	52704.0
443.10	10290.0
444.10	990.0

Instrument :
BNA_M
ClientSampleId :
DFTPP57

m/z	Abundance
38.00	355.0
39.00	1918.0
40.00	635.0
43.90	938.0
49.10	373.0
50.10	8510.0
51.10	29504.0
52.00	1352.0
56.00	788.0
57.00	1743.0
61.10	339.0
61.90	508.0
63.00	1423.0
65.00	542.0
68.10	616.0
69.00	31640.0
73.10	547.0
74.00	3785.0
75.00	5395.0
76.10	1888.0
77.10	32632.0
78.00	2164.0
79.00	3274.0
80.00	2100.0
81.00	3073.0
82.00	723.0
82.90	529.0
85.00	447.0
85.90	846.0
90.90	581.0
91.80	715.0
93.00	5894.0
93.90	398.0
98.00	4099.0
99.00	3321.0
101.00	1352.0
103.00	612.0
104.00	964.0
105.00	970.0
107.00	13472.0
108.00	1693.0
109.00	430.0
110.00	19120.0
111.00	3245.0
112.00	485.0
116.10	712.0
117.00	13068.0
118.00	992.0
122.00	1068.0
123.00	1341.0
124.00	599.0
125.00	499.0
127.00	37368.0
128.00	2775.0
129.00	17016.0
130.00	1424.0
133.90	629.0
135.00	1276.0
136.00	697.0
136.90	720.0
141.00	2221.0
142.00	991.0
143.00	439.0
146.00	426.0
147.00	1384.0
148.00	3106.0
149.00	559.0
150.90	384.0
153.00	723.0
153.90	456.0
155.00	1291.0
156.00	2110.0
157.10	422.0
158.00	378.0
158.90	345.0
160.00	733.0
161.00	881.0
165.00	1035.0
166.00	720.0
167.00	5727.0
168.00	2875.0
169.00	468.0
171.80	402.0
173.00	590.0
174.00	1281.0
175.00	1983.0
175.90	348.0
176.90	863.0
177.90	332.0
179.00	3715.0
180.00	2998.0

Instrument :
BNA_M
ClientSampleId :
DFTPP57

181.00	1097.0
185.00	1533.0
186.00	14063.0
187.00	3979.0
187.90	472.0
188.90	965.0
190.90	691.0
192.00	1340.0
193.00	1425.0
196.00	2333.0
197.00	510.0
197.90	89608.0
199.00	6387.0
200.00	585.0
201.20	349.0
203.00	817.0
204.00	3959.0
205.00	6290.0
206.10	26576.0
207.00	3874.0
208.00	914.0
209.00	371.0
209.90	369.0
211.00	1145.0
215.00	359.0
216.20	660.0
217.00	8330.0
218.00	927.0
221.00	2945.0
221.80	1134.0
222.90	1897.0
224.00	15188.0
225.00	4215.0
226.00	453.0
227.00	7375.0
227.90	1094.0
229.00	1498.0
231.00	656.0
233.90	615.0
235.00	687.0
236.00	393.0
237.00	737.0
240.80	303.0
242.00	833.0
243.00	750.0
244.00	11108.0
244.90	1238.0
246.00	3082.0
247.00	671.0
249.00	423.0
254.10	455.0
255.00	60960.0
256.00	9193.0
257.00	710.0
258.00	4183.0
259.10	644.0
265.00	1837.0
273.00	1671.0
274.00	5068.0
275.00	26456.0
276.00	3309.0
277.00	2673.0
278.00	641.0
284.90	436.0
293.00	742.0
296.00	9280.0
297.00	1034.0
303.00	984.0
304.00	331.0
314.00	383.0
315.00	1029.0
316.10	364.0
321.00	314.0
323.00	2732.0
324.00	609.0
326.90	476.0
333.00	377.0
334.00	1556.0
335.00	442.0
341.00	302.0
346.00	419.0
352.00	575.0
353.00	594.0
354.00	995.0
365.00	4333.0
366.10	537.0
372.10	1237.0
383.00	317.0
401.90	496.0
403.00	695.0
404.00	364.0
421.00	858.0
422.00	722.0
423.10	4406.0
424.00	1452.0

Instrument :
BNA_M
ClientSampleId :
DFTPP57

441.10	11949.0
442.10	83296.0
443.10	16640.0
444.00	1665.0

Instrument :
BNA_M
ClientSampleId :
DFTPP57

m/z	Abundance
39.00	1455.0
39.90	401.0
44.00	756.0
50.00	5462.0
51.00	18232.0
52.00	977.0
56.00	702.0
57.00	1267.0
63.10	524.0
65.00	543.0
67.90	366.0
69.00	19576.0
74.00	2258.0
75.00	3573.0
76.10	889.0
77.10	20392.0
78.00	1217.0
79.00	2017.0
79.90	1304.0
81.00	1878.0
82.00	401.0
83.00	348.0
85.90	729.0
91.00	496.0
92.00	498.0
93.00	3445.0
98.00	2500.0
99.00	1942.0
101.00	965.0
103.90	755.0
105.00	574.0
107.00	7537.0
108.10	1194.0
110.00	13288.0
111.00	2064.0
111.90	307.0
116.00	529.0
117.00	8665.0
118.00	518.0
122.00	720.0
122.90	904.0
123.90	478.0
125.00	364.0
127.00	24336.0
128.00	2075.0
129.00	10918.0
130.10	846.0
133.90	467.0
135.00	888.0
136.00	348.0
137.00	430.0
141.00	1563.0
142.00	526.0
143.00	364.0
146.00	427.0
146.90	754.0
148.00	2035.0
149.00	496.0
152.90	537.0
154.00	313.0
155.00	1045.0
156.10	1161.0
158.00	370.0
159.90	444.0
161.00	821.0
165.00	790.0
166.00	561.0
167.00	3416.0
168.00	1652.0
169.10	314.0
171.90	459.0
172.90	337.0
173.90	712.0
175.10	1451.0
175.90	378.0
177.00	597.0
179.00	2782.0
180.00	1732.0
181.00	838.0
184.00	443.0
185.00	1318.0
186.00	9239.0
187.00	2481.0
188.00	389.0
189.00	710.0
190.90	386.0
192.00	758.0
193.10	1063.0
194.10	324.0
196.00	1662.0
197.10	420.0

Instrument :
BNA_M
ClientSampleId :
DFTPP57

198.00	62984.0
198.90	3964.0
200.00	379.0
201.50	308.0
202.90	534.0
204.00	3023.0
205.00	5002.0
206.00	19856.0
207.00	2808.0
208.00	786.0
208.90	416.0
210.00	315.0
210.90	685.0
214.90	308.0
216.00	354.0
217.00	5841.0
218.00	693.0
221.00	2712.0
221.80	838.0
223.00	1182.0
224.00	10571.0
225.00	3094.0
226.00	331.0
227.00	5302.0
227.90	872.0
229.00	922.0
231.00	331.0
233.90	303.0
235.00	345.0
236.90	598.0
242.00	907.0
243.00	618.0
244.00	7836.0
244.90	1057.0
246.00	2251.0
246.90	478.0
255.00	47680.0
256.00	7322.0
257.00	477.0
258.00	3452.0
259.00	586.0
265.00	1857.0
266.00	329.0
273.00	1326.0
274.00	3579.0
275.00	19768.0
276.00	3014.0
277.00	1864.0
278.00	395.0
283.00	306.0
285.10	349.0
293.00	362.0
296.00	6952.0
296.90	871.0
303.00	752.0
314.00	305.0
314.90	642.0
316.00	504.0
323.10	1955.0
324.00	320.0
326.80	475.0
334.00	1575.0
335.00	351.0
341.00	360.0
346.00	349.0
352.00	561.0
353.00	354.0
354.00	696.0
365.00	3589.0
365.90	338.0
372.00	1157.0
383.00	452.0
402.00	431.0
403.00	707.0
421.00	636.0
422.00	468.0
423.00	4252.0
423.90	854.0
441.10	11173.0
442.10	74832.0
443.10	13755.0
444.10	1402.0

Instrument :
BNA_M
ClientSampleId :
DFTPP57

Scan 2516 (17.486 min): BM001635.D
DFTPP57

m/z	Abundance
39.90	374.0
44.00	694.0
207.10	488.0


Instrument :
BNA_M
ClientSampleId :
DFTPP57

Data Path : S:\HPCHEM1\BNA_M\DATA\BM061115\
 Data File : BM001635.D
 Acq On : 10 Jun 2015 19:43
 Operator : TP/IZ
 Sample : DFTPP57
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP57

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-SIM-BM061115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 11 07:52:35 2015

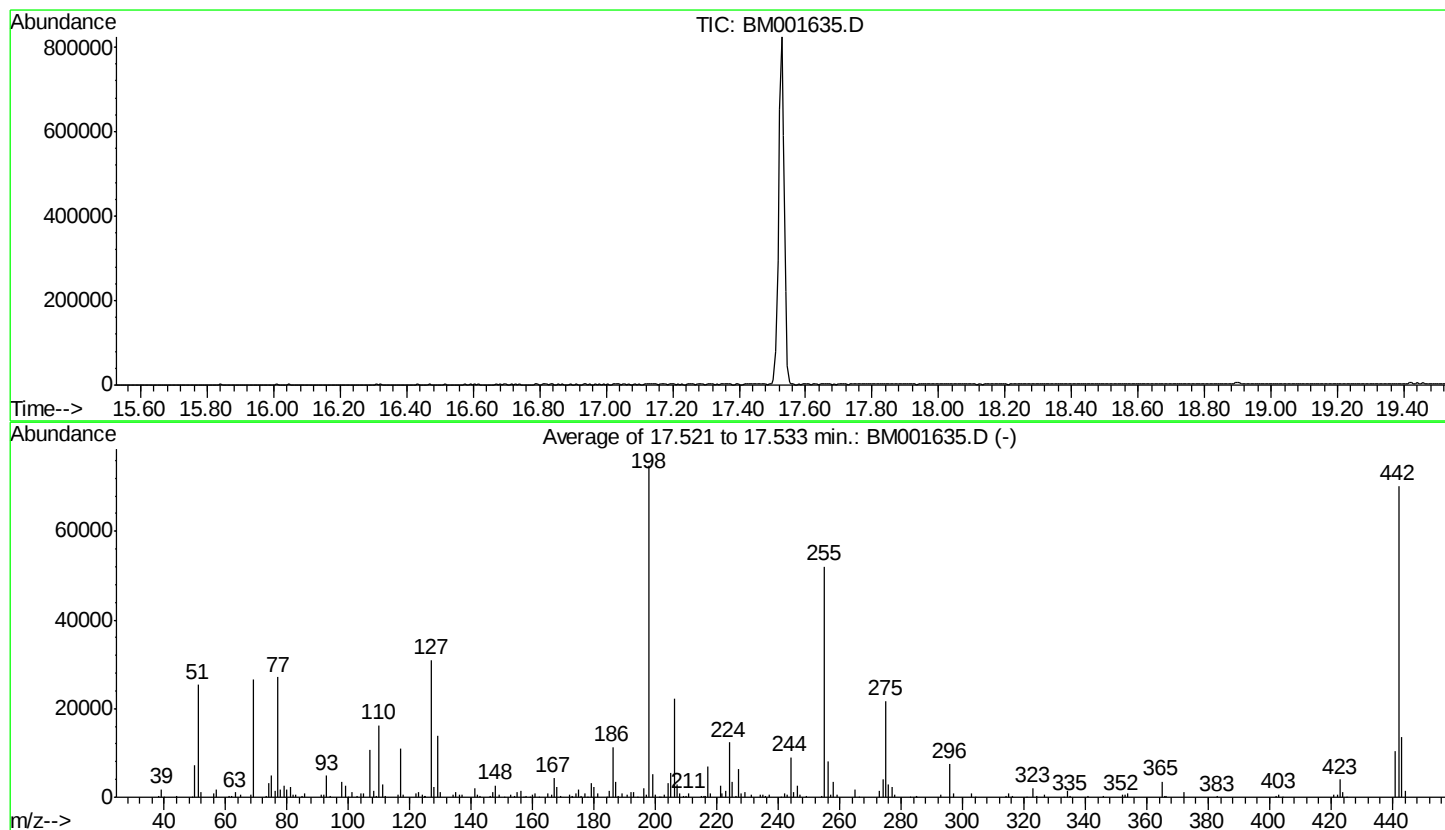

AutoFind: Scans 2522, 2523, 2524; Background Corrected with Scan 2516

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.9	25402	PASS
68	69	0.00	2	2.0	522	PASS
69	198	0.00	100	35.5	26581	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.4	30960	PASS
197	198	0.00	1	0.7	490	PASS
198	198	100	100	100.0	74840	PASS
199	198	5	9	7.0	5239	PASS
275	198	10	60	29.0	21730	PASS
365	198	1	100	4.7	3522	PASS
441	443	0.01	100	76.7	10402	PASS
442	198	50	100	93.9	70277	PASS
443	442	15	24	19.3	13561	PASS