
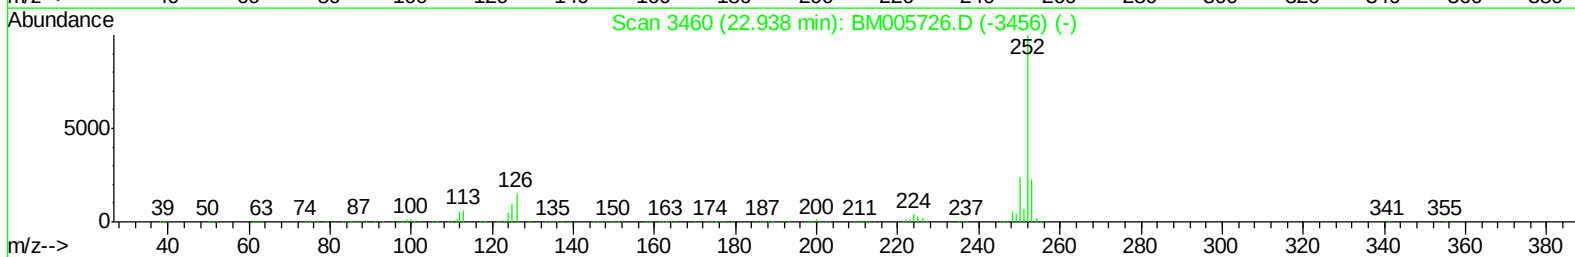
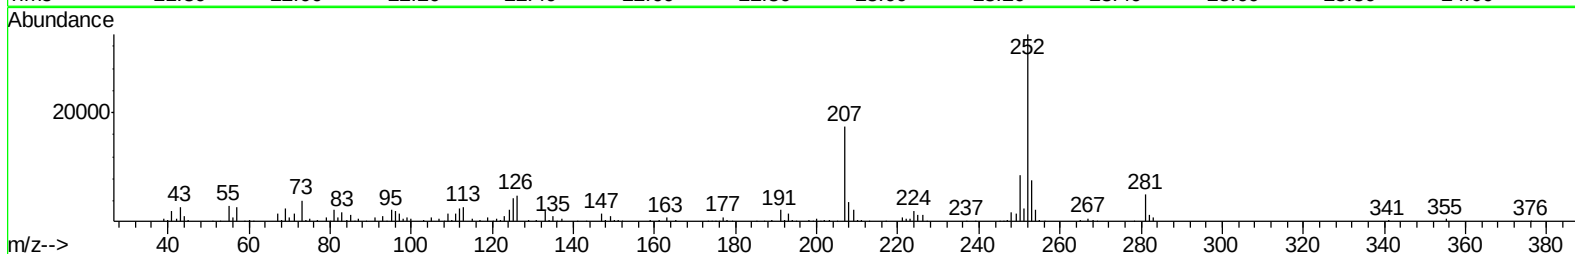


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061116\
Data File : BM005727.D
Acq On : 11 Jun 2016 15:19
Operator : UM/SJ
Sample : H3411-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Jun 11 23:25:58 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061016.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jun 11 23:08:56 2016
Response via : Initial Calibration

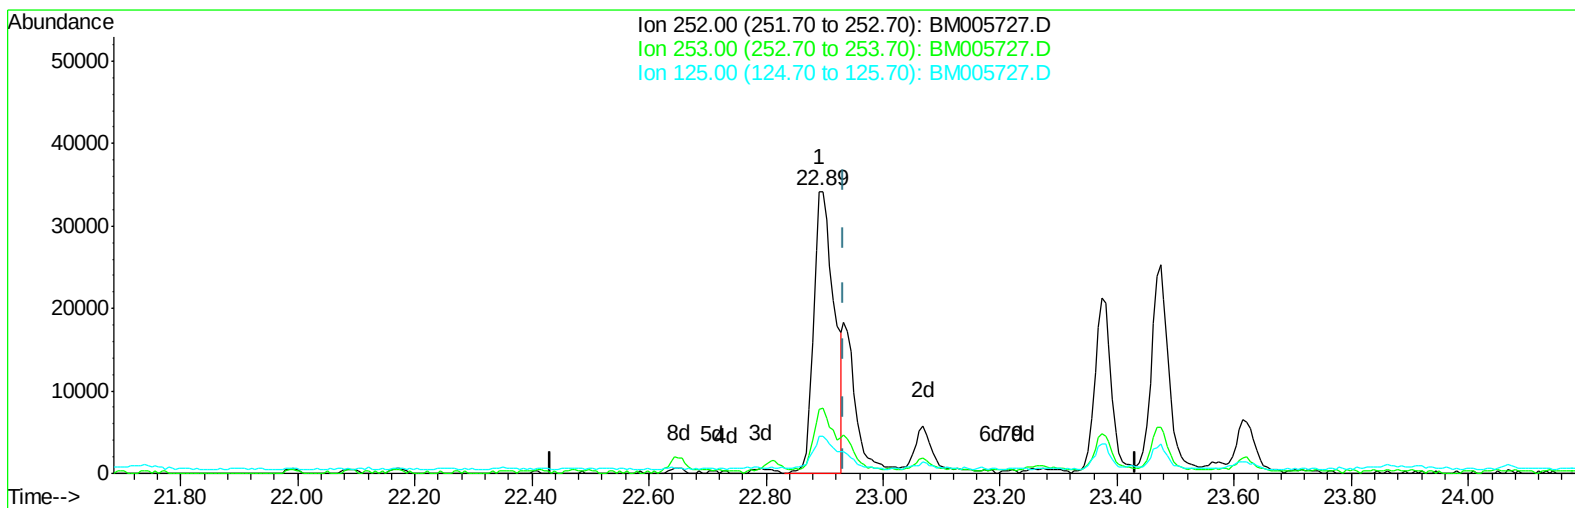

TIC: BM005727.D

(36) Benzo(k)fluoranthene

22.891min (-0.041) 2.44ng/ul

response 83091

Ion	Exp%	Act%
252.00	100	100
253.00	21.90	22.79
125.00	10.20	12.98#
0.00	0.00	0.00