
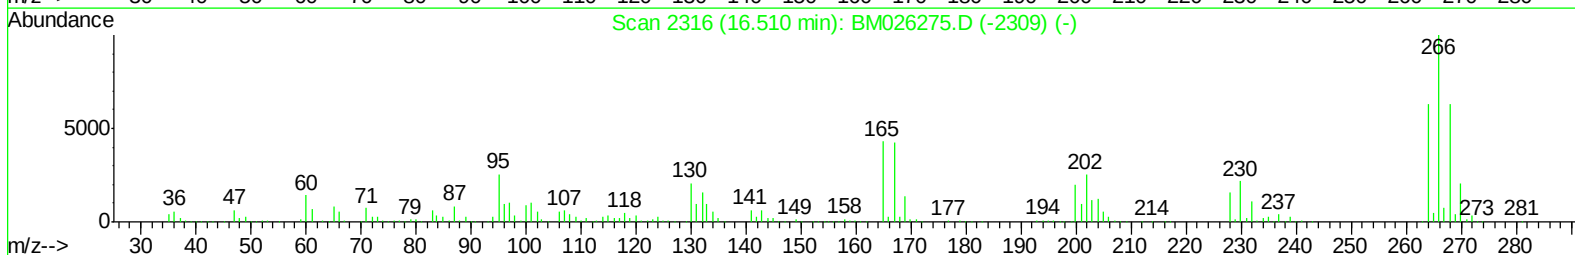
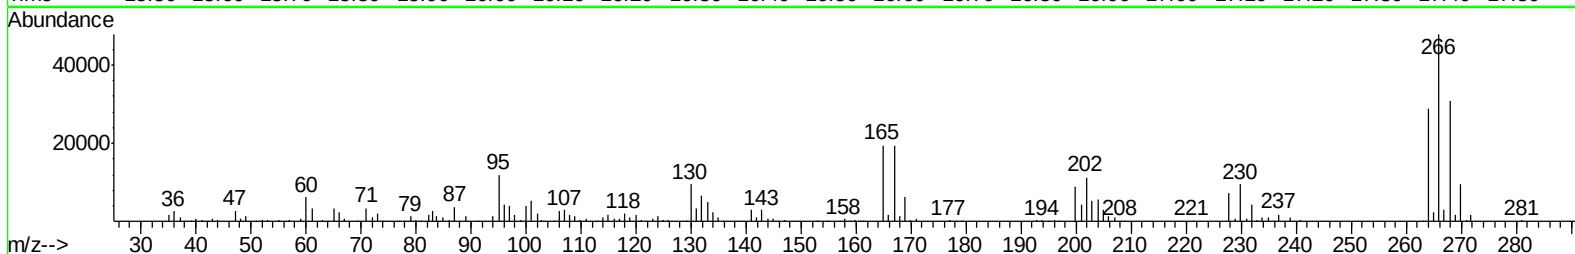


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061120\
Data File : BM026366.D
Acq On : 11 Jun 2020 23:04
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 12 00:31:42 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 09 14:46:47 2020
Response via : Initial Calibration

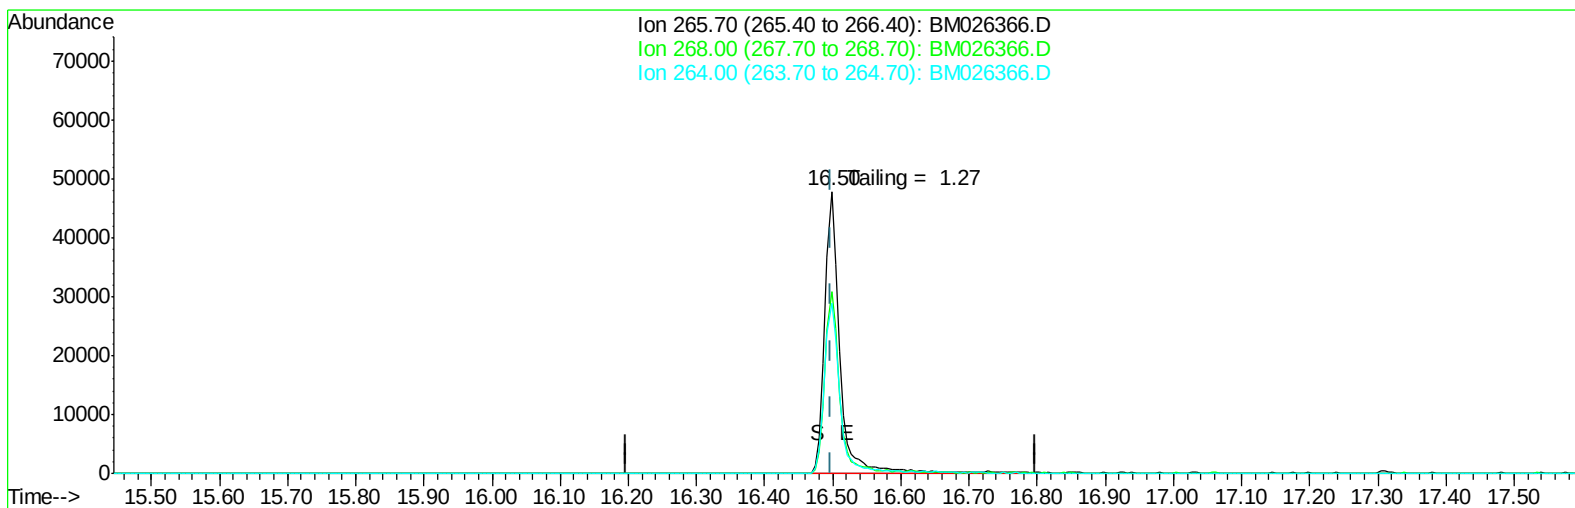

TIC: BM026366.D

(70) Pentachlorophenol (C)




16.498min (+0.000) 0.00ng

response 69848

Ion	Exp%	Act%
265.70	100	100
268.00	63.10	64.41
264.00	62.80	60.63
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061120\
 Data File : BM026366.D
 Acq On : 11 Jun 2020 23:04
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 12 00:31:42 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM060520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 09 14:46:47 2020
 Response via : Initial Calibration

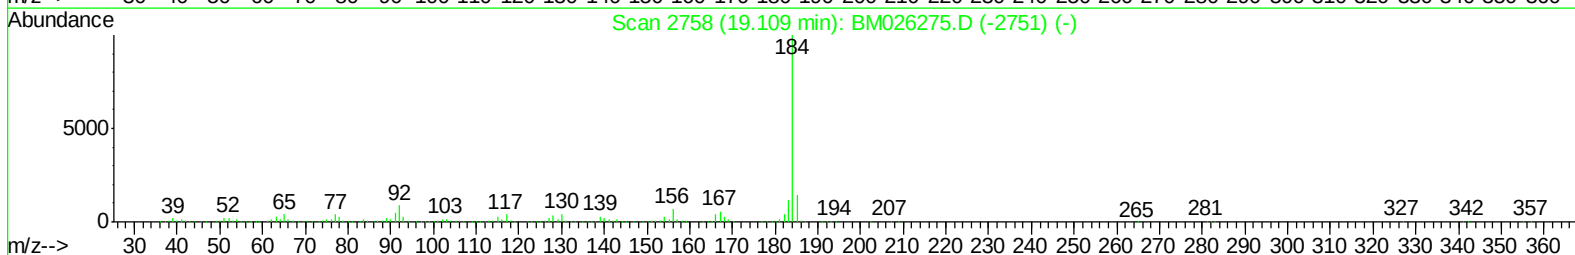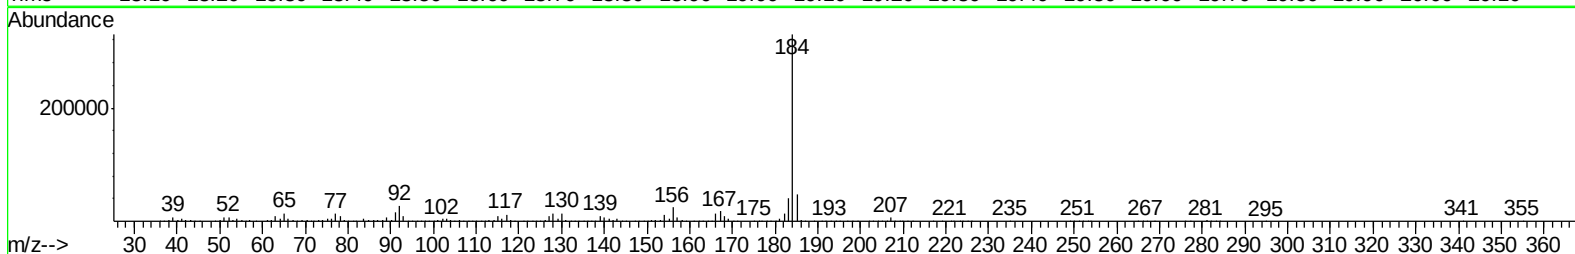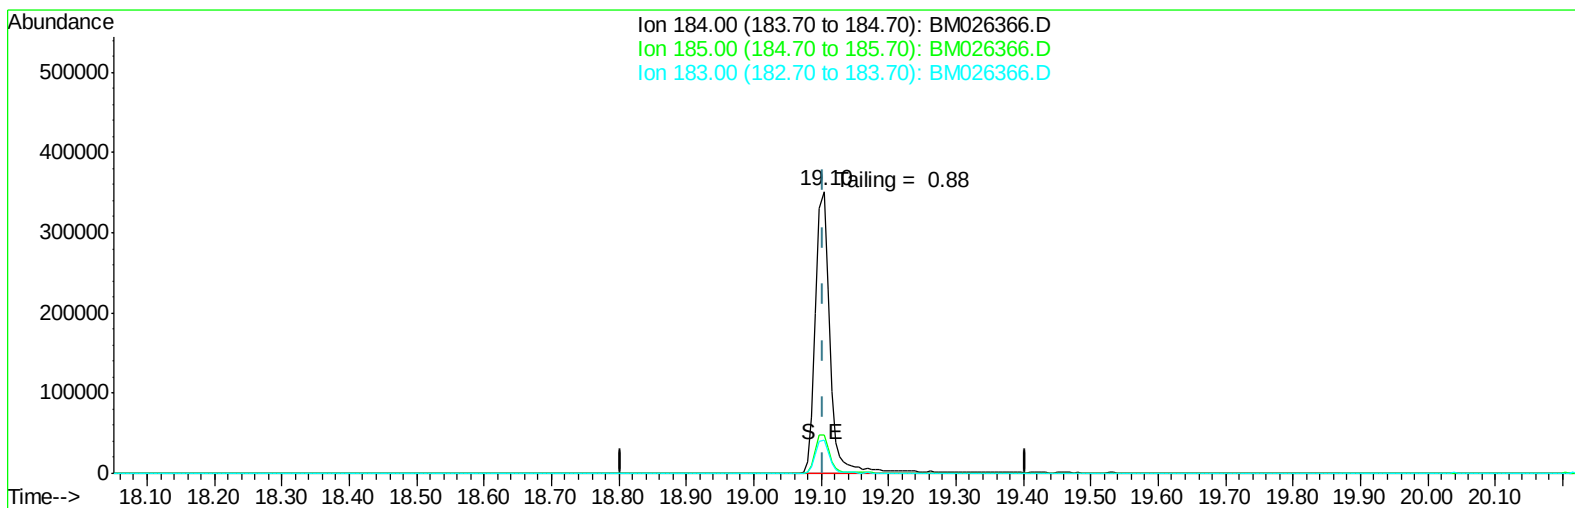

TIC: BM026366.D

(77) Benzidine

19.104min (+0.000) 31073.94ng

response 511845

Ion	Exp%	Act%
184.00	100	100
185.00	14.60	13.76
183.00	11.60	12.04
0.00	0.00	0.00