


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061120\  
 Data File : BM026349.D  
 Acq On : 11 Jun 2020 09:21  
 Operator : JU/CG  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\8270-BM060520.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Tue Jun 09 14:46:47 2020

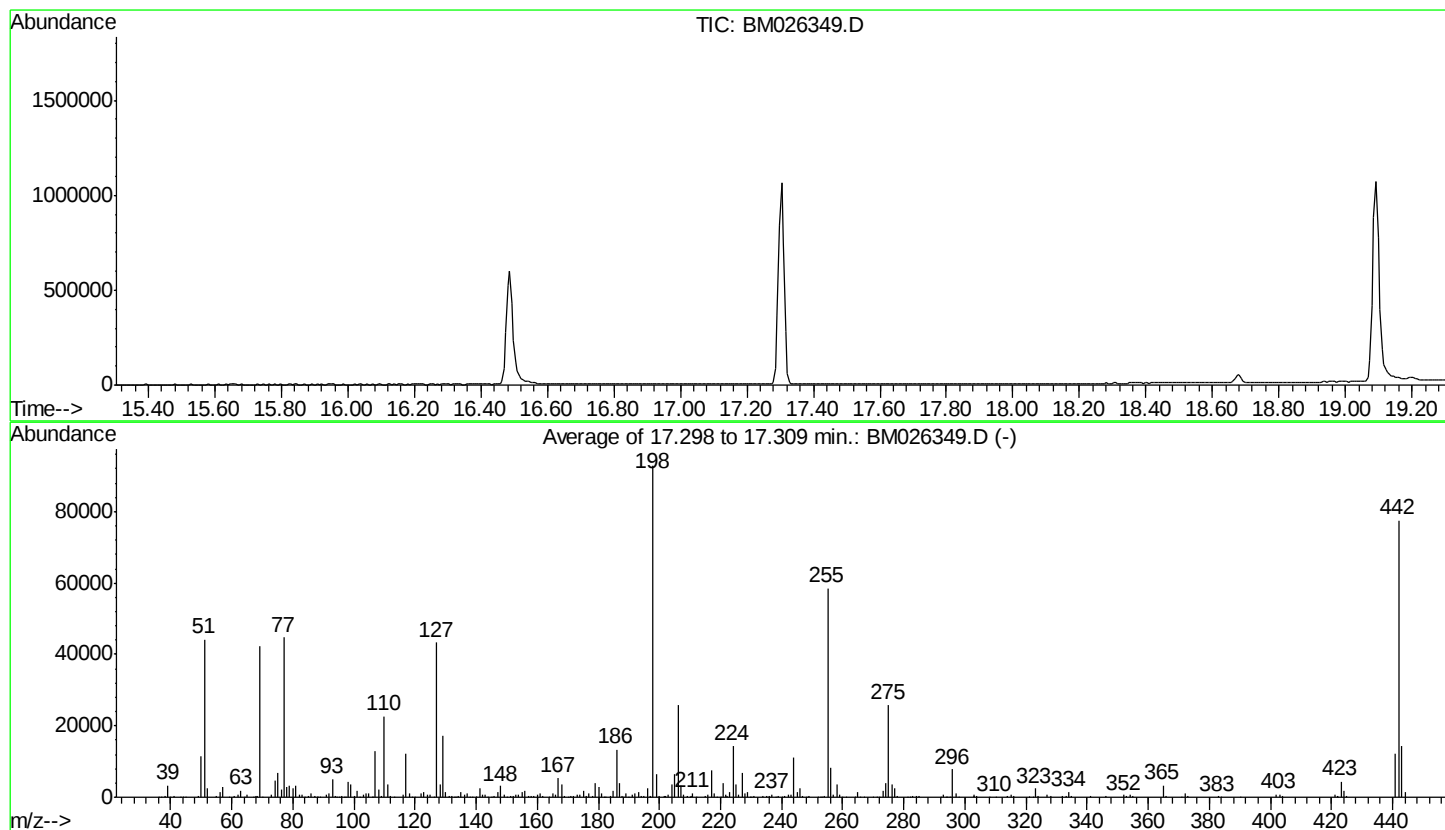

AutoFind: Scans 2450, 2451, 2452; Background Corrected with Scan 2444

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 47.5      | 44138   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.0       | 410     | PASS             |
| 69          | 198          | 0.00         | 100          | 45.5      | 42293   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.4       | 186     | PASS             |
| 127         | 198          | 10           | 80           | 46.6      | 43240   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.5       | 419     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 92880   | PASS             |
| 199         | 198          | 5            | 9            | 6.9       | 6420    | PASS             |
| 275         | 198          | 10           | 60           | 28.0      | 25997   | PASS             |
| 365         | 198          | 1            | 100          | 3.7       | 3391    | PASS             |
| 441         | 198          | 0.01         | 100          | 13.1      | 12127   | PASS             |
| 442         | 198          | 50           | 100          | 83.5      | 77538   | PASS             |
| 443         | 442          | 15           | 24           | 18.6      | 14421   | PASS             |