


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061120\
 Data File : BM026366.D
 Acq On : 11 Jun 2020 23:04
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM060520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 09 14:46:47 2020

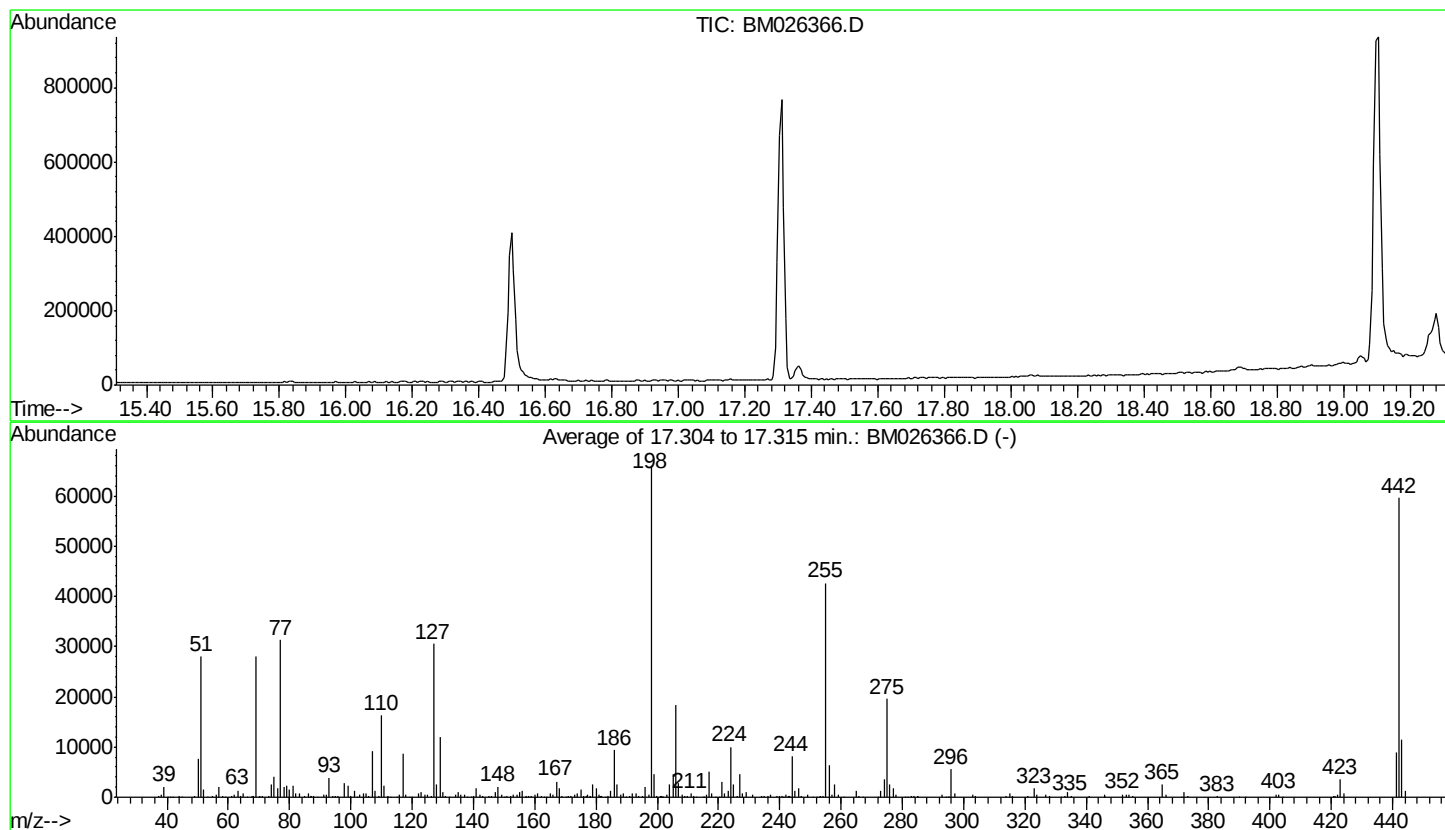

AutoFind: Scans 2451, 2452, 2453; Background Corrected with Scan 2444

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.3	27931	PASS
68	69	0.00	2	1.1	313	PASS
69	198	0.00	100	42.5	28021	PASS
70	69	0.00	2	0.7	190	PASS
127	198	10	80	46.2	30522	PASS
197	198	0.00	2	0.8	510	PASS
198	198	100	100	100.0	66000	PASS
199	198	5	9	7.1	4707	PASS
275	198	10	60	29.7	19604	PASS
365	198	1	100	3.7	2466	PASS
441	198	0.01	100	13.7	9048	PASS
442	198	50	100	90.3	59594	PASS
443	442	15	24	19.1	11381	PASS