

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061124\
 Data File : BM045977.D
 Acq On : 11 Jun 2024 15:43
 Operator : MA/JU
 Sample : PB161248BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK248

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045977.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.040	5	9	15	rBV	29136	48059	1.52%	0.147%
2	3.128	23	24	27	rBV3	3311	3627	0.11%	0.011%
3	3.451	77	79	100	rBV	257673	666354	21.06%	2.041%
4	3.728	120	126	133	rVB	30675	45771	1.45%	0.140%
5	4.146	195	197	201	rVB4	6464	8697	0.27%	0.027%
6	4.234	205	212	218	rVB2	6948	18282	0.58%	0.056%
7	4.587	271	272	276	rBV3	2808	3537	0.11%	0.011%
8	5.216	376	379	381	rBV4	3089	3989	0.13%	0.012%
9	5.504	426	428	430	rBV3	3173	3949	0.12%	0.012%
10	6.540	599	604	608	rBV6	4273	8296	0.26%	0.025%
11	6.698	624	631	644	rBV	453341	911567	28.82%	2.792%
12	6.804	644	649	671	rVB	324688	677952	21.43%	2.077%
13	7.004	676	683	697	rVB	498206	864079	27.31%	2.647%
14	7.439	751	757	774	rVB	380926	618216	19.54%	1.894%
15	8.210	882	888	904	rBV	548041	1027194	32.47%	3.146%
16	8.610	948	956	970	rVV	531558	941071	29.75%	2.883%
17	9.245	1058	1064	1067	rBV7	2287	4204	0.13%	0.013%
18	9.316	1069	1076	1089	rBV	398704	750287	23.72%	2.298%
19	9.798	1157	1158	1162	rVB4	3053	3315	0.10%	0.010%
20	9.869	1162	1170	1197	rBV	474697	1031044	32.59%	3.158%
21	10.210	1220	1228	1237	rBV	536433	903651	28.57%	2.768%
22	10.392	1252	1259	1276	rBV	463322	1102734	34.86%	3.378%
23	10.704	1311	1312	1318	rVB5	2710	3405	0.11%	0.010%
24	11.839	1500	1505	1510	rBV5	6048	11429	0.36%	0.035%
25	12.304	1579	1584	1587	rBV7	1931	3847	0.12%	0.012%
26	13.539	1787	1794	1805	rBV	1067534	1667471	52.71%	5.108%
27	13.774	1828	1834	1852	rBV2	1200708	1823457	57.64%	5.585%
28	14.086	1880	1887	1896	rBV	855981	1223444	38.67%	3.747%
29	14.386	1931	1938	1962	rBV	434413	934956	29.55%	2.864%
30	15.086	2049	2057	2071	rBV	1540578	2216918	70.08%	6.791%
31	15.227	2075	2081	2094	rBV	540029	767376	24.26%	2.351%
32	15.327	2095	2098	2101	rVB3	8111	10203	0.32%	0.031%
33	15.492	2122	2126	2130	rBV6	2441	3297	0.10%	0.010%
34	16.033	2212	2218	2219	rBV6	2839	3550	0.11%	0.011%
35	16.833	2345	2354	2364	rBV	1084750	1516716	47.94%	4.646%
36	16.933	2364	2371	2383	rBV	1655299	2468528	78.03%	7.561%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061124\
Data File : BM045977.D
Acq On : 11 Jun 2024 15:43
Operator : MA/JU
Sample : PB161248BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK248

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
Title : SVOA CALIBRATION

37	17.256	2423	2426	2429	rVB5	2641	3484	0.11%	0.011%
38	17.409	2450	2452	2457	rBV6	2708	3984	0.13%	0.012%
39	17.780	2509	2515	2523	rBV2	33007	78854	2.49%	0.242%
40	18.139	2571	2576	2577	rBV4	3558	4822	0.15%	0.015%
41	18.180	2580	2583	2586	rBV5	2132	3180	0.10%	0.010%
42	18.792	2683	2687	2692	rBV2	21797	32567	1.03%	0.100%
43	18.868	2696	2700	2704	rVB2	18254	23733	0.75%	0.073%
44	19.062	2729	2733	2734	rBV3	14874	18501	0.58%	0.057%
45	19.233	2756	2762	2772	rVB	2116521	2918396	92.25%	8.939%
46	20.268	2935	2938	2942	rBV	63443	69711	2.20%	0.214%
47	21.044	3065	3070	3082	rBV	1233606	1746529	55.21%	5.350%
48	22.974	3394	3398	3403	rVB2	78807	126413	4.00%	0.387%
49	23.562	3491	3498	3509	rVB2	1501413	3163459	100.00%	9.690%
50	23.744	3522	3529	3540	rVB	911016	2153136	68.06%	6.595%




Sum of corrected areas: 32647241

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061124\
Data File : BM045977.D
Acq On : 11 Jun 2024 15:43
Operator : MA/JU
Sample : PB161248BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK248

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

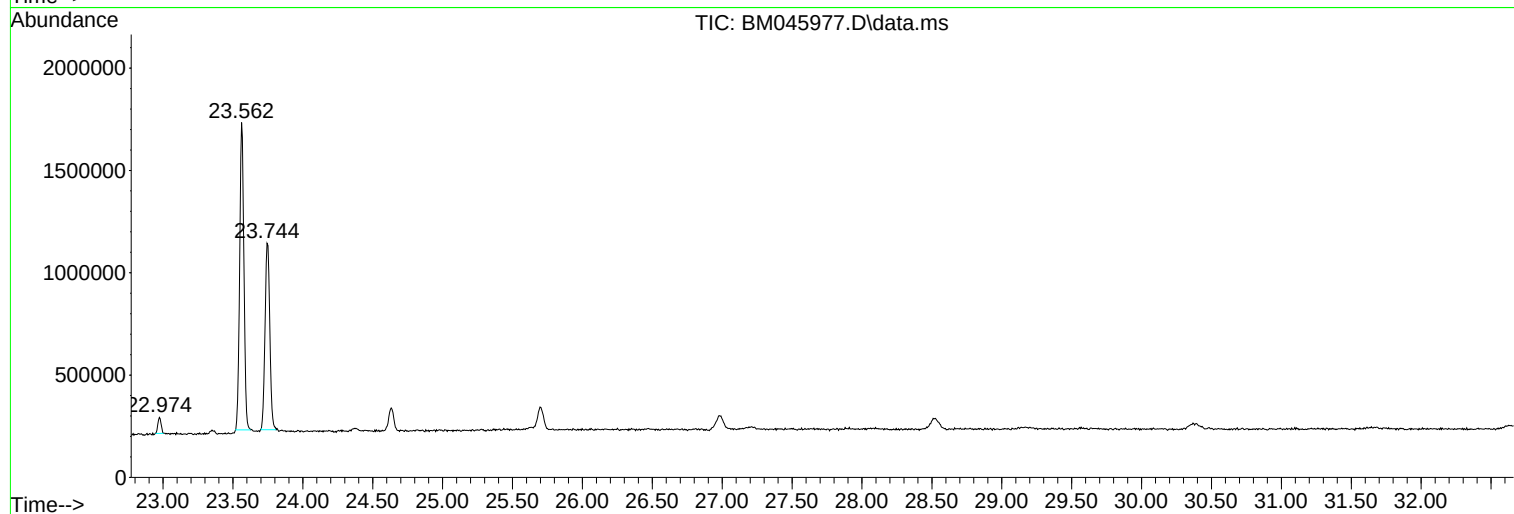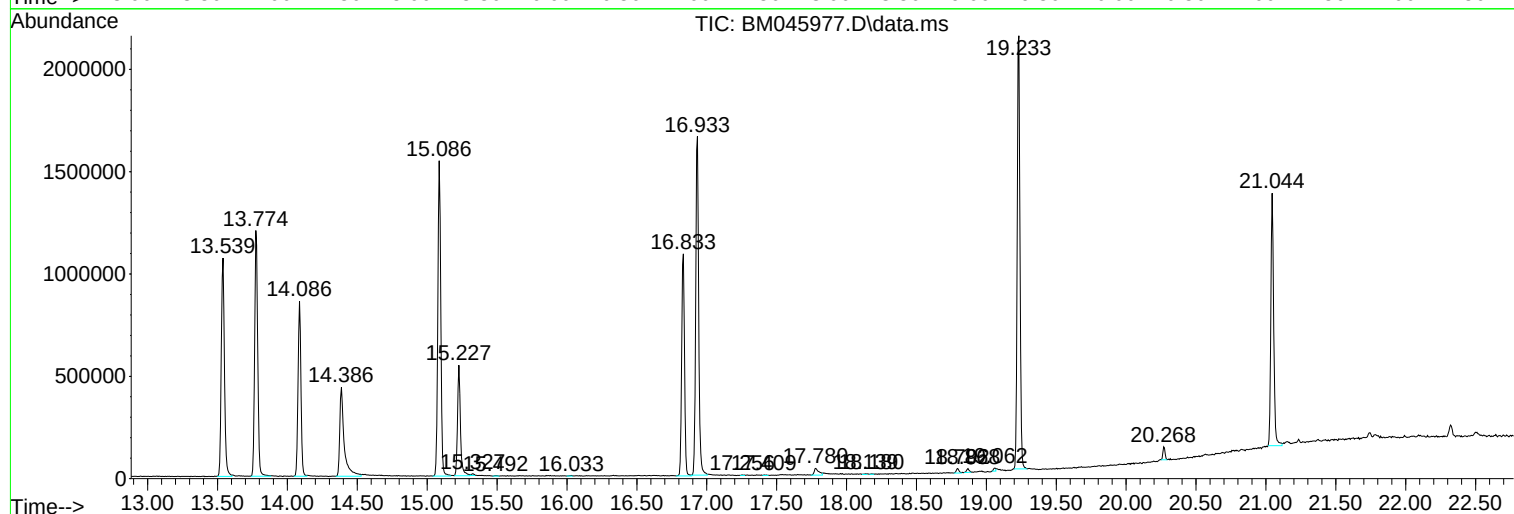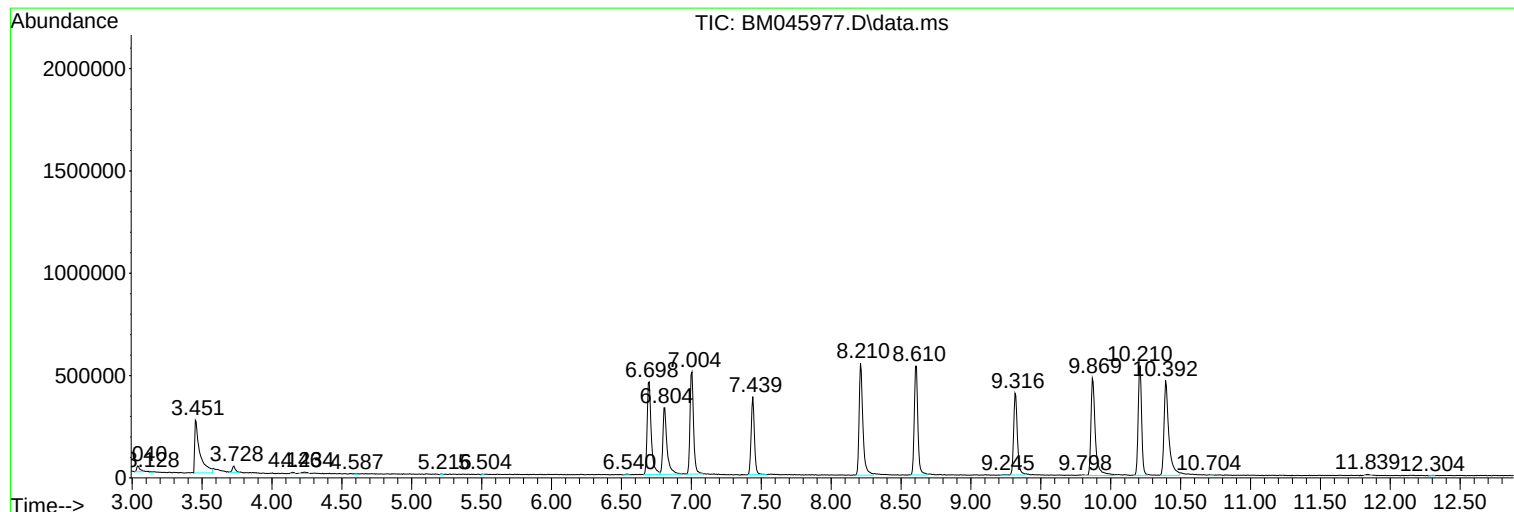

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061124\
Data File : BM045977.D
Acq On : 11 Jun 2024 15:43
Operator : MA/JU
Sample : PB161248BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK248

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061124\
Data File : BM045977.D
Acq On : 11 Jun 2024 15:43
Operator : MA/JU
Sample : PB161248BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK248

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc