
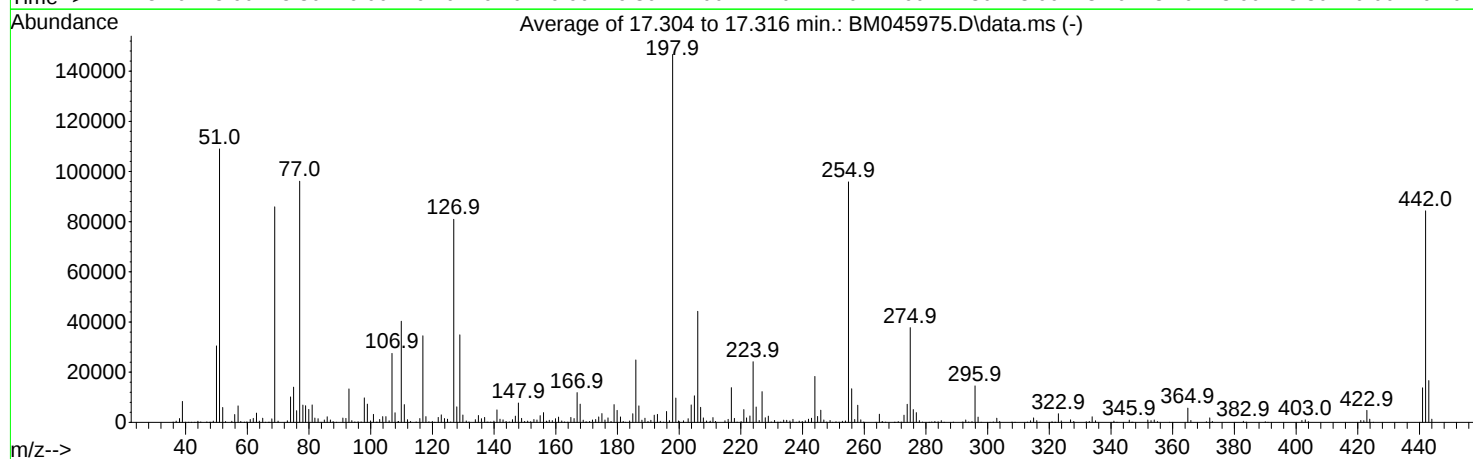


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061124\
Data File : BM045975.D
Acq On : 11 Jun 2024 14:24
Operator : MA/JU
Sample : DFTPP025
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP025

Integration File: LSCINT.P

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
Title : SVOA CALIBRATION
Last Update : Tue Jun 11 16:01:34 2024

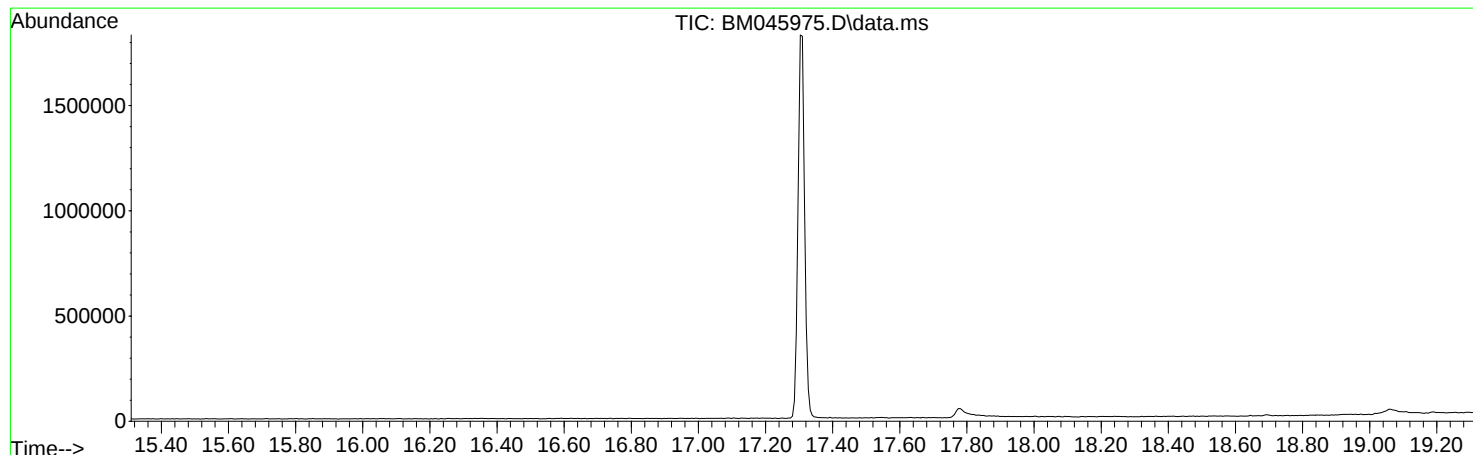

AutoFind: Scans 2434, 2435, 2436; Background Corrected with Scan 2428

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	74.3	109013	PASS
68	69	0.00	2	1.7	1434	PASS
69	198	0.00	100	58.6	85920	PASS
70	69	0.00	2	0.6	509	PASS
127	198	10	80	55.2	80949	PASS
197	198	0.00	2	0.5	720	PASS
198	198	100	100	100.0	146632	PASS
199	198	5	9	6.6	9722	PASS
275	198	10	60	25.8	37760	PASS
365	198	1	100	3.9	5709	PASS
441	198	0.01	100	9.4	13793	PASS
442	198	50	100	57.5	84320	PASS
443	442	15	24	19.7	16631	PASS

m/z	Abundance
38.90	288.0
39.90	2671.0
41.00	423.0
41.90	184.0
43.10	389.0
44.00	3690.0
44.90	263.0
48.90	688.0
51.00	454.0
54.90	211.0
73.00	946.0
75.00	248.0
76.90	211.0
78.00	252.0
83.80	342.0
85.90	169.0
95.80	181.0
133.00	333.0
134.90	181.0
146.90	240.0
190.70	154.0
206.90	1482.0
207.80	173.0
209.00	157.0
221.00	215.0
280.90	435.0
282.90	199.0

Instrument :

BNA_M

ClientSampleId :

DFTPP025

m/z	Abundance
35.90	170.0
37.00	828.0
38.00	1731.0
39.00	11044.0
39.90	2933.0
41.00	676.0
41.90	255.0
42.90	557.0
44.00	4256.0
45.00	493.0
46.90	179.0
47.80	197.0
49.00	1468.0
50.00	38688.0
51.00	136640.0
52.00	7436.0
52.90	353.0
55.00	889.0
55.90	3819.0
57.00	7759.0
57.90	429.0
59.00	186.0
59.90	159.0
60.90	1473.0
61.90	1877.0
63.00	4171.0
63.90	833.0
65.00	2169.0
65.90	164.0
66.90	294.0
68.00	1721.0
68.90	106912.0
70.00	524.0
73.00	1694.0
74.00	12866.0
75.00	17864.0
76.00	5586.0
77.00	118656.0
78.00	8145.0
78.90	8506.0
79.90	6529.0
81.00	8968.0
81.90	2219.0
82.90	1703.0
83.90	355.0
85.00	1159.0
85.90	2970.0
87.00	1193.0
87.80	535.0
88.90	230.0
90.90	2093.0
92.00	2047.0
92.90	16160.0
93.90	993.0
94.80	165.0
95.90	670.0
96.90	318.0
97.90	11656.0
98.90	8770.0
100.00	671.0
100.90	4034.0
101.80	266.0
102.90	1386.0
103.90	2846.0
104.90	2664.0
105.90	888.0
106.90	34344.0
107.90	4484.0
108.80	722.0
109.90	49768.0
110.90	8466.0
112.00	1300.0
112.90	575.0
114.70	223.0
115.90	1744.0
116.90	41432.0
117.90	2436.0
118.90	259.0
119.90	381.0
120.80	152.0
121.90	2482.0
122.90	3796.0
123.90	2086.0
124.90	1469.0
126.00	239.0
126.90	96592.0
127.90	7187.0
128.90	42464.0
129.90	3150.0
130.90	632.0
132.80	361.0
133.90	1315.0

Instrument :
BNA_M
ClientSampleId :
DFTPP025

135.00	4076.0
135.90	1788.0
136.90	2312.0
137.70	313.0
138.80	371.0
140.00	670.0
140.90	5978.0
141.90	1551.0
142.90	1356.0
143.90	316.0
144.90	292.0
145.90	1161.0
146.90	3056.0
147.90	8533.0
148.90	2301.0
149.90	403.0
150.90	766.0
151.80	460.0
152.90	1351.0
153.90	1134.0
154.90	3303.0
156.00	4377.0
156.90	616.0
157.80	852.0
158.90	987.0
159.90	1865.0
160.90	2390.0
162.00	764.0
162.80	242.0
163.90	164.0
164.90	2253.0
166.00	1873.0
166.90	14112.0
167.90	8548.0
168.90	1046.0
170.00	409.0
171.00	412.0
171.90	1138.0
172.90	1253.0
173.90	2782.0
175.00	3896.0
175.90	1200.0
176.90	2162.0
177.90	529.0
178.90	7825.0
179.90	5517.0
180.90	2836.0
181.80	467.0
182.70	156.0
183.90	717.0
185.00	3772.0
185.90	29280.0
186.90	7414.0
187.90	1058.0
188.90	2214.0
189.90	393.0
190.90	791.0
191.90	3376.0
192.90	3226.0
193.90	589.0
195.00	197.0
195.90	4863.0
196.90	787.0
197.90	168000.0
198.90	11811.0
199.80	1323.0
201.40	771.0
202.90	1631.0
203.90	8020.0
204.90	11920.0
206.00	49720.0
207.00	8402.0
207.90	2210.0
208.90	571.0
210.00	710.0
211.00	2266.0
211.70	536.0
214.90	701.0
215.90	1236.0
216.90	15744.0
217.90	1754.0
218.80	238.0
220.10	366.0
221.00	5971.0
221.90	2077.0
222.90	3001.0
224.00	26744.0
224.90	6554.0
225.90	985.0
226.90	13537.0
227.90	2049.0
228.90	2711.0
229.90	273.0
230.90	992.0
232.00	170.0
232.80	174.0

Instrument :
BNA_M
ClientSampleId :
DFTPP025

233.90	855.0
234.80	873.0
235.90	745.0
236.90	1293.0
238.90	763.0
239.90	421.0
240.90	744.0
241.90	1634.0
242.90	1716.0
244.00	20240.0
244.90	2722.0
245.90	5271.0
246.90	993.0
247.90	229.0
248.90	691.0
250.80	386.0
251.90	163.0
252.90	665.0
253.90	639.0
254.90	104384.0
255.90	14695.0
256.90	1127.0
257.90	7578.0
258.90	951.0
259.90	299.0
264.90	3282.0
265.80	372.0
269.80	165.0
271.10	294.0
272.00	223.0
272.90	3227.0
273.90	7777.0
274.90	40904.0
275.90	5749.0
276.90	4157.0
277.90	783.0
279.00	154.0
281.00	374.0
281.90	245.0
283.00	751.0
283.90	337.0
284.90	864.0
291.80	275.0
292.90	988.0
293.90	280.0
294.90	272.0
295.90	15153.0
296.90	1902.0
300.80	177.0
301.90	288.0
302.90	1675.0
303.90	463.0
307.90	220.0
308.90	156.0
313.80	561.0
314.90	1939.0
315.90	785.0
320.80	373.0
322.90	3345.0
323.90	755.0
326.90	1000.0
327.90	400.0
332.00	274.0
332.90	393.0
333.90	2647.0
334.90	661.0
340.90	542.0
345.90	733.0
346.70	154.0
352.00	802.0
352.90	837.0
354.00	1083.0
355.00	395.0
359.00	172.0
364.90	5462.0
365.90	557.0
370.90	242.0
372.00	1953.0
372.80	363.0
382.90	439.0
383.80	212.0
390.00	201.0
390.90	169.0
401.90	699.0
403.00	873.0
403.90	444.0
421.00	561.0
421.90	613.0
422.90	4622.0
423.90	1431.0
441.00	13481.0
442.00	77864.0
443.00	16159.0
444.00	1507.0

Instrument :
BNA_M
ClientSampleId :
DFTPP025

m/z	Abundance
36.00	210.0
36.90	514.0
38.00	1840.0
39.00	9519.0
40.00	2857.0
41.00	508.0
42.00	302.0
43.00	444.0
44.00	3888.0
45.00	473.0
46.90	225.0
48.00	226.0
49.00	1311.0
50.00	34720.0
51.00	123960.0
52.00	6541.0
53.00	412.0
55.00	569.0
55.90	3436.0
57.00	7421.0
57.90	489.0
59.00	159.0
59.80	229.0
61.00	1249.0
62.00	1824.0
62.90	4398.0
63.90	406.0
65.00	1688.0
67.10	214.0
67.90	1573.0
68.90	98288.0
70.00	582.0
73.00	1862.0
74.00	11409.0
75.00	15826.0
76.00	5515.0
77.00	111264.0
78.00	8609.0
78.90	7486.0
79.90	5794.0
81.00	8146.0
81.90	1741.0
83.00	1838.0
83.80	479.0
84.90	1178.0
86.00	2492.0
86.90	1126.0
87.80	306.0
91.00	1713.0
91.90	1912.0
93.00	15031.0
93.90	736.0
94.80	238.0
96.00	384.0
96.80	192.0
97.90	11308.0
98.90	8227.0
99.90	813.0
100.90	3549.0
102.00	237.0
102.90	1284.0
103.90	2675.0
105.00	2838.0
106.00	750.0
106.90	30312.0
107.90	4464.0
109.00	729.0
109.90	45200.0
110.90	8189.0
111.90	1173.0
112.90	425.0
114.80	309.0
115.90	1582.0
116.90	39808.0
117.90	2955.0
118.90	380.0
119.90	468.0
120.80	150.0
121.90	2397.0
122.90	3046.0
123.90	1471.0
124.90	1390.0
125.90	297.0
126.90	92952.0
127.90	7216.0
128.90	40448.0
129.90	3702.0
130.90	701.0
131.90	255.0
132.90	362.0
133.90	1308.0
134.90	2747.0

Instrument :
BNA_M
ClientSampleId :
DFTPP025

135.90	1735.0
137.00	2539.0
138.00	319.0
139.00	230.0
139.90	638.0
140.90	6217.0
141.90	1548.0
142.90	1173.0
143.90	527.0
145.00	207.0
146.00	1352.0
146.90	3175.0
147.90	9068.0
148.90	1556.0
149.90	370.0
150.90	570.0
151.80	389.0
152.90	1265.0
153.90	1052.0
155.00	3125.0
156.00	4762.0
157.00	998.0
157.90	1015.0
158.80	730.0
159.90	1565.0
160.90	2294.0
161.90	763.0
162.90	379.0
163.90	227.0
164.90	2428.0
165.90	1699.0
166.90	13655.0
167.90	7892.0
168.90	1169.0
169.70	379.0
170.90	493.0
171.90	1005.0
173.00	1476.0
173.90	2472.0
174.90	4061.0
176.00	1064.0
176.90	1969.0
177.90	561.0
178.90	8291.0
179.90	5487.0
181.00	2389.0
181.90	422.0
184.00	689.0
184.90	3972.0
186.00	28992.0
187.00	7622.0
187.90	1239.0
188.90	1626.0
189.90	445.0
190.90	1293.0
191.90	3402.0
192.90	3679.0
193.90	518.0
194.90	293.0
195.90	5046.0
196.90	809.0
197.90	171520.0
198.90	10879.0
200.00	992.0
201.30	681.0
202.90	1942.0
203.90	8127.0
205.00	11804.0
206.00	52272.0
207.00	8554.0
207.90	2362.0
208.90	1082.0
210.10	911.0
210.90	2221.0
211.80	339.0
214.80	765.0
215.90	1355.0
216.90	15462.0
217.90	2050.0
218.80	189.0
220.20	309.0
220.90	5996.0
221.80	2216.0
222.90	2642.0
223.90	29464.0
225.00	7313.0
226.00	979.0
226.90	14567.0
227.90	2453.0
228.90	2869.0
229.80	416.0
230.90	740.0
232.80	211.0
233.90	1147.0
234.90	949.0
235.90	664.0

Instrument :
BNA_M
ClientSampleId :
DFTPP025

236.90	1236.0
238.00	209.0
238.80	514.0
239.90	403.0
240.90	866.0
241.90	1392.0
242.90	1998.0
244.00	21072.0
244.90	2711.0
245.90	5443.0
246.90	1233.0
247.80	243.0
248.90	921.0
249.80	194.0
250.90	298.0
251.80	230.0
252.90	421.0
253.90	676.0
254.90	111736.0
255.90	15827.0
256.90	1505.0
257.90	7365.0
258.90	1394.0
259.70	193.0
263.80	171.0
264.90	3760.0
265.80	328.0
266.00	333.0
267.00	286.0
270.00	155.0
271.00	487.0
272.00	235.0
272.90	3296.0
273.90	8285.0
274.90	44208.0
275.90	5741.0
276.90	4847.0
277.80	624.0
278.80	176.0
280.90	321.0
281.90	355.0
282.90	582.0
284.00	307.0
285.00	647.0
285.90	150.0
288.90	246.0
292.10	189.0
292.90	1116.0
293.90	266.0
295.00	273.0
295.90	17368.0
296.90	2480.0
297.90	169.0
301.80	194.0
303.00	1986.0
303.90	521.0
312.90	170.0
313.90	767.0
314.90	1897.0
316.00	958.0
316.90	154.0
320.80	293.0
321.80	286.0
323.00	4231.0
323.90	561.0
326.90	1198.0
327.90	440.0
331.90	280.0
333.00	422.0
333.90	2236.0
335.00	759.0
341.00	488.0
341.90	170.0
345.90	1303.0
346.90	228.0
352.00	1128.0
353.00	897.0
354.00	1028.0
355.10	301.0
364.90	6677.0
365.90	1052.0
370.90	311.0
372.00	2056.0
372.90	487.0
382.90	451.0
383.90	202.0
390.00	290.0
401.90	794.0
403.00	1323.0
403.90	308.0
421.00	1124.0
422.00	838.0
423.00	5544.0
423.90	1459.0
441.00	15643.0
442.00	97584.0

Instrument :
BNA_M
ClientSampleId :
DFTPP025

443.0019160.0

444.001343.0

Instrument :

BNA_M

ClientSampleId :

DFTPP025

m/z	Abundance
37.00	307.0
37.90	1010.0
39.00	5321.0
40.00	2407.0
41.00	343.0
42.00	199.0
43.00	461.0
44.00	4342.0
44.90	491.0
46.90	197.0
49.00	927.0
50.00	18136.0
51.00	67800.0
52.00	3799.0
52.90	277.0
55.00	529.0
55.90	2081.0
56.90	4509.0
57.90	190.0
59.90	267.0
60.90	744.0
61.90	1118.0
62.90	2615.0
64.00	302.0
64.90	1047.0
67.90	1009.0
68.90	52560.0
69.90	421.0
73.00	1120.0
74.00	6135.0
75.00	9258.0
76.00	2846.0
77.00	59136.0
78.00	4630.0
79.00	3974.0
80.00	3195.0
80.90	3848.0
81.90	1310.0
83.00	930.0
84.00	439.0
84.90	551.0
85.90	1669.0
87.00	527.0
87.90	232.0
90.90	1402.0
92.00	886.0
92.90	8815.0
93.90	395.0
94.90	267.0
95.90	309.0
97.00	182.0
98.00	6283.0
98.90	4769.0
100.00	200.0
100.90	2030.0
102.00	211.0
103.00	803.0
103.80	1325.0
104.90	1475.0
106.00	334.0
106.90	17856.0
107.90	2559.0
109.00	427.0
109.90	26032.0
110.90	4703.0
112.00	867.0
112.90	267.0
115.90	1228.0
116.90	22216.0
117.90	1511.0
118.90	186.0
120.00	310.0
121.90	1143.0
122.90	2137.0
123.80	973.0
124.90	1012.0
126.90	53304.0
127.90	4205.0
128.90	21816.0
129.90	2015.0
131.00	458.0
131.80	281.0
132.90	221.0
133.90	625.0
135.00	1991.0
135.90	834.0
136.90	1028.0
140.00	207.0
140.90	2775.0
142.00	804.0
142.90	489.0
143.90	240.0

Instrument :
BNA_M
ClientSampleId :
DFTPP025

144.80	183.0
145.90	766.0
146.90	1937.0
147.90	5583.0
148.80	1010.0
149.90	409.0
151.00	316.0
152.00	245.0
152.90	929.0
154.00	717.0
154.90	1629.0
156.00	2577.0
157.20	447.0
158.00	557.0
158.90	356.0
159.90	1029.0
160.90	1745.0
161.80	276.0
165.00	1269.0
165.90	1106.0
166.90	7922.0
167.90	5462.0
168.90	551.0
170.00	242.0
170.90	288.0
171.90	725.0
172.90	731.0
173.90	1323.0
174.90	2493.0
176.00	636.0
176.90	1263.0
177.90	180.0
178.90	5226.0
179.90	3433.0
181.00	1286.0
181.90	206.0
183.90	347.0
184.90	2590.0
185.90	16432.0
186.90	4646.0
187.90	448.0
188.90	1099.0
190.00	251.0
190.90	822.0
191.90	1877.0
193.00	2656.0
193.90	352.0
195.90	3159.0
196.70	563.0
197.90	100376.0
198.90	6476.0
199.80	445.0
201.50	557.0
202.90	852.0
203.90	4649.0
205.00	8028.0
206.00	30816.0
207.00	5535.0
207.90	1347.0
208.90	565.0
209.80	462.0
210.90	1178.0
211.90	239.0
214.90	460.0
215.90	1033.0
216.90	10409.0
217.90	1067.0
220.00	251.0
220.90	4097.0
221.80	1114.0
223.00	2054.0
224.00	16339.0
224.90	4545.0
226.00	368.0
226.90	8562.0
227.90	1154.0
228.90	1875.0
230.90	638.0
232.00	207.0
233.00	184.0
233.90	606.0
234.90	617.0
235.80	388.0
236.90	1183.0
239.00	342.0
239.90	261.0
240.90	392.0
241.80	772.0
242.90	1220.0
243.90	13697.0
245.00	1679.0
245.90	3802.0
246.90	637.0
248.90	595.0
250.80	196.0
252.80	309.0

Instrument :
BNA_M
ClientSampleId :
DFTPP025

254.00	417.0
254.90	71456.0
255.90	9684.0
256.90	858.0
257.90	5504.0
258.90	672.0
264.90	2812.0
265.90	368.0
266.90	171.0
270.90	190.0
272.90	2176.0
273.90	5528.0
274.90	28168.0
275.90	3911.0
276.90	2661.0
277.90	625.0
280.90	616.0
282.80	366.0
284.00	200.0
285.00	596.0
288.80	198.0
291.80	167.0
292.90	811.0
295.00	366.0
295.90	11118.0
296.90	1900.0
301.90	155.0
302.90	1422.0
303.90	254.0
307.90	169.0
312.90	165.0
314.00	609.0
314.90	1461.0
315.90	410.0
321.00	329.0
322.00	194.0
322.90	2812.0
323.90	506.0
326.90	880.0
327.90	400.0
331.90	204.0
332.90	275.0
333.90	1838.0
334.90	411.0
341.00	481.0
345.90	631.0
347.10	173.0
351.90	1038.0
352.90	424.0
354.00	804.0
355.00	359.0
364.90	4987.0
365.90	617.0
370.90	223.0
372.00	1341.0
372.80	397.0
382.90	475.0
390.00	350.0
401.90	813.0
403.00	867.0
404.00	261.0
420.90	535.0
422.00	626.0
422.90	4144.0
424.00	867.0
425.00	199.0
441.00	12256.0
442.00	77512.0
443.00	14575.0
444.00	940.0

Instrument :
BNA_M
ClientSampleId :
DFTPP025