

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061125\
 Data File : BM050286.D
 Acq On : 11 Jun 2025 22:40
 Operator : RC/JU
 Sample : Q2272-04
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 TP-6

Quant Time: Jun 12 02:57:19 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 09 11:54:38 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.763	152	379971	20.000	ng	0.00
21) Naphthalene-d8	10.551	136	1429067	20.000	ng	0.00
39) Acenaphthene-d10	14.392	164	753041	20.000	ng	0.00
64) Phenanthrene-d10	17.133	188	1356380	20.000	ng	0.00
76) Chrysene-d12	21.356	240	1403302	20.000	ng	-0.02
86) Perylene-d12	24.327	264	1484069	20.000	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.357	112	3274198	143.743	ng	0.00
7) Phenol-d6	6.934	99	3702054	123.463	ng	0.00
23) Nitrobenzene-d5	8.916	82	2660425	96.821	ng	0.00
42) 2,4,6-Tribromophenol	15.880	330	1217755	142.173	ng	0.00
45) 2-Fluorobiphenyl	13.022	172	5101659	91.720	ng	0.00
79) Terphenyl-d14	19.762	244	6629982	89.531	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061125\
Data File : BM050286.D
Acq On : 11 Jun 2025 22:40
Operator : RC/JU
Sample : Q2272-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TP-6

Quant Time: Jun 12 02:57:19 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

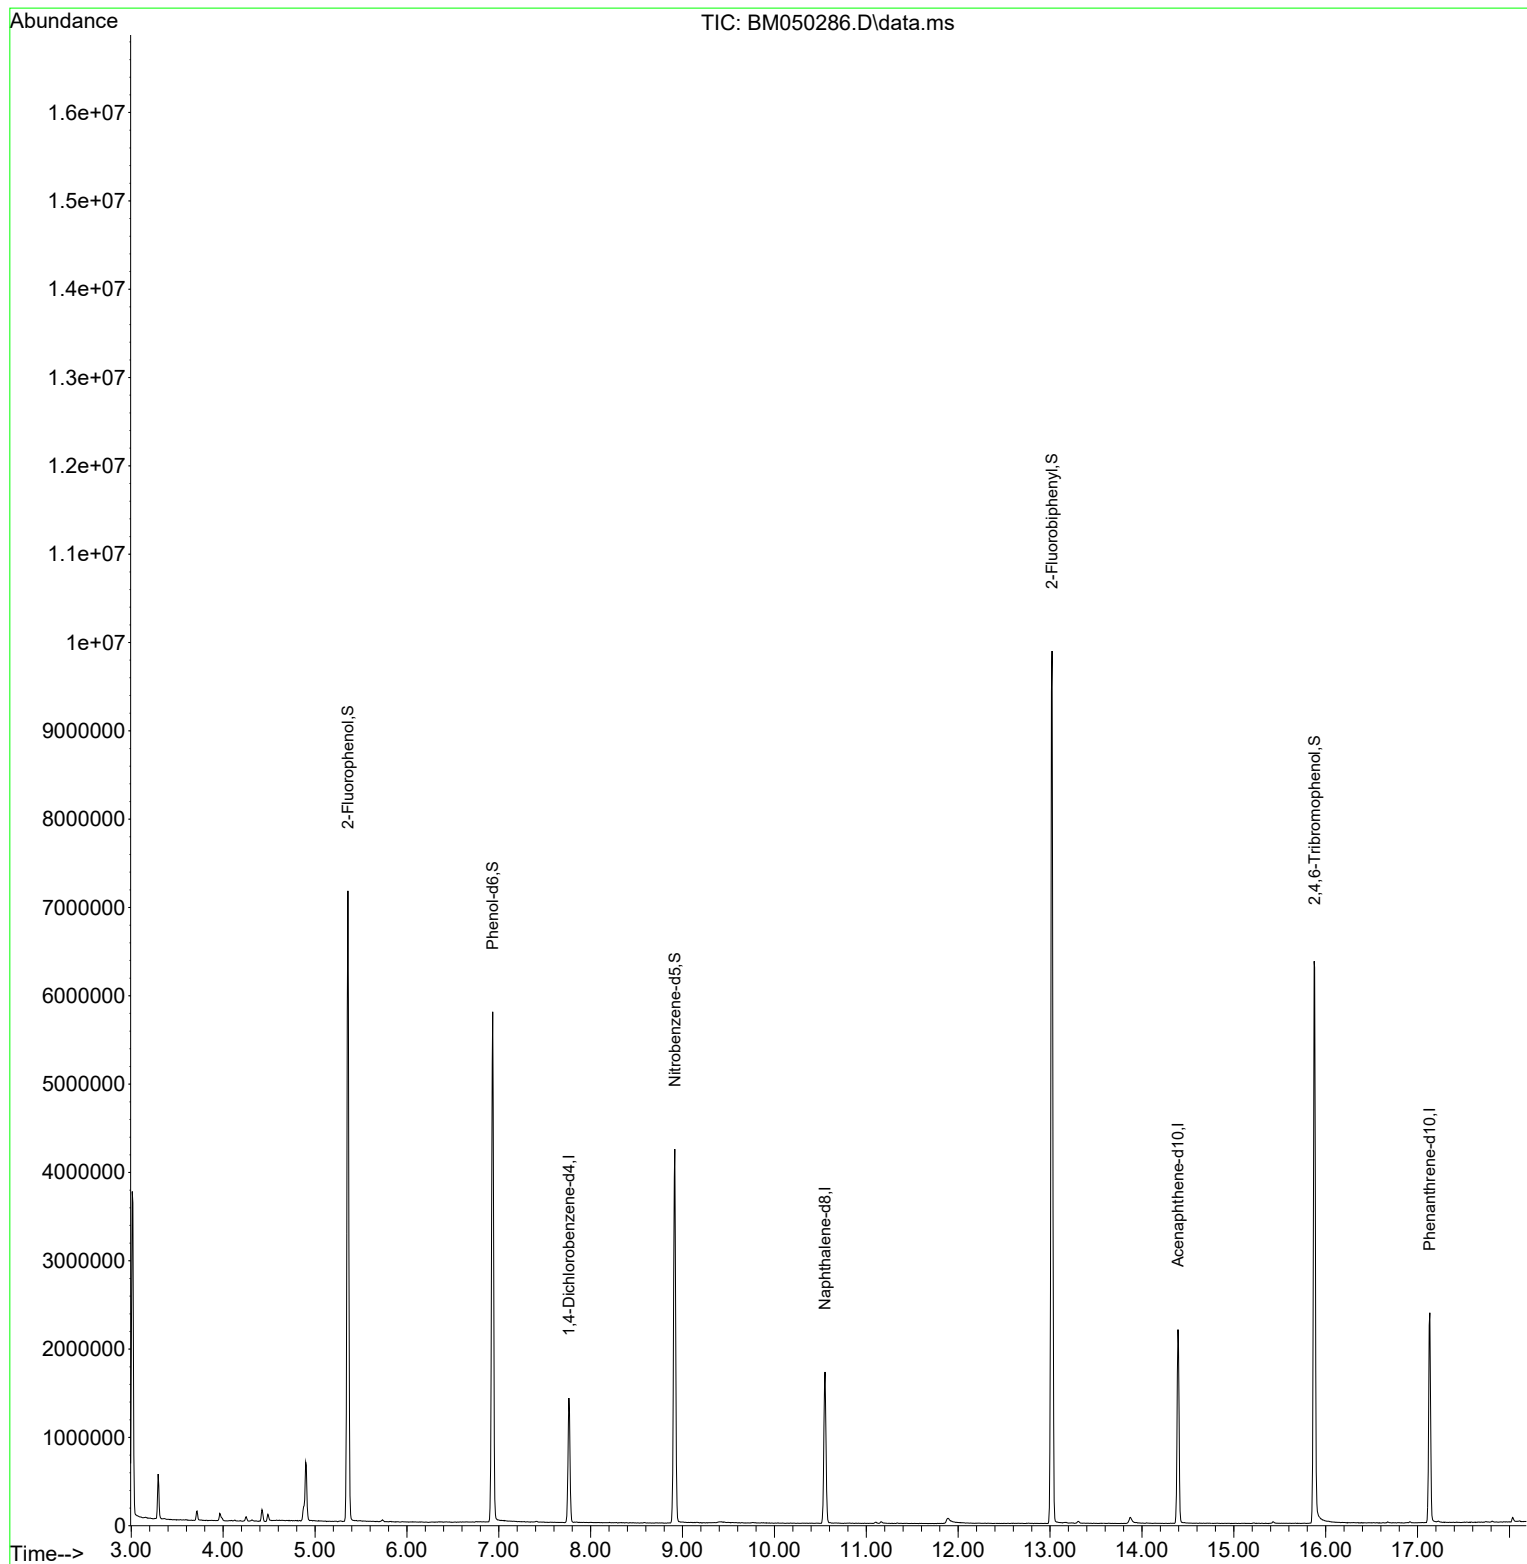

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061125\
Data File : BM050286.D
Acq On : 11 Jun 2025 22:40
Operator : RC/JU
Sample : Q2272-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TP-6

Quant Time: Jun 12 02:57:19 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

