
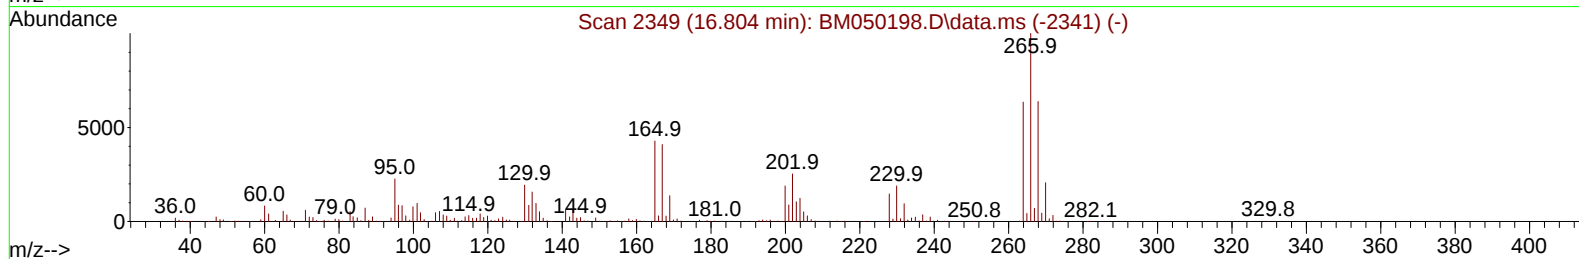
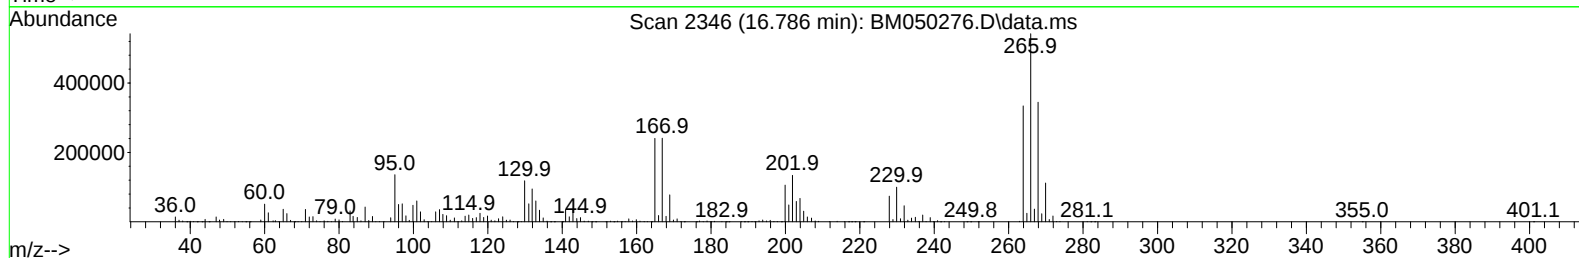


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061125\
Data File : BM050276.D
Acq On : 11 Jun 2025 15:46
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 11 18:44:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

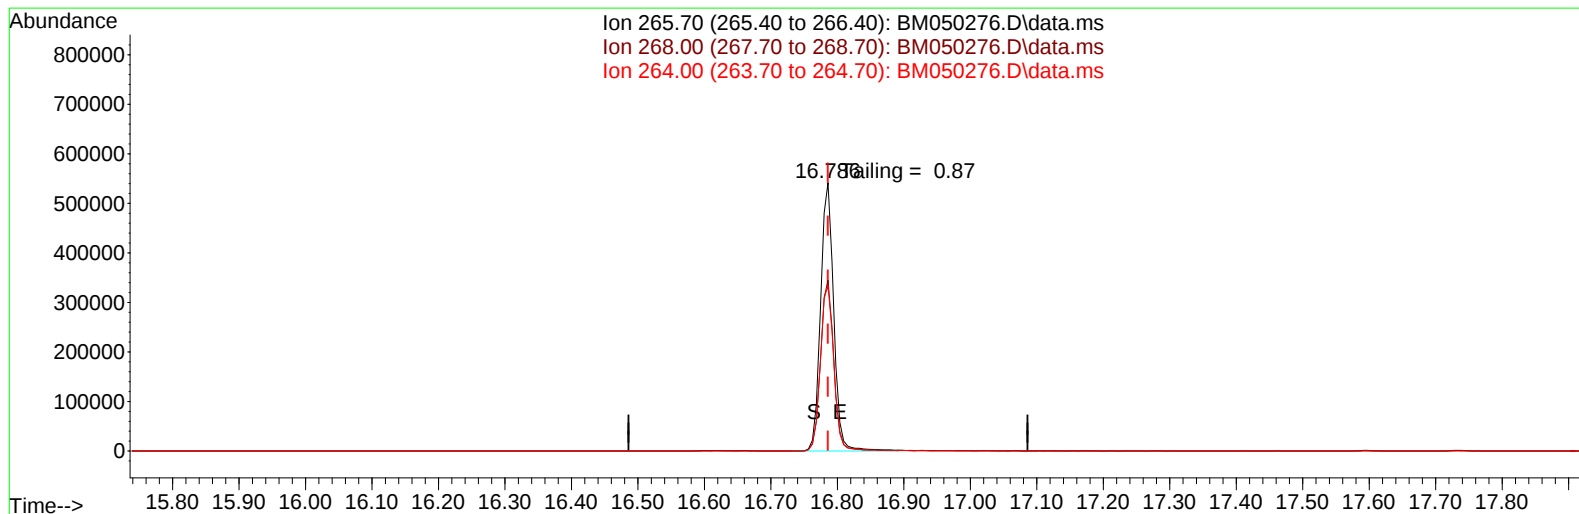

TIC: BM050276.D\data.ms

(70) Pentachlorophenol (C)




16.786min (-0.000) 1703653.44 ng

response 745212

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.56
264.00	63.50	61.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061125\
Data File : BM050276.D
Acq On : 11 Jun 2025 15:46
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 11 18:44:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

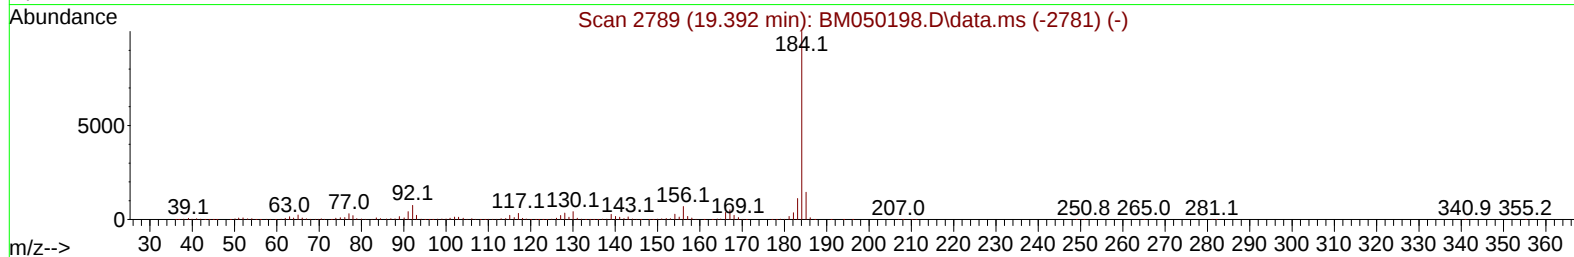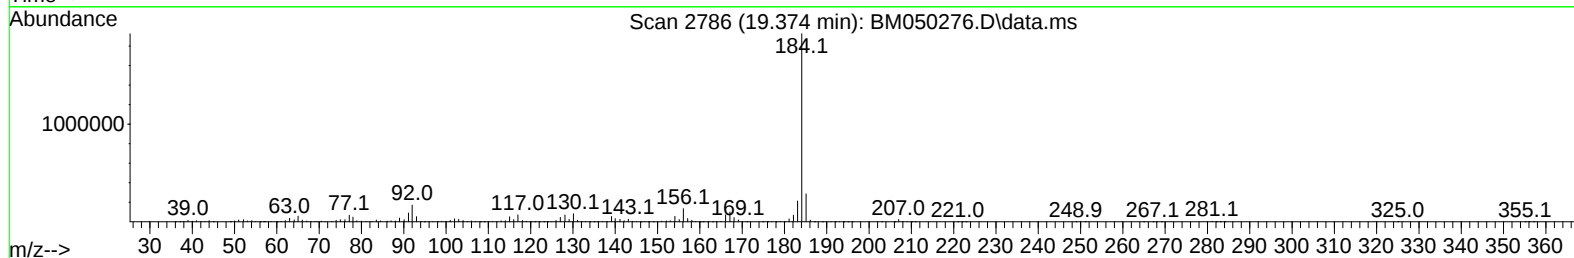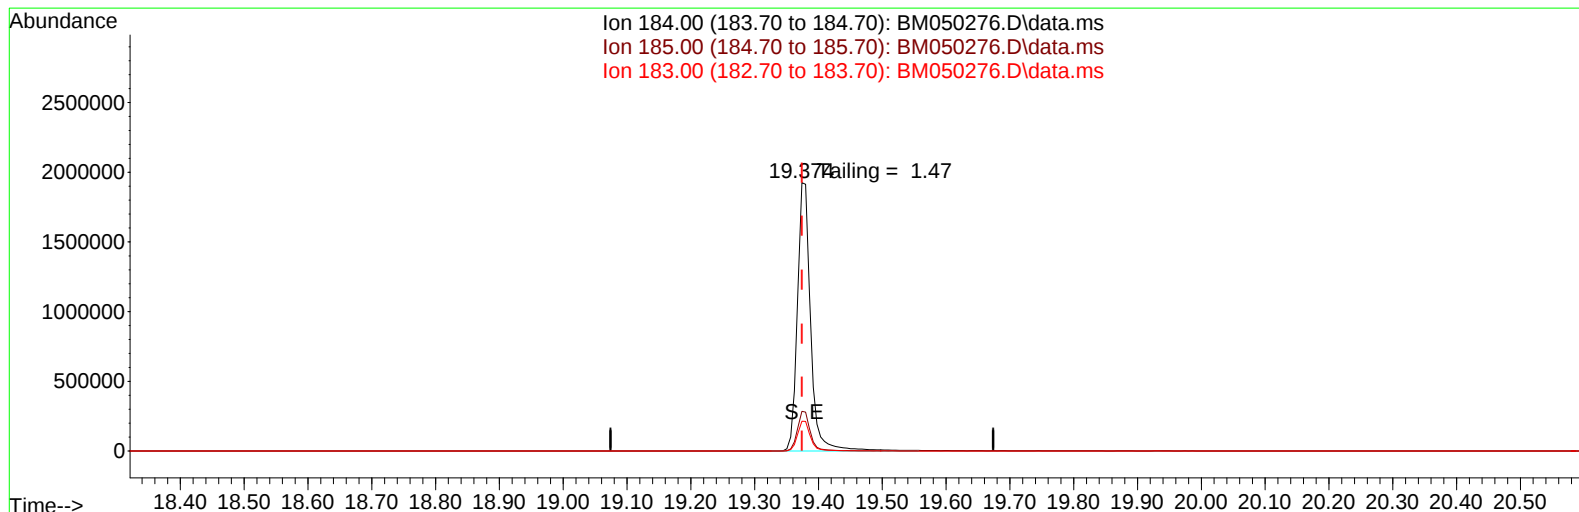

TIC: BM050276.D\data.ms

(77) Benzidine**19.374min (-0.000) 2147.98 ng****response 2793632**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.78
183.00	11.20	11.11
0.00	0.00	0.00