
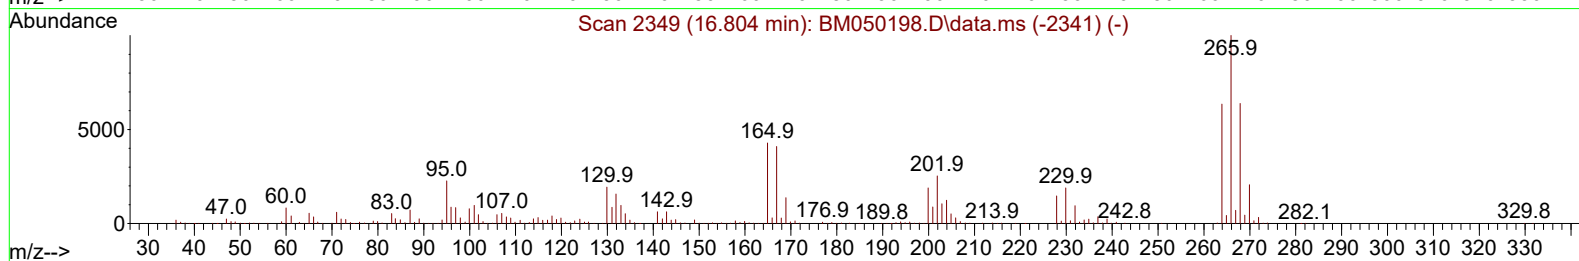
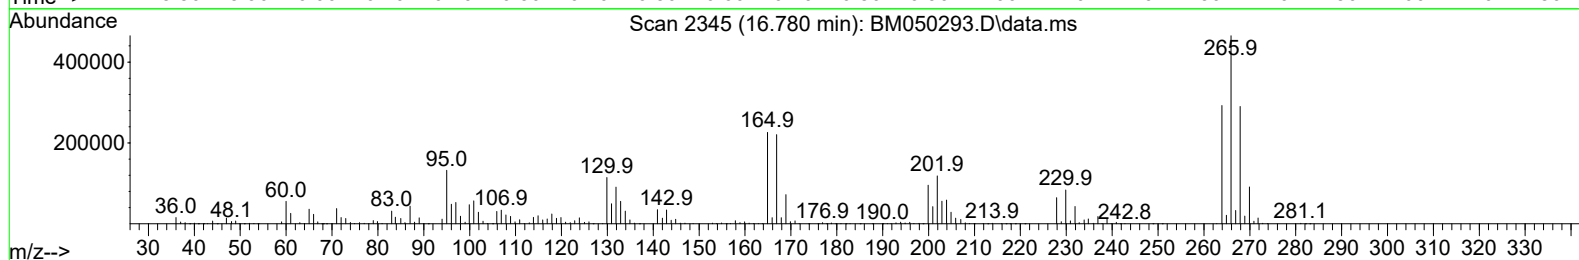


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061125\
Data File : BM050293.D
Acq On : 12 Jun 2025 03:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 12 05:28:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

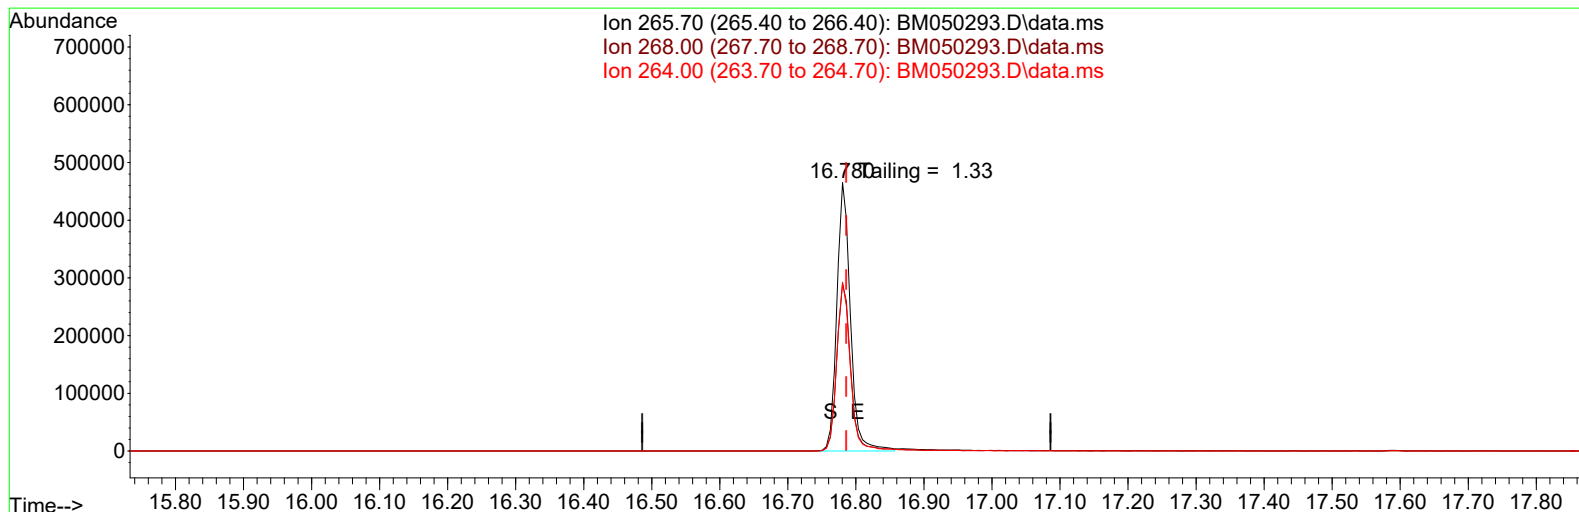

TIC: BM050293.D\data.ms

(70) Pentachlorophenol (C)




16.780min (-0.006) 258016.11 ng

response 647908

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	62.36
264.00	63.50	62.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061125\
Data File : BM050293.D
Acq On : 12 Jun 2025 03:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 12 05:28:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

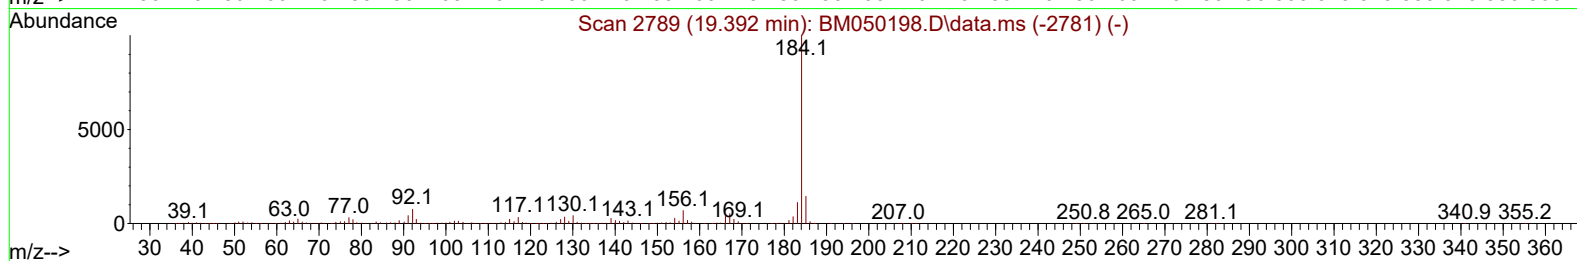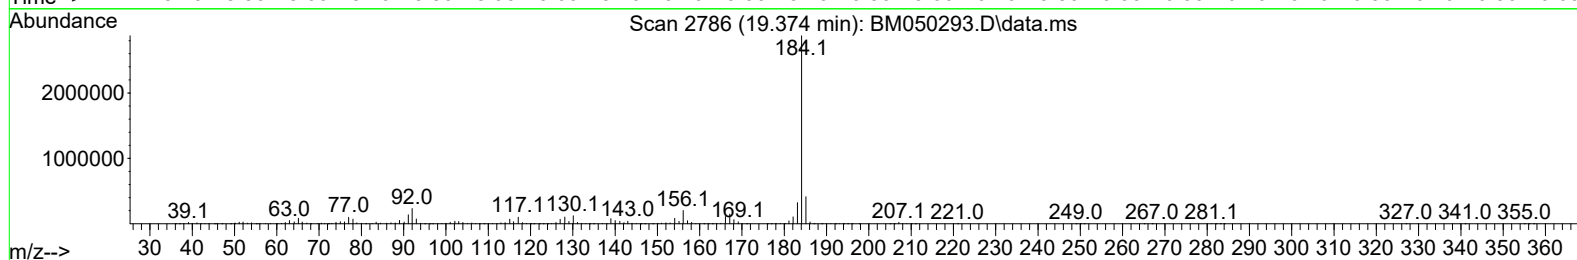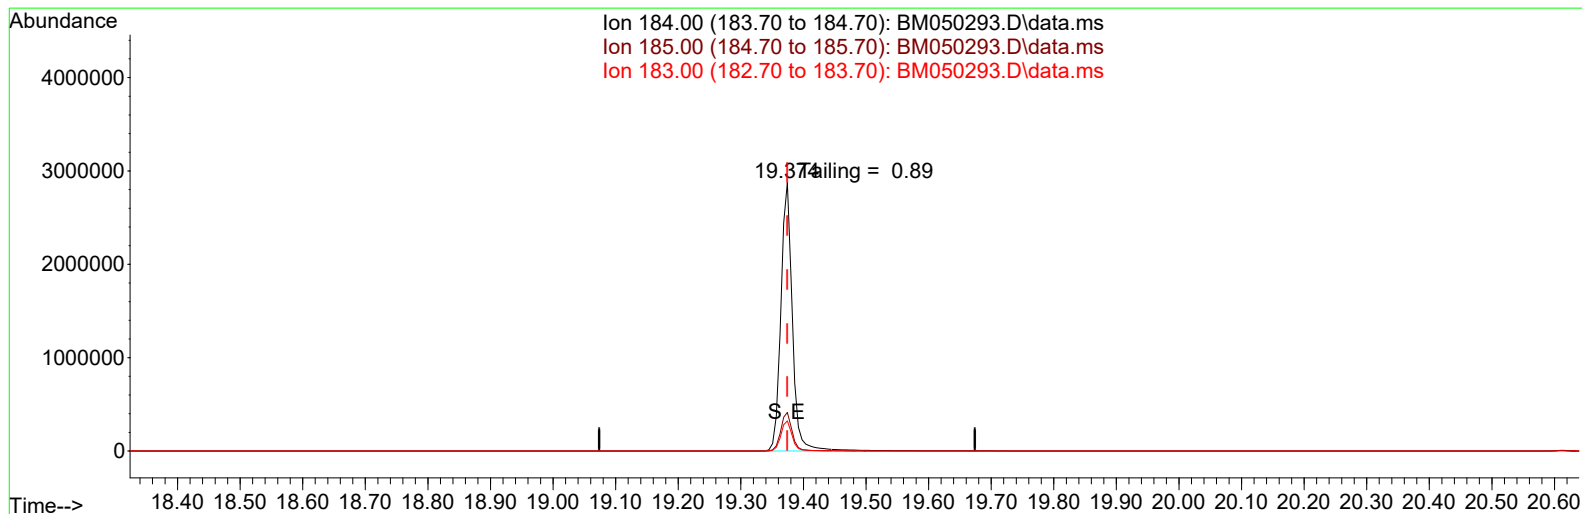

TIC: BM050293.D\data.ms

(77) Benzidine**19.374min (+ 0.000) 81131.91 ng****response 3702866**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.37
183.00	11.20	11.22
0.00	0.00	0.00