

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061215\
 Data File : BM001662.D
 Acq On : 12 Jun 2015 05:27
 Operator : TP/IZ
 Sample : PB83950BS
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jun 12 16:51:40 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SIM-BM061215.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 12 16:27:37 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	21089	5.00	ng	0.00
6) Naphthalene-d8	10.47	136	83880	5.00	ng	0.00
12) Acenaphthene-d10	14.34	164	43187	5.00	ng	0.00
18) Phenanthrene-d10	17.06	188	47459	5.00	ng	0.00
25) Chrysene-d12	21.27	240	80901	5.00	ng	0.00
32) Perylene-d12	23.50	264	64958	5.00	ng	0.00

System Monitoring Compounds

4) 2-Fluorophenol	5.27	112	48717	9.76	ng	0.00
5) Phenol-d6	6.84	99	68457	10.91	ng	0.00
7) Nitrobenzene-d5	8.85	82	44203	6.88	ng	0.00
13) 2,4,6-Tribromophenol	15.83	330	25478	16.20	ng	0.00
14) 2-Fluorobiphenyl	12.96	172	97174	6.44	ng	0.00
27) Terphenyl-d14	19.72	244	82334	6.75	ng	0.00

Target Compounds


						Qvalue
2) 1,4-Dioxane	3.21	88	13834	6.42	ng	96
3) n-Nitrosodimethylamine	3.51	42	26088	7.09	ng	# 99
8) Nitrobenzene	8.89	77	51916	7.47	ng	98
9) Naphthalene	10.52	128	131950	6.49	ng	99
10) Hexachlorobutadiene	10.80	225	22055	6.53	ng	99
11) 2-Methylnaphthalene	12.15	142	90682	6.92	ng	97
15) Acenaphthylene	14.05	152	153206	7.59	ng	100
16) Acenaphthene	14.40	154	87463	6.81	ng	99
17) Fluorene	15.36	166	100115	7.63	ng	99
19) 4-Bromophenyl-phenylether	16.27	248	37030	7.78	ng	# 87
20) Hexachlorobenzene	16.38	284	38814	8.99	ng	93
21) Pentachlorophenol	16.72	266	173361	98.72	ng	96
23) Anthracene	17.19	178	282417	15.35	ng	# 48
24) Fluoranthene	19.14	202	205566	8.92	ng	100
26) Pyrene	19.50	202	222423	8.01	ng	99
28) Benzo(a)anthracene	21.25	228	197802	7.78	ng	100
29) Chrysene	21.30	228	173234	7.12	ng	99
30) Bis(2-ethylhexyl)phthalate	21.18	149	151659	8.22	ng	99
31) Indeno(1,2,3-cd)pyrene	25.75	276	141193	7.39	ng	99
33) Benzo(b)fluoranthene	22.82	252	164808	7.78	ng	98
34) Benzo(k)fluoranthene	22.88	252	162745	7.91	ng	95
35) Benzo(a)pyrene	23.40	252	148047	8.39	ng	97
36) Dibenzo(a,h)anthracene	25.77	278	112455	7.58	ng	97
37) Benzo(g,h,i)perylene	26.44	276	115912	7.67	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061215\
Data File : BM001662.D
Acq On : 12 Jun 2015 05:27
Operator : TP/IZ
Sample : PB83950BS
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jun 12 16:51:40 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SIM-BM061215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 12 16:27:37 2015
Response via : Initial Calibration

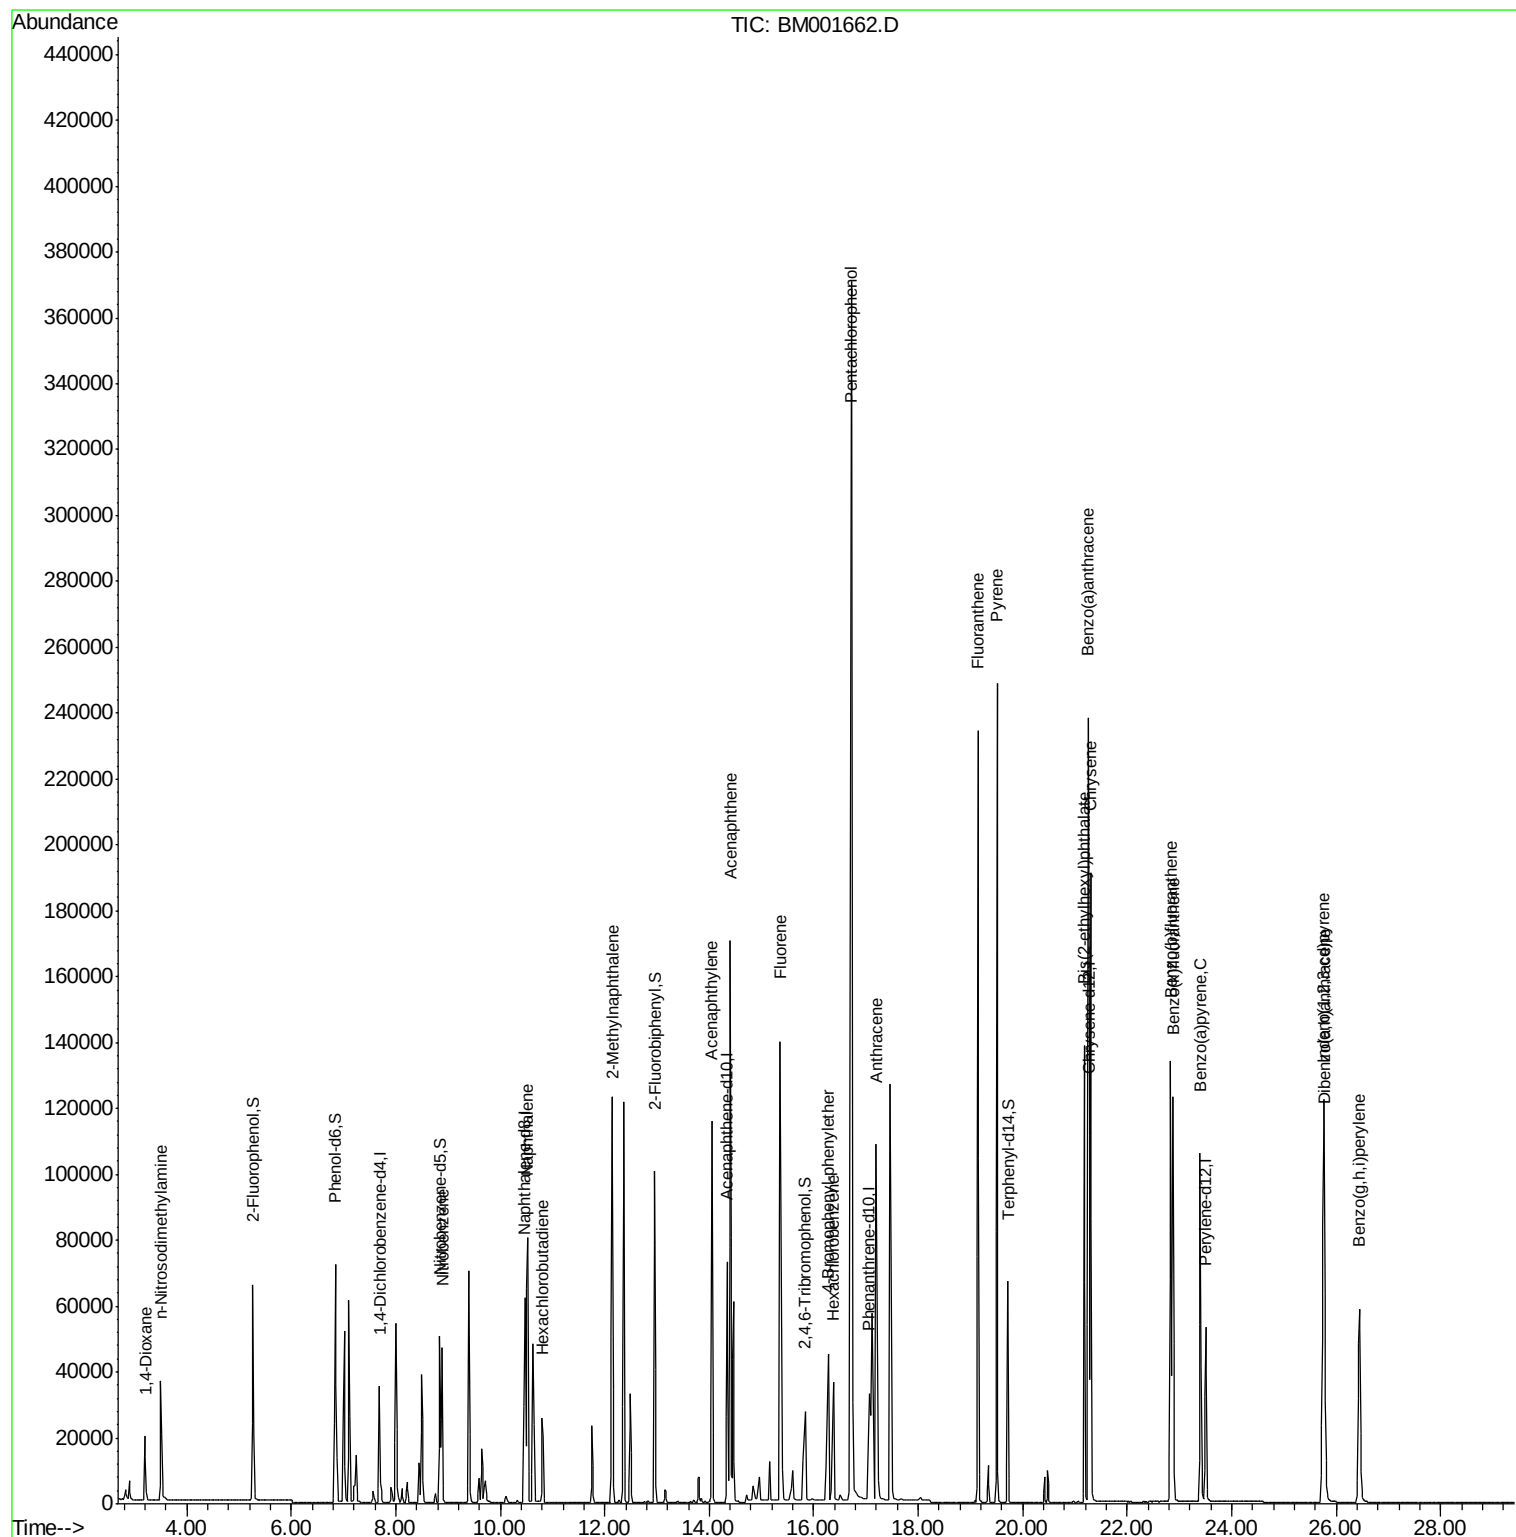




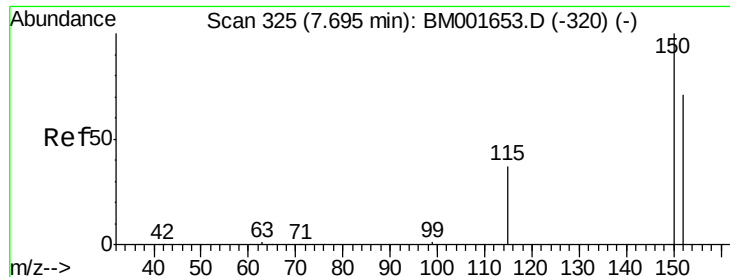


#1

1,4-Dichlorobenzene-d4
Concen: 5.00 ng
RT: 7.70 min Scan# 325
Delta R.T. 0.00 min
Lab File: BM001662.D
Acq: 12 Jun 2015 05:27

Instrument :
BNA_M
ClientSampled :




Tgt Ion:152 Resp: 21089
Ion Ratio Lower Upper
152 100
150 136.8 112.2 168.2
115 49.3 41.7 62.5

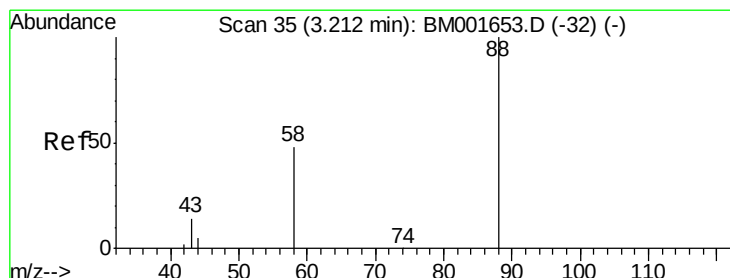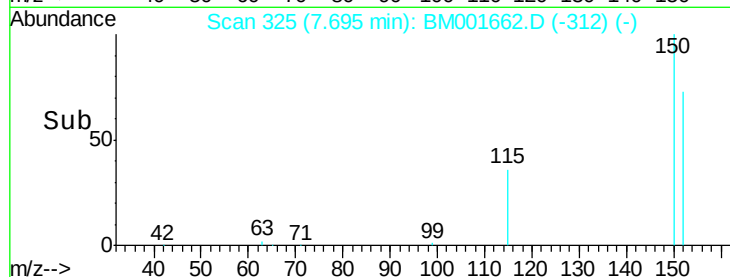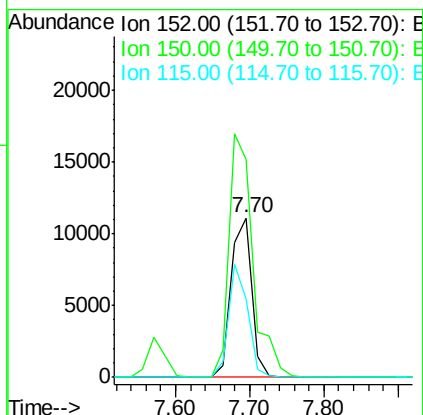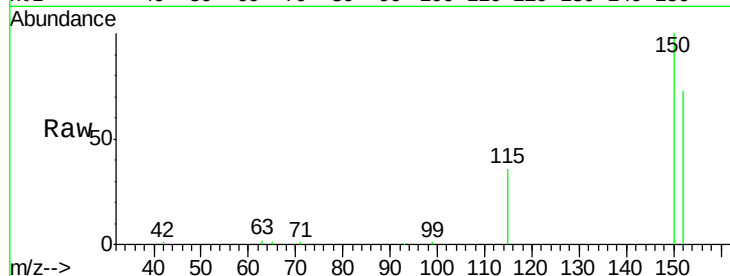


#2

1,4-Dioxane
Concen: 6.42 ng
RT: 3.21 min Scan# 35
Delta R.T. 0.00 min
Lab File: BM001662.D
Acq: 12 Jun 2015 05:27

Tgt Ion: 88 Resp: 13834
Ion Ratio Lower Upper
88 100
58 92.4 70.5 105.7
43 42.8 33.3 49.9

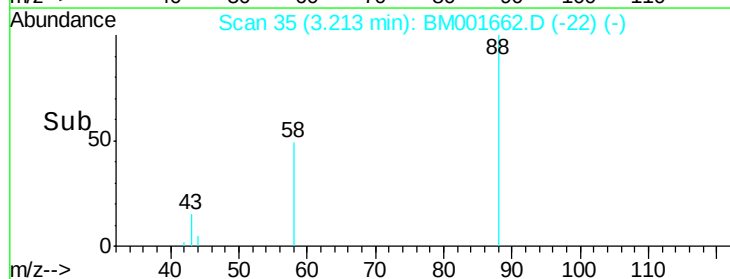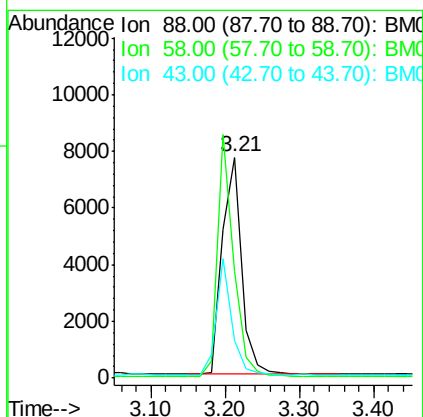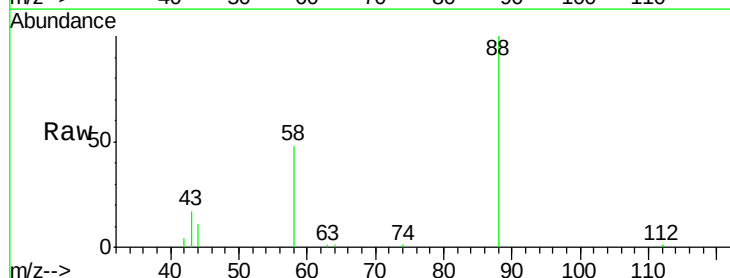

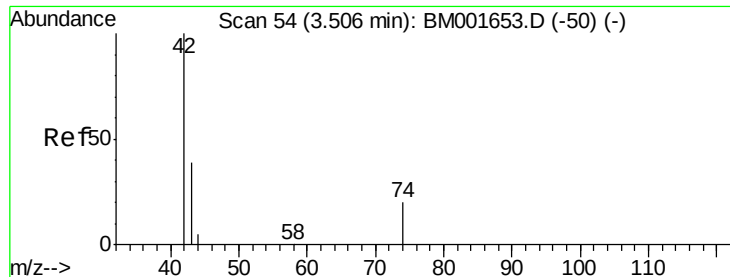

#3

n-Nitrosodimethylamine

Concen: 7.09 ng

RT: 3.51 min Scan# 54

Delta R.T. 0.00 min

Lab File: BM001662.D

Acq: 12 Jun 2015 05:27

Instrument :

BNA_M

ClientSampleId :


Tgt Ion: 42 Resp: 26088

Ion Ratio Lower Upper

42 100

74 94.7 75.7 113.5




44 6.2 6.7 10.1#

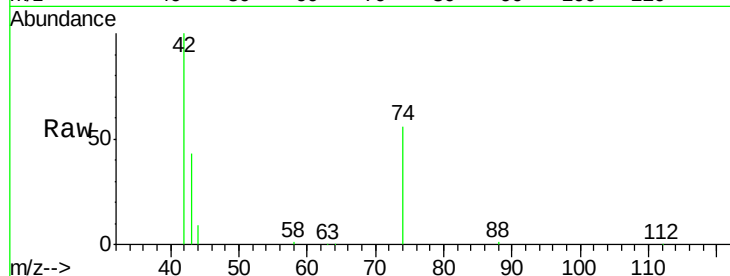

Abundance Ion 42.00 (41.70 to 42.70): BM001653.D (-50) (-)

Ion 74.00 (73.70 to 74.70): BM001653.D (-50) (-)

Ion 44.00 (43.70 to 44.70): BM001653.D (-50) (-)

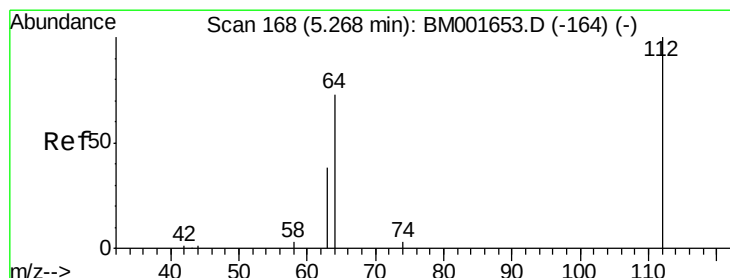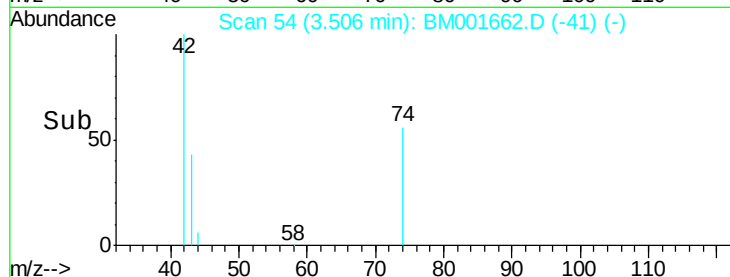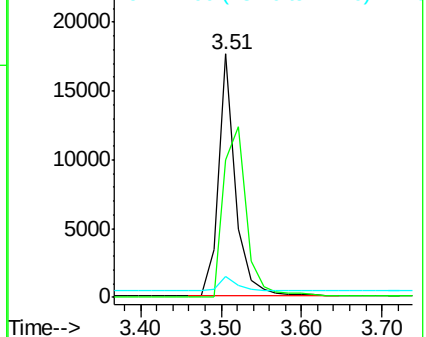

#4

2-Fluorophenol

Concen: 9.76 ng

RT: 5.27 min Scan# 168

Delta R.T. 0.00 min

Lab File: BM001662.D

Acq: 12 Jun 2015 05:27


Tgt Ion: 112 Resp: 48717

Ion Ratio Lower Upper

112 100

64 69.3 55.5 83.3



63 38.3 29.9 44.9

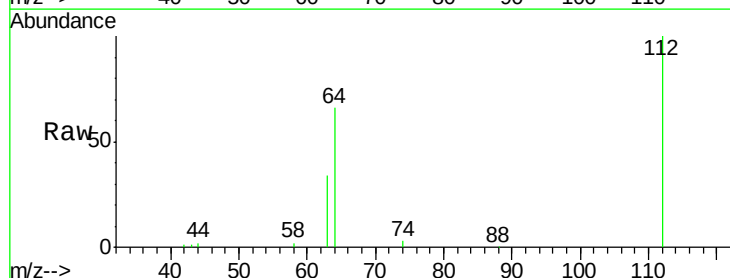


Abundance Ion 112.00 (111.70 to 112.70): BM001653.D (-164) (-)

Ion 64.00 (63.70 to 64.70): BM001653.D (-164) (-)

Ion 63.00 (62.70 to 63.70): BM001653.D (-164) (-)

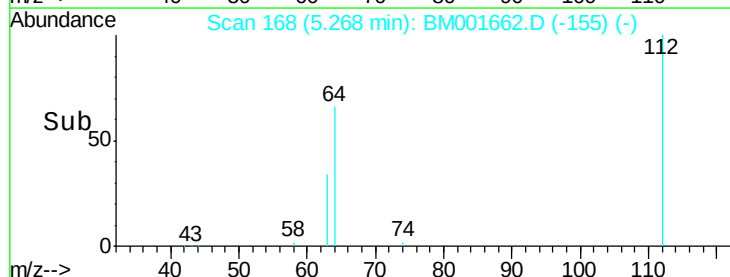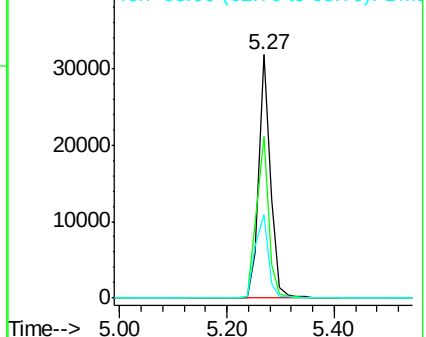

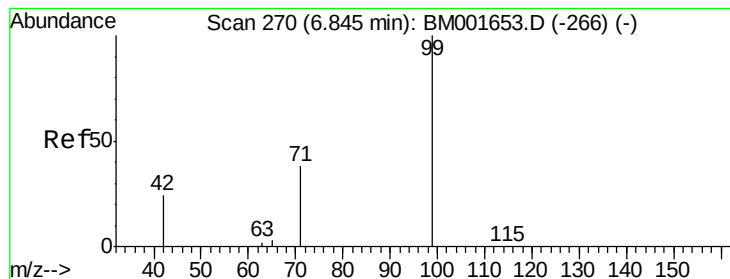

#5

Phenol-d6

Concen: 10.91 ng

RT: 6.84 min Scan# 270

Delta R.T. 0.00 min

Lab File: BM001662.D

Acq: 12 Jun 2015 05:27

Instrument :

BNA_M

ClientSampleId :


Tgt Ion: 99 Resp: 68457

Ion Ratio Lower Upper




99 100

42 27.6 21.6 32.4

71 36.7 28.7 43.1

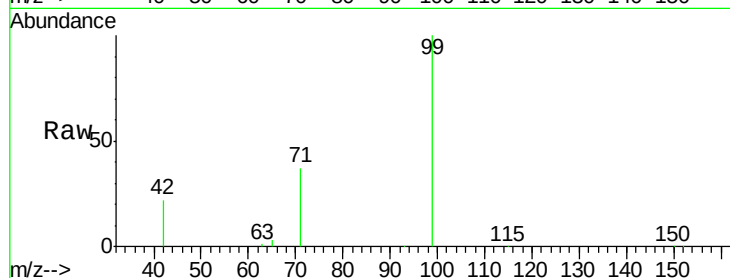

Abundance Ion 99.00 (98.70 to 99.70): BM001662.D (-257) (-)

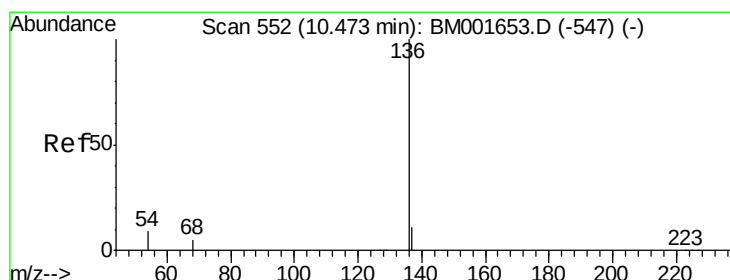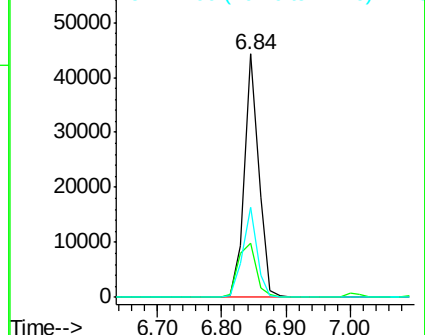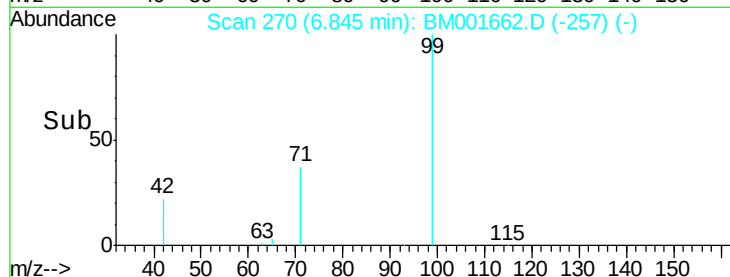

#6

Naphthalene-d8

Concen: 5.00 ng

RT: 10.47 min Scan# 552

Delta R.T. 0.00 min

Lab File: BM001662.D

Acq: 12 Jun 2015 05:27

Tgt Ion: 136 Resp: 83880


Ion Ratio Lower Upper

136 100



137 10.9 8.7 13.1


54 7.8 6.9 10.3

68 5.0 4.4 6.6

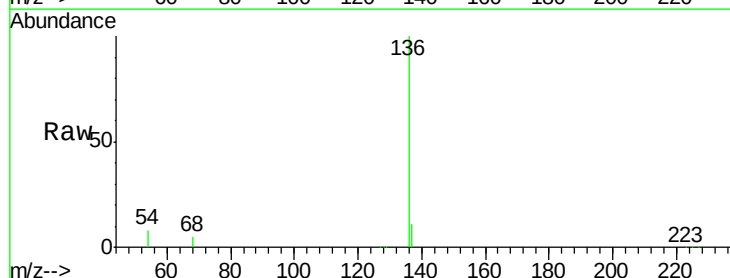

Abundance Ion 136.00 (135.70 to 136.70): BM001662.D (-540) (-)

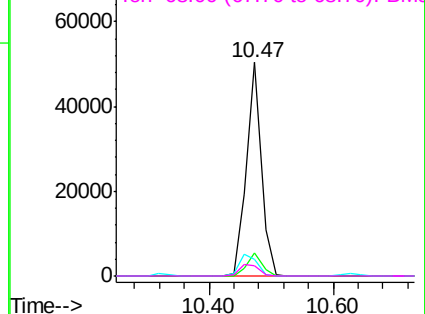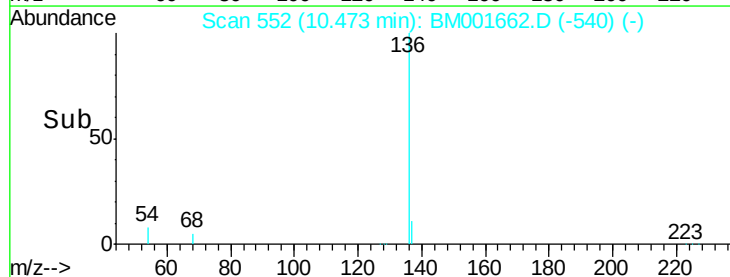



#7

Nitrobenzene-d5

Concen: 6.88 ng

RT: 8.85 min Scan# 421

Delta R.T. 0.00 min


Lab File: BM001662.D

Acq: 12 Jun 2015 05:27

Instrument :

BNA_M

ClientSampleId :






Tgt Ion: 82 Resp: 44203

Ion Ratio Lower Upper

82 100

128 38.9 29.7 44.5

54 52.4 45.1 67.7

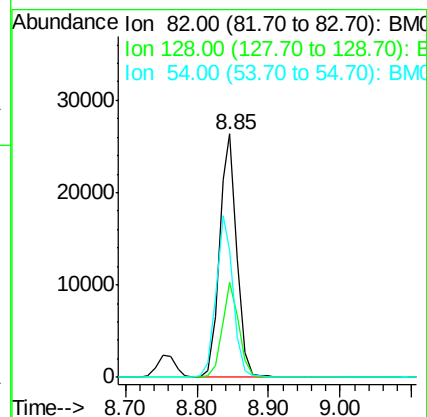

#8

Nitrobenzene

Concen: 7.47 ng

RT: 8.89 min Scan# 425

Delta R.T. 0.00 min

Lab File: BM001662.D

Acq: 12 Jun 2015 05:27




Tgt Ion: 77 Resp: 51916


Ion Ratio Lower Upper

77 100

123 39.0 30.3 45.5

65 14.6 11.2 16.8

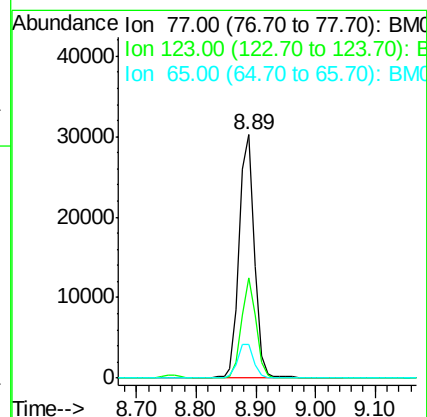



#9

Naphthalene

Concen: 6.49 ng

RT: 10.52 min Scan# 555

Delta R.T. 0.00 min


Lab File: BM001662.D

Acq: 12 Jun 2015 05:27

Instrument :

BNA_M

ClientSampleId :






Tgt Ion:128 Resp: 131950

Ion Ratio Lower Upper

128 100

129 11.7 9.4 14.2

127 11.4 9.7 14.5

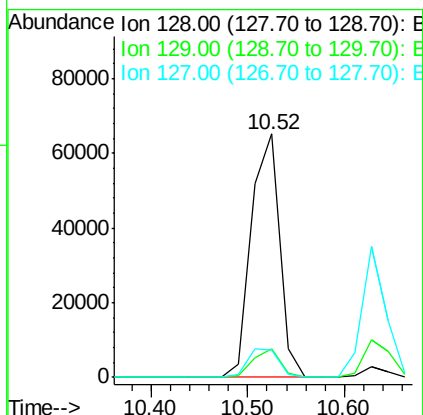

#10

Hexachlorobutadiene

Concen: 6.53 ng

RT: 10.80 min Scan# 571

Delta R.T. 0.00 min

Lab File: BM001662.D

Acq: 12 Jun 2015 05:27




Tgt Ion:225 Resp: 22055


Ion Ratio Lower Upper

225 100

223 63.1 51.0 76.4

227 63.5 51.2 76.8



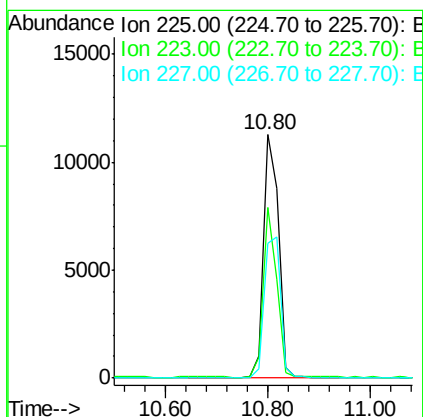



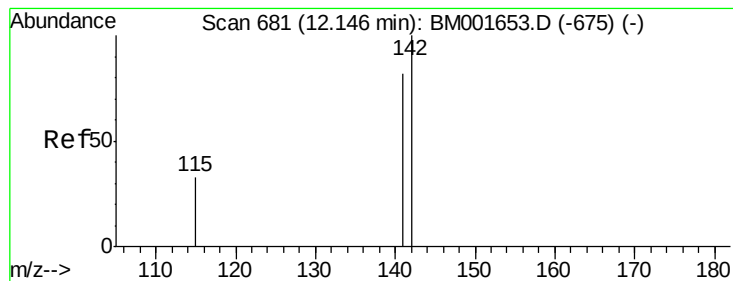

#11
2-Methylnaphthalene
Concen: 6.92 ng
RT: 12.15 min Scan# 681
Delta R.T. 0.00 min
Lab File: BM001662.D
Acq: 12 Jun 2015 05:27




Instrument :
BNA_M
ClientSampleId :


Tgt Ion:142 Resp: 90682
Ion Ratio Lower Upper
142 100
141 79.8 65.8 98.6
115 32.4 27.0 40.6

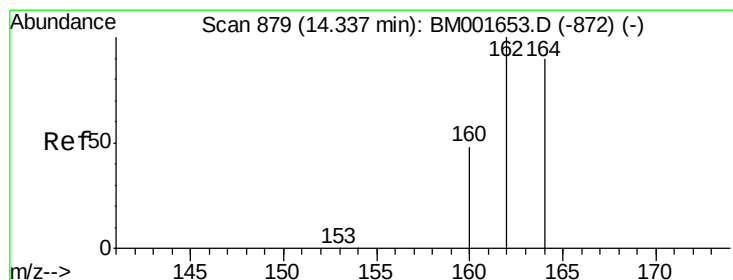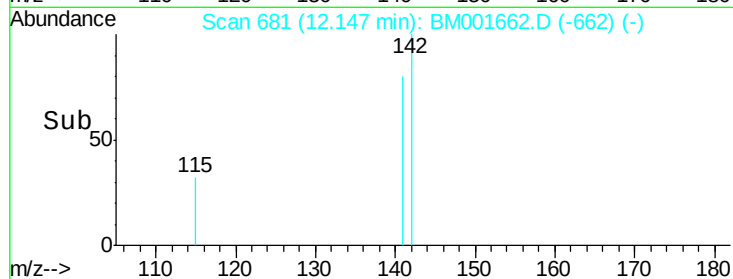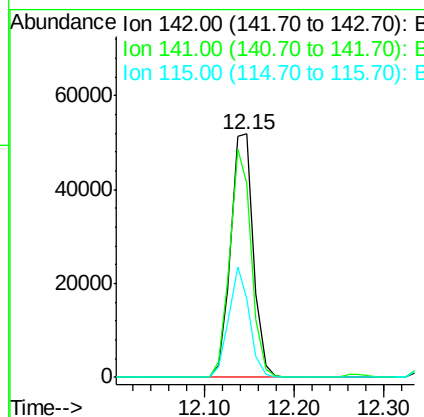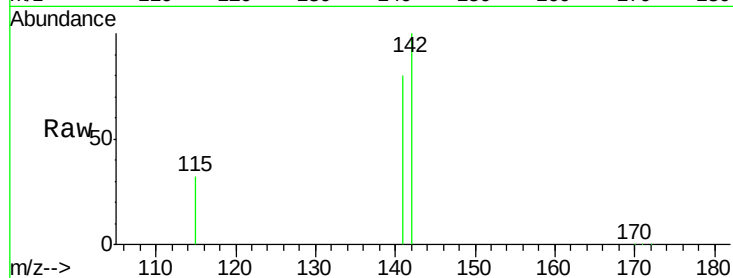

#12
Acenaphthene-d10
Concen: 5.00 ng
RT: 14.34 min Scan# 879
Delta R.T. 0.00 min
Lab File: BM001662.D
Acq: 12 Jun 2015 05:27

Tgt Ion:164 Resp: 43187
Ion Ratio Lower Upper
164 100
162 108.1 89.0 133.4
160 50.3 42.6 63.8

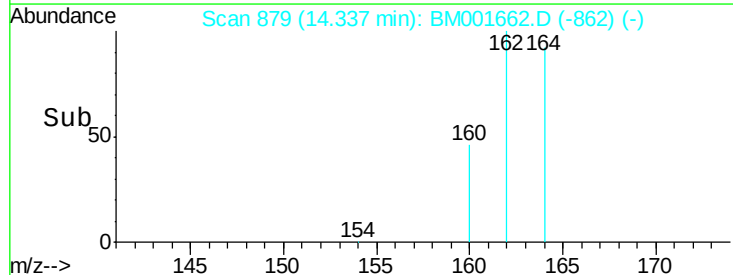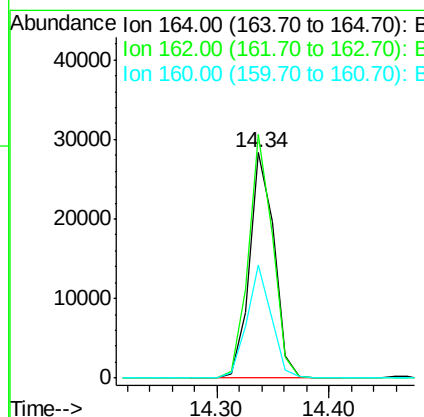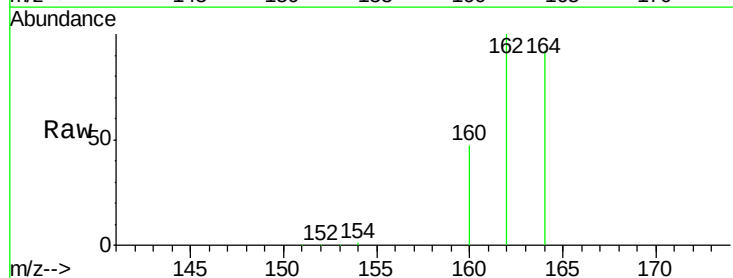







#13
 2,4,6-Tribromophenol
 Concen: 16.20 ng
 RT: 15.83 min Scan# 943
 Delta R.T. 0.00 min
 Lab File: BM001662.D
 Acq: 12 Jun 2015 05:27

Instrument :
 BNA_M
 ClientSampleId :

Tgt Ion:330 Resp: 25478
 Ion Ratio Lower Upper
 330 100
 332 106.2 80.6 120.8
 141 0.0 0.0 0.0

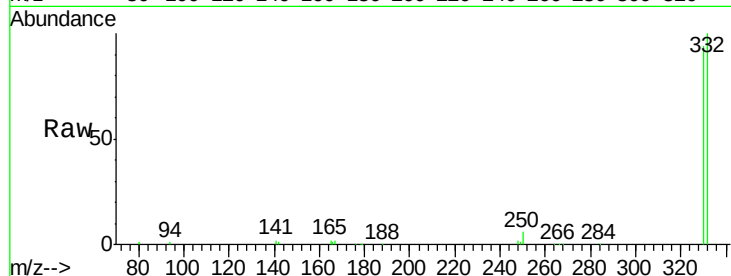


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


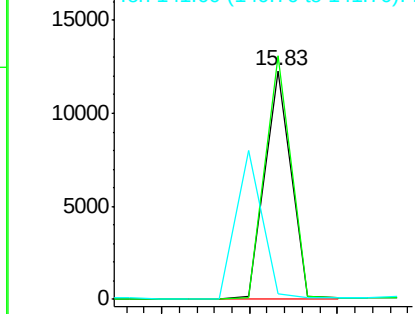



#14
 2-Fluorobiphenyl
 Concen: 6.44 ng
 RT: 12.96 min Scan# 759
 Delta R.T. 0.00 min
 Lab File: BM001662.D
 Acq: 12 Jun 2015 05:27

Tgt Ion:172 Resp: 97174
 Ion Ratio Lower Upper
 172 100
 171 32.6 26.6 40.0
 170 20.6 17.1 25.7



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E




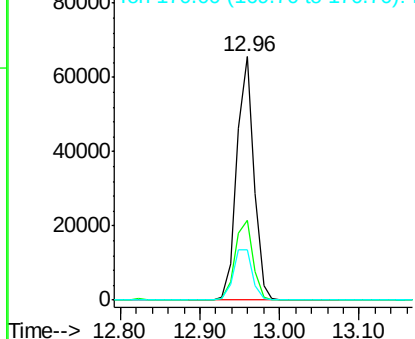




#15
Acenaphthylene
Concen: 7.59 ng
RT: 14.05 min Scan# 855
Delta R.T. -0.01 min
Lab File: BM001662.D
Acq: 12 Jun 2015 05:27




Instrument :
BNA_M
ClientSampleId :


Tgt Ion	Ratio	Lower	Upper
152	100		
151	19.2	15.5	23.3
153	12.9	10.2	15.4

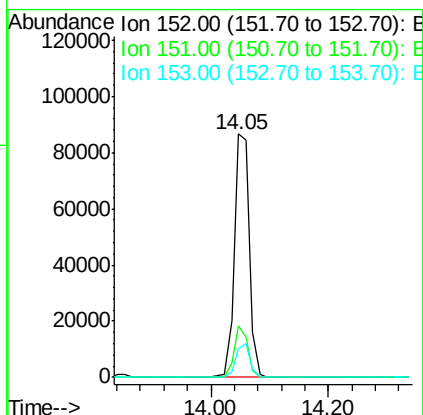

#16
Acenaphthene
Concen: 6.81 ng
RT: 14.40 min Scan# 884
Delta R.T. 0.00 min
Lab File: BM001662.D
Acq: 12 Jun 2015 05:27

Tgt Ion	Ratio	Lower	Upper
154	100		
153	112.2	91.0	136.6
152	54.2	43.8	65.8



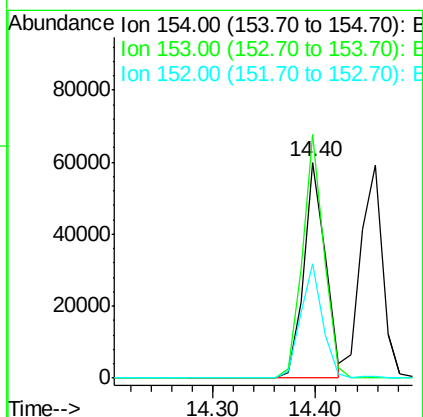





#17
 Fluorene
 Concen: 7.63 ng
 RT: 15.36 min Scan# 929
 Delta R.T. 0.00 min
 Lab File: BM001662.D
 Acq: 12 Jun 2015 05:27




Instrument :
 BNA_M
 ClientSampleId :


Tgt Ion:166 Resp: 100115
 Ion Ratio Lower Upper
 166 100
 165 114.0 90.7 136.1
 167 11.7 9.4 14.0

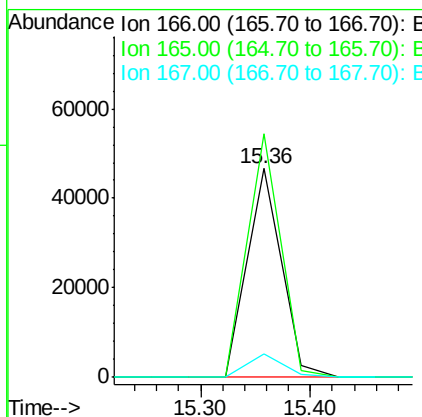

#18
 Phenanthrene-d10
 Concen: 5.00 ng
 RT: 17.06 min Scan# 979
 Delta R.T. 0.00 min
 Lab File: BM001662.D
 Acq: 12 Jun 2015 05:27

Tgt Ion:188 Resp: 47459
 Ion Ratio Lower Upper
 188 100
 94 59.1 48.3 72.5
 80 72.1 58.6 88.0



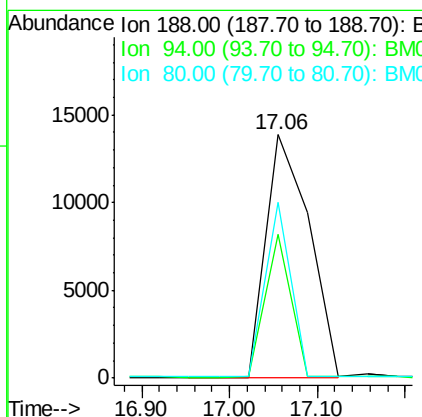





#19
4-Bromophenyl-phenylether
Concen: 7.78 ng
RT: 16.27 min Scan# 956
Delta R.T. 0.00 min
Lab File: BM001662.D
Acq: 12 Jun 2015 05:27




Instrument :
BNA_M
ClientSampleId :


Tgt Ion:248 Resp: 37030
Ion Ratio Lower Upper
248 100
250 122.6 87.5 131.3
141 0.0 0.0 0.0

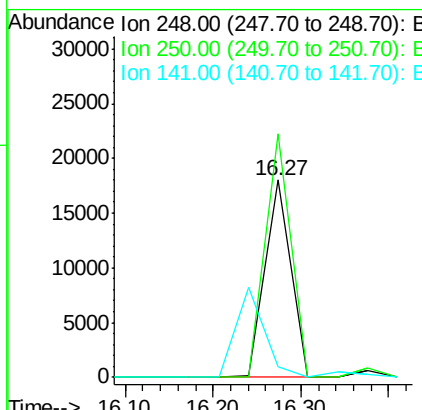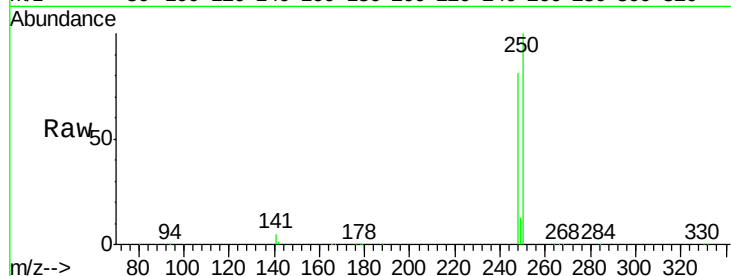

#20
Hexachlorobenzene
Concen: 8.99 ng
RT: 16.38 min Scan# 959
Delta R.T. 0.00 min
Lab File: BM001662.D
Acq: 12 Jun 2015 05:27

Tgt Ion:284 Resp: 38814
Ion Ratio Lower Upper
284 100
142 22.8 21.5 32.3
249 61.3 53.8 80.6

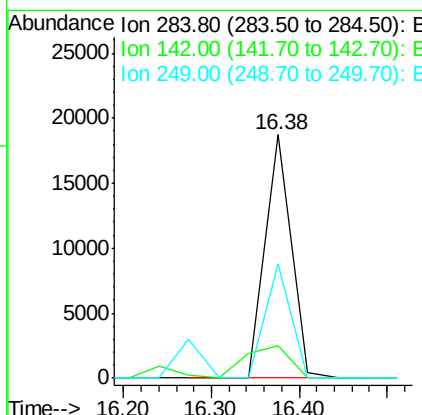

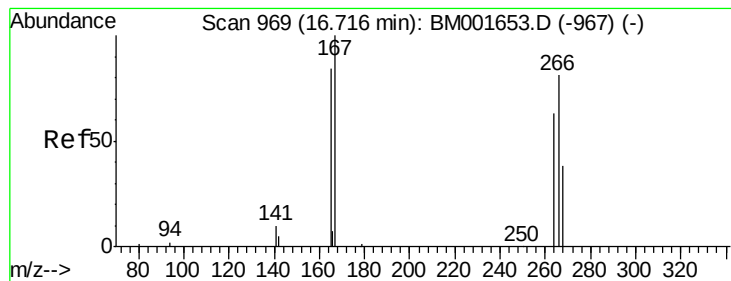

#21

Pentachlorophenol

Concen: 98.72 ng

RT: 16.72 min Scan# 969

Delta R.T. 0.00 min

Lab File: BM001662.D

Acq: 12 Jun 2015 05:27

Instrument :

BNA_M

ClientSampleId :


Tgt Ion:266 Resp: 173361

Ion Ratio Lower Upper

266 100

268 46.9 43.3 64.9




264 80.8 64.5 96.7



Abundance Ion 265.70 (265.40 to 266.40): E

Ion 268.00 (267.70 to 268.70): E

Ion 264.00 (263.70 to 264.70): E

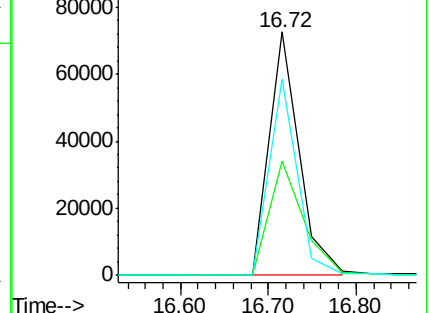

#23

Anthracene

Concen: 15.35 ng

RT: 17.19 min Scan# 983

Delta R.T. 0.00 min

Lab File: BM001662.D

Acq: 12 Jun 2015 05:27


Tgt Ion:178 Resp: 282417

Ion Ratio Lower Upper

178 100

176 19.7 0.0 0.0#



179 0.0 21.4 32.0#




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

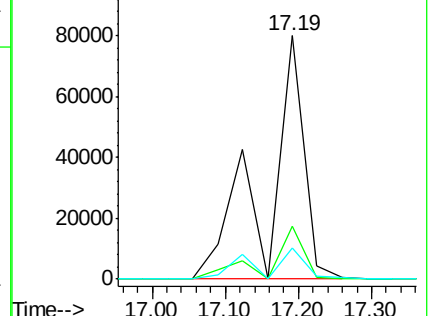



#24

Fluoranthene

Concen: 8.92 ng

RT: 19.14 min Scan# 1088

Delta R.T. 0.00 min

Lab File: BM001662.D

Acq: 12 Jun 2015 05:27

Instrument :

BNA_M

ClientSampleId :


Tgt Ion:202 Resp: 205566

Ion Ratio Lower Upper

202 100

101 13.3 10.8 16.2




203 17.3 13.8 20.8

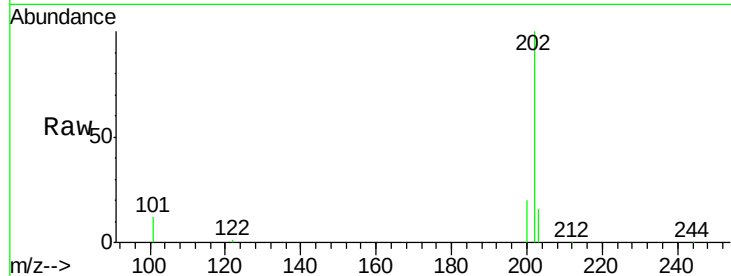

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

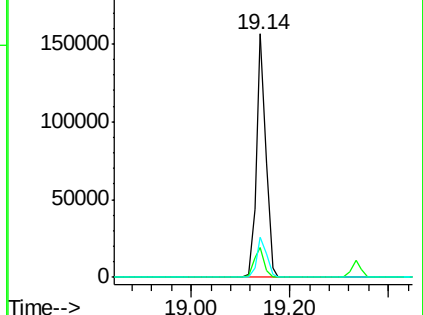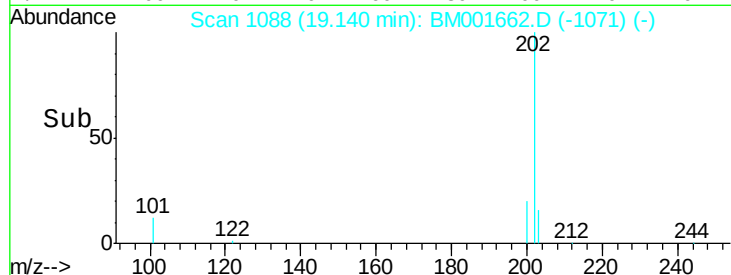

#25

Chrysene-d12

Concen: 5.00 ng

RT: 21.27 min Scan# 1251

Delta R.T. 0.00 min

Lab File: BM001662.D

Acq: 12 Jun 2015 05:27


Tgt Ion:240 Resp: 80901

Ion Ratio Lower Upper

240 100

120 10.6 8.9 13.3



236 29.8 24.6 36.8




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E



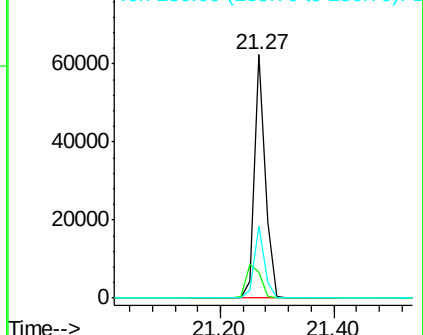





#26
 Pyrene
 Concen: 8.01 ng
 RT: 19.50 min Scan# 1118
 Delta R.T. 0.00 min
 Lab File: BM001662.D
 Acq: 12 Jun 2015 05:27




Instrument :
 BNA_M
 ClientSampleId :


Tgt Ion: 202 Resp: 222423
 Ion Ratio Lower Upper
 202 100
 200 20.7 16.6 24.8
 203 17.8 13.8 20.8

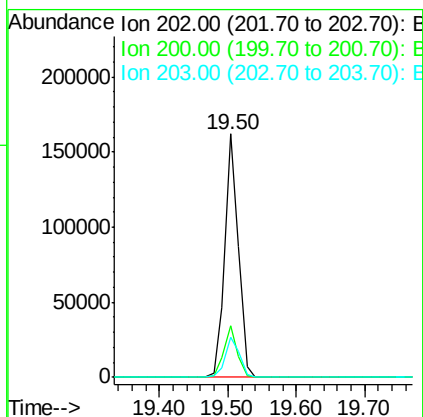

#27
 Terphenyl-d14
 Concen: 6.75 ng
 RT: 19.72 min Scan# 1136
 Delta R.T. 0.00 min
 Lab File: BM001662.D
 Acq: 12 Jun 2015 05:27

Tgt Ion: 244 Resp: 82334
 Ion Ratio Lower Upper
 244 100
 212 9.1 7.7 11.5
 122 7.0 6.9 10.3

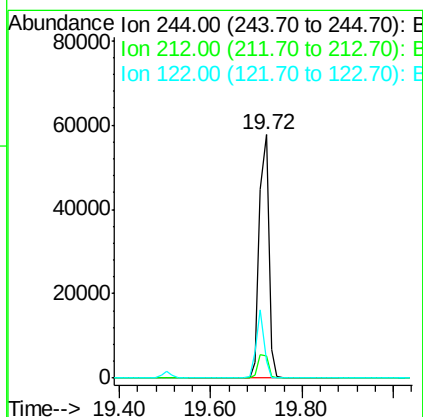



#28

Benzo(a)anthracene

Concen: 7.78 ng

RT: 21.25 min Scan# 1250

Delta R.T. 0.00 min

Lab File: BM001662.D

Acq: 12 Jun 2015 05:27

Instrument :

BNA_M

ClientSampleId :


Tgt Ion:228 Resp: 197802

Ion Ratio Lower Upper




228 100

226 25.2 20.2 30.4

229 20.0 15.7 23.5

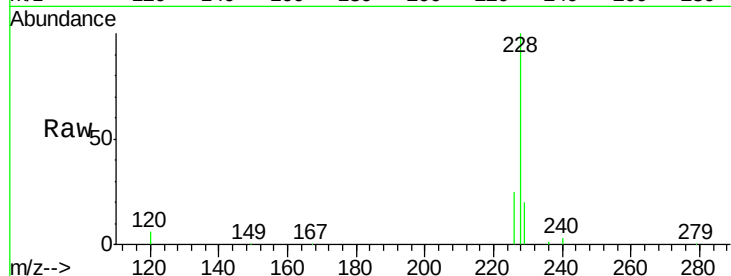

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

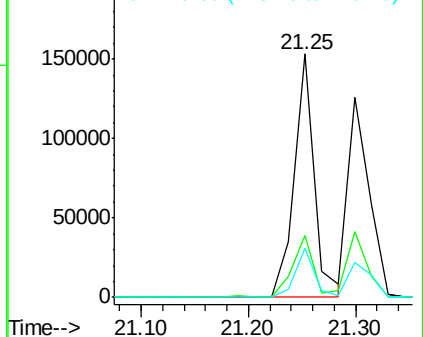

#29

Chrysene

Concen: 7.12 ng

RT: 21.30 min Scan# 1253

Delta R.T. 0.00 min

Lab File: BM001662.D

Acq: 12 Jun 2015 05:27


Tgt Ion:228 Resp: 173234

Ion Ratio Lower Upper



228 100


226 32.8 25.8 38.8

229 17.5 14.1 21.1



Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E




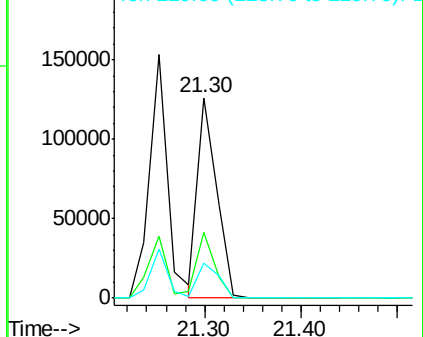




#30
 Bis(2-ethylhexyl)phthalate
 Concen: 8.22 ng
 RT: 21.18 min Scan# 1245
 Delta R.T. 0.00 min
 Lab File: BM001662.D
 Acq: 12 Jun 2015 05:27




Instrument :
 BNA_M
 ClientSampleId :


Tgt Ion:149 Resp: 151659
 Ion Ratio Lower Upper
 149 100
 167 24.8 20.2 30.2
 279 2.2 1.7 2.5

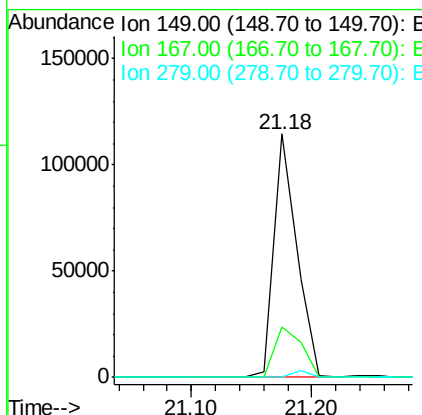

#31
 Indeno(1,2,3-cd)pyrene
 Concen: 7.39 ng
 RT: 25.75 min Scan# 1658
 Delta R.T. 0.00 min
 Lab File: BM001662.D
 Acq: 12 Jun 2015 05:27

Tgt Ion:276 Resp: 141193
 Ion Ratio Lower Upper
 276 100
 138 36.6 28.8 43.2
 277 24.6 19.6 29.4



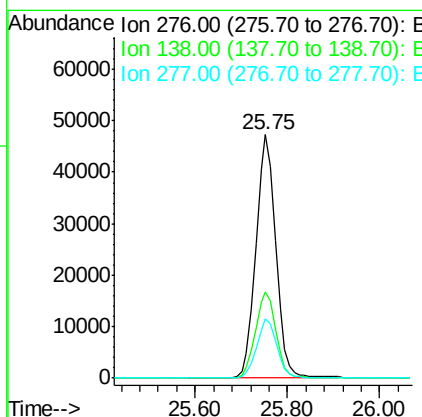



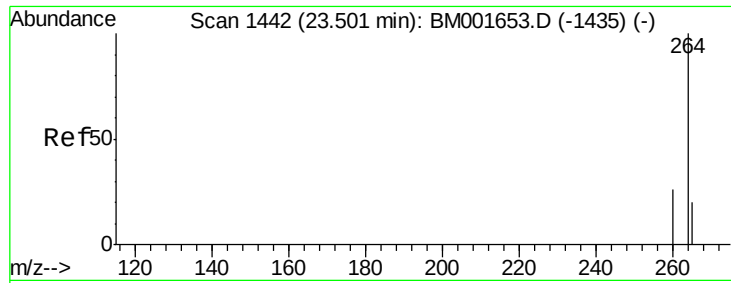

#32
Perylene-d12
Concen: 5.00 ng
RT: 23.50 min Scan# 1442
Delta R.T. 0.00 min
Lab File: BM001662.D
Acq: 12 Jun 2015 05:27




Instrument :
BNA_M
ClientSampleId :


Tgt Ion:264 Resp: 64958
Ion Ratio Lower Upper
264 100
260 26.0 20.8 31.2
265 20.9 16.9 25.3

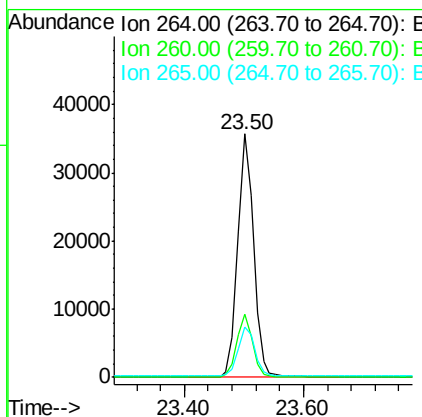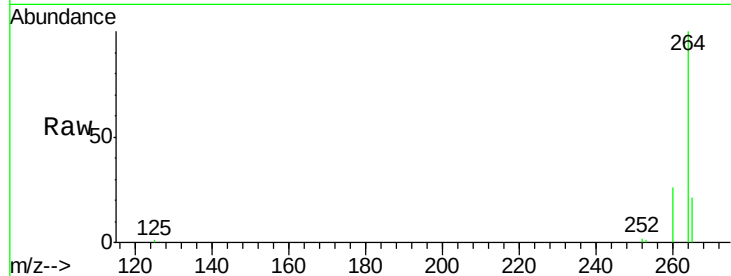

#33
Benzo(b)fluoranthene
Concen: 7.78 ng
RT: 22.82 min Scan# 1377
Delta R.T. 0.00 min
Lab File: BM001662.D
Acq: 12 Jun 2015 05:27

Tgt Ion:252 Resp: 164808
Ion Ratio Lower Upper
252 100
253 20.9 17.4 26.2
125 14.5 12.0 18.0

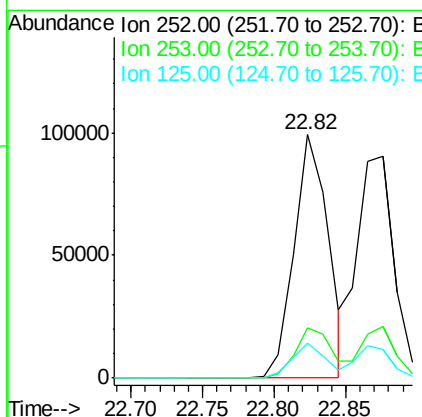



#34

Benzo(k)fluoranthene

Concen: 7.91 ng

RT: 22.88 min Scan# 1382

Delta R.T. 0.01 min


Lab File: BM001662.D

Acq: 12 Jun 2015 05:27



Instrument :

BNA_M

ClientSampleId :

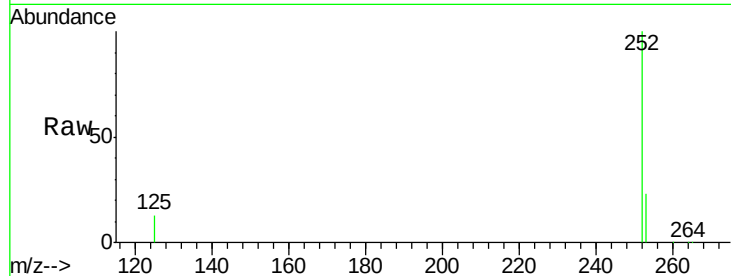

Tgt Ion:	252	Resp:	162745
Ion Ratio	Lower	Upper	
252	100		
253	23.0	17.0	25.6
125	12.9	12.5	18.7

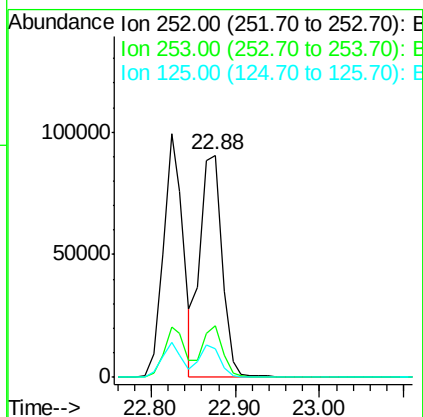

#35

Benzo(a)pyrene

Concen: 8.39 ng




RT: 23.40 min Scan# 1432


Delta R.T. 0.00 min

Lab File: BM001662.D

Acq: 12 Jun 2015 05:27

Tgt Ion:	252	Resp:	148047
Ion Ratio	Lower	Upper	
252	100		
253	20.5	17.4	26.0
125	16.2	14.0	21.0

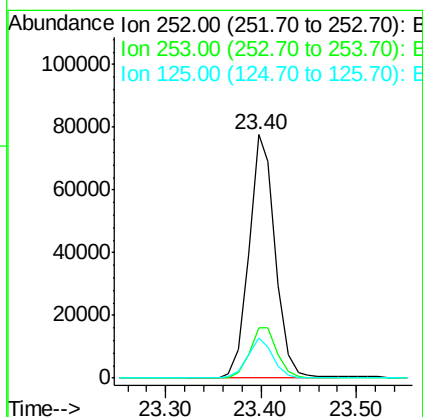







#36
Dibenzo(a,h)anthracene
Concen: 7.58 ng
RT: 25.77 min Scan# 1660
Delta R.T. 0.00 min
Lab File: BM001662.D
Acq: 12 Jun 2015 05:27

Instrument :
BNA_M
ClientSampled :

Tgt Ion: 278 Resp: 112455

Ion	Ratio	Lower	Upper
278	100		
139	21.4	19.1	28.7
279	23.9	19.7	29.5

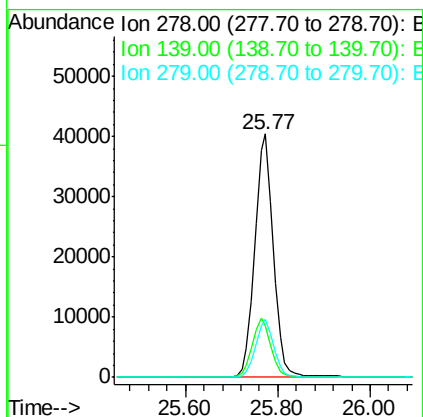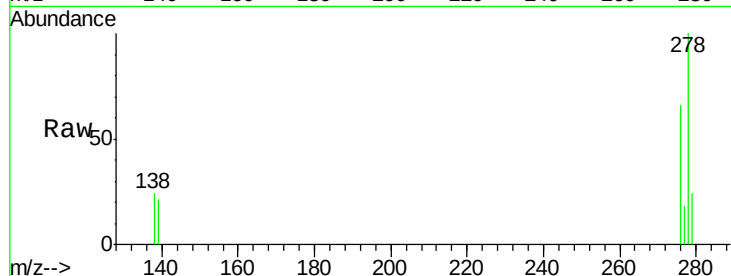

#37
Benzo(g,h,i)perylene
Concen: 7.67 ng
RT: 26.44 min Scan# 1724
Delta R.T. 0.00 min
Lab File: BM001662.D
Acq: 12 Jun 2015 05:27

Tgt Ion: 276 Resp: 115912

Ion	Ratio	Lower	Upper
276	100		
277	23.3	19.3	28.9
138	31.4	25.0	37.4

