


Data Path : Z:\HPCHEM1\BNA\_M\DATA\BM061215\  
 Data File : BM001649.D  
 Acq On : 11 Jun 2015 19:45  
 Operator : TP/IZ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_M\METHODS\8270-BM031115.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Sat Mar 28 05:37:34 2015

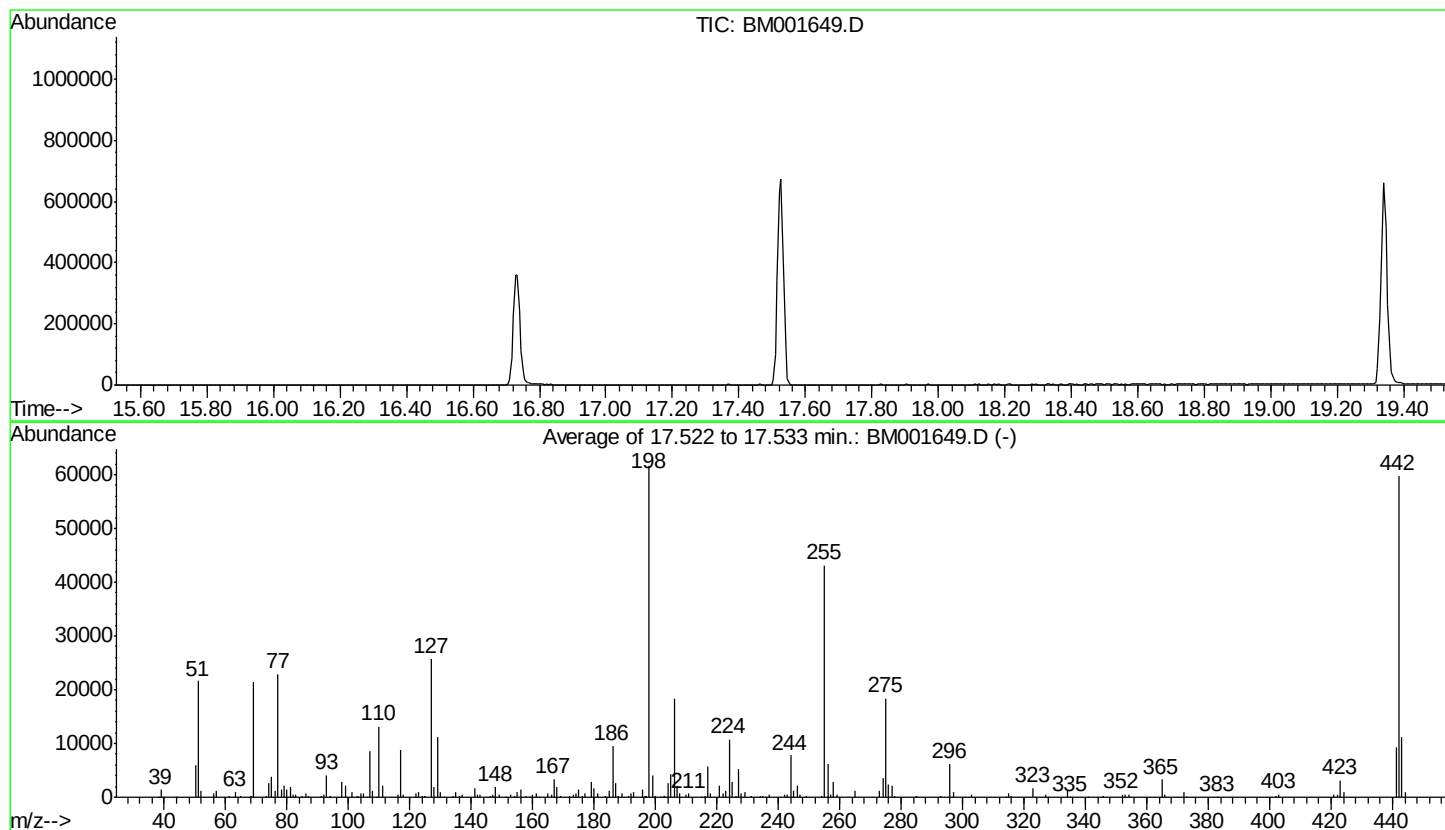

AutoFind: Scans 2522, 2523, 2524; Background Corrected with Scan 2515

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 35.1      | 21662   | PASS             |
| 68          | 69           | 0.00         | 2            | 0.7       | 144     | PASS             |
| 69          | 198          | 0.00         | 100          | 34.8      | 21469   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 127         | 198          | 10           | 80           | 41.8      | 25770   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.5       | 311     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 61685   | PASS             |
| 199         | 198          | 5            | 9            | 6.7       | 4142    | PASS             |
| 275         | 198          | 10           | 60           | 29.8      | 18373   | PASS             |
| 365         | 198          | 1            | 100          | 5.2       | 3230    | PASS             |
| 441         | 442          | 0.01         | 24           | 15.4      | 9222    | PASS             |
| 442         | 198          | 50           | 100          | 97.1      | 59872   | PASS             |
| 443         | 442          | 15           | 24           | 18.6      | 11120   | PASS             |