


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061215\
 Data File : BM001659.D
 Acq On : 12 Jun 2015 02:25
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM031115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Mar 28 05:37:34 2015

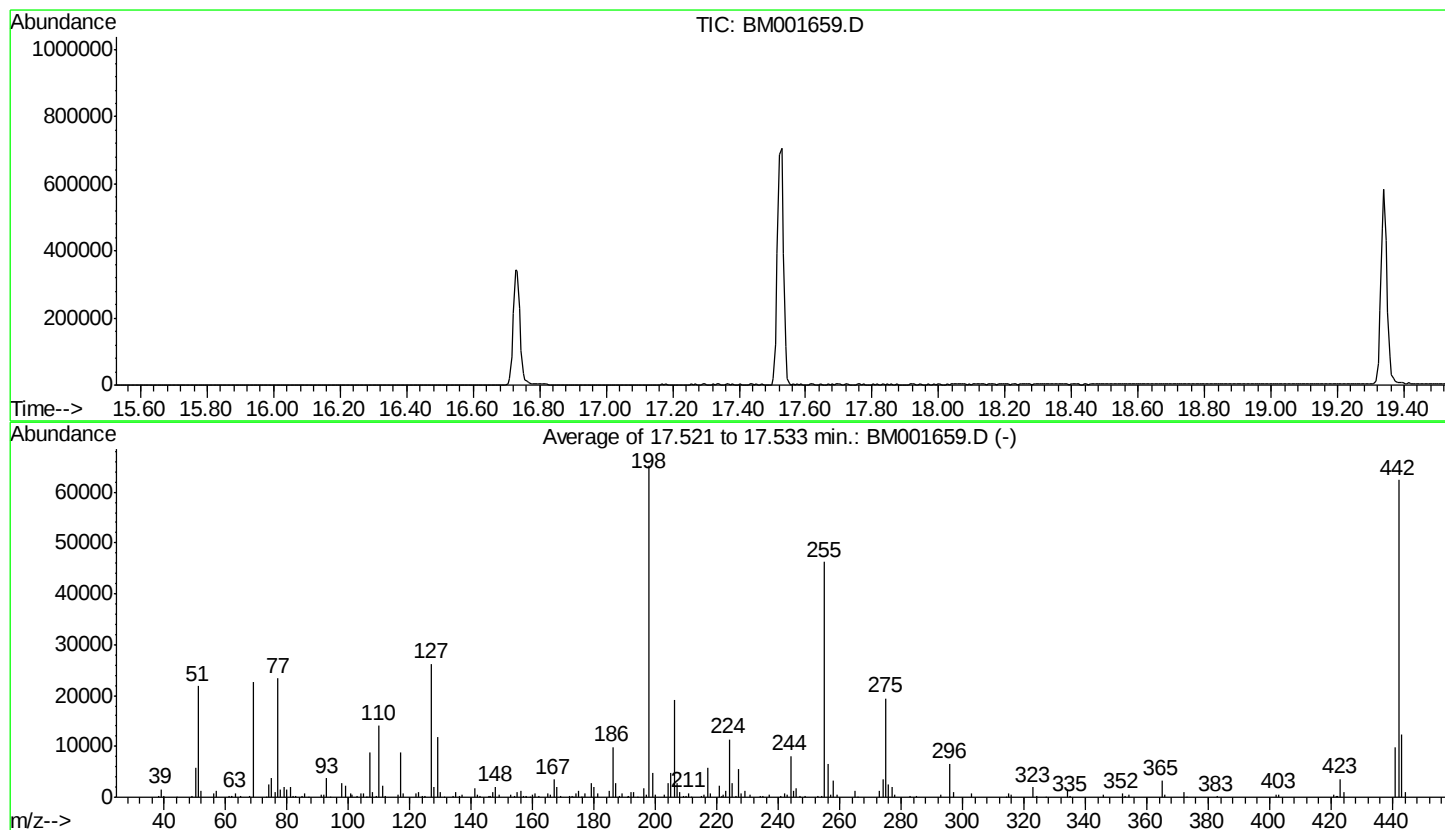

AutoFind: Scans 2522, 2523, 2524; Background Corrected with Scan 2516

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.5	21843	PASS
68	69	0.00	2	1.5	341	PASS
69	198	0.00	100	34.9	22771	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.2	26229	PASS
197	198	0.00	2	0.9	567	PASS
198	198	100	100	100.0	65202	PASS
199	198	5	9	7.3	4762	PASS
275	198	10	60	29.7	19391	PASS
365	198	1	100	4.9	3164	PASS
441	442	0.01	24	15.6	9743	PASS
442	198	50	100	95.7	62373	PASS
443	442	15	24	19.8	12347	PASS