

Data File : BM010530.D
Acq On : 12 Jun 2017 12:06
Operator : SJ/MA
Sample : PB99650BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Jun 13 02:16:29 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 13 02:16:10 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.89	152	97256	20.00	ng/ul	0.00
18) Naphthalene-d8	10.69	136	338298	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.53	164	243914	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.27	188	645163	20.00	ng/ul	0.00
75) Chrysene-d12	21.44	240	978262	20.00	ng/ul	0.00
83) Perylene-d12	23.77	264	1083585	20.00	ng/ul	0.00

System Monitoring Compounds


3) 1,4-Dioxane-d8	3.36	96	16317	6.88	ng/uL	0.00
5) Phenol-d5	7.07	99	200703	27.23	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.23	67	115847	27.97	ng/ul	0.00
9) 2-Chlorophenol-d4	7.43	132	177637	30.24	ng/ul	0.00
13) 4-Methylphenol-d8	8.61	113	171382	28.82	ng/ul	0.00
19) Nitrobenzene-d5	9.07	128	85176	34.37	ng/ul	0.00
22) 2-Nitrophenol-d4	9.79	143	99132	34.53	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.32	165	212044	35.96	ng/ul	0.00
29) 4-Chloroaniline-d4	10.86	131	216451	38.04	ng/ul	0.00
43) Dimethylphthalate-d6	13.94	166	763385	37.67	ng/ul	0.00
46) Acenaphthylene-d8	14.23	160	815878	34.51	ng/ul	0.00
51) 4-Nitrophenol-d4	14.77	143	84203	27.77	ng/ul	0.00
57) Fluorene-d10	15.52	176	652195	36.61	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.64	200	134139	29.35	ng/ul	0.00
70) Anthracene-d10	17.37	188	1151636	36.68	ng/ul	0.00
76) Pyrene-d10	19.66	212	1447615	35.79	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.63	264	1779502	35.27	ng/ul	0.00


Target Compounds					Qvalue
15) N-Nitroso-di-n-propylamine	8.61	70	7793	1.61 ng/ul#	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM010530.D
Acq On : 12 Jun 2017 12:06
Operator : SJ/MA
Sample : PB99650BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Jun 13 02:16:29 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 13 02:16:10 2017
Response via : Initial Calibration

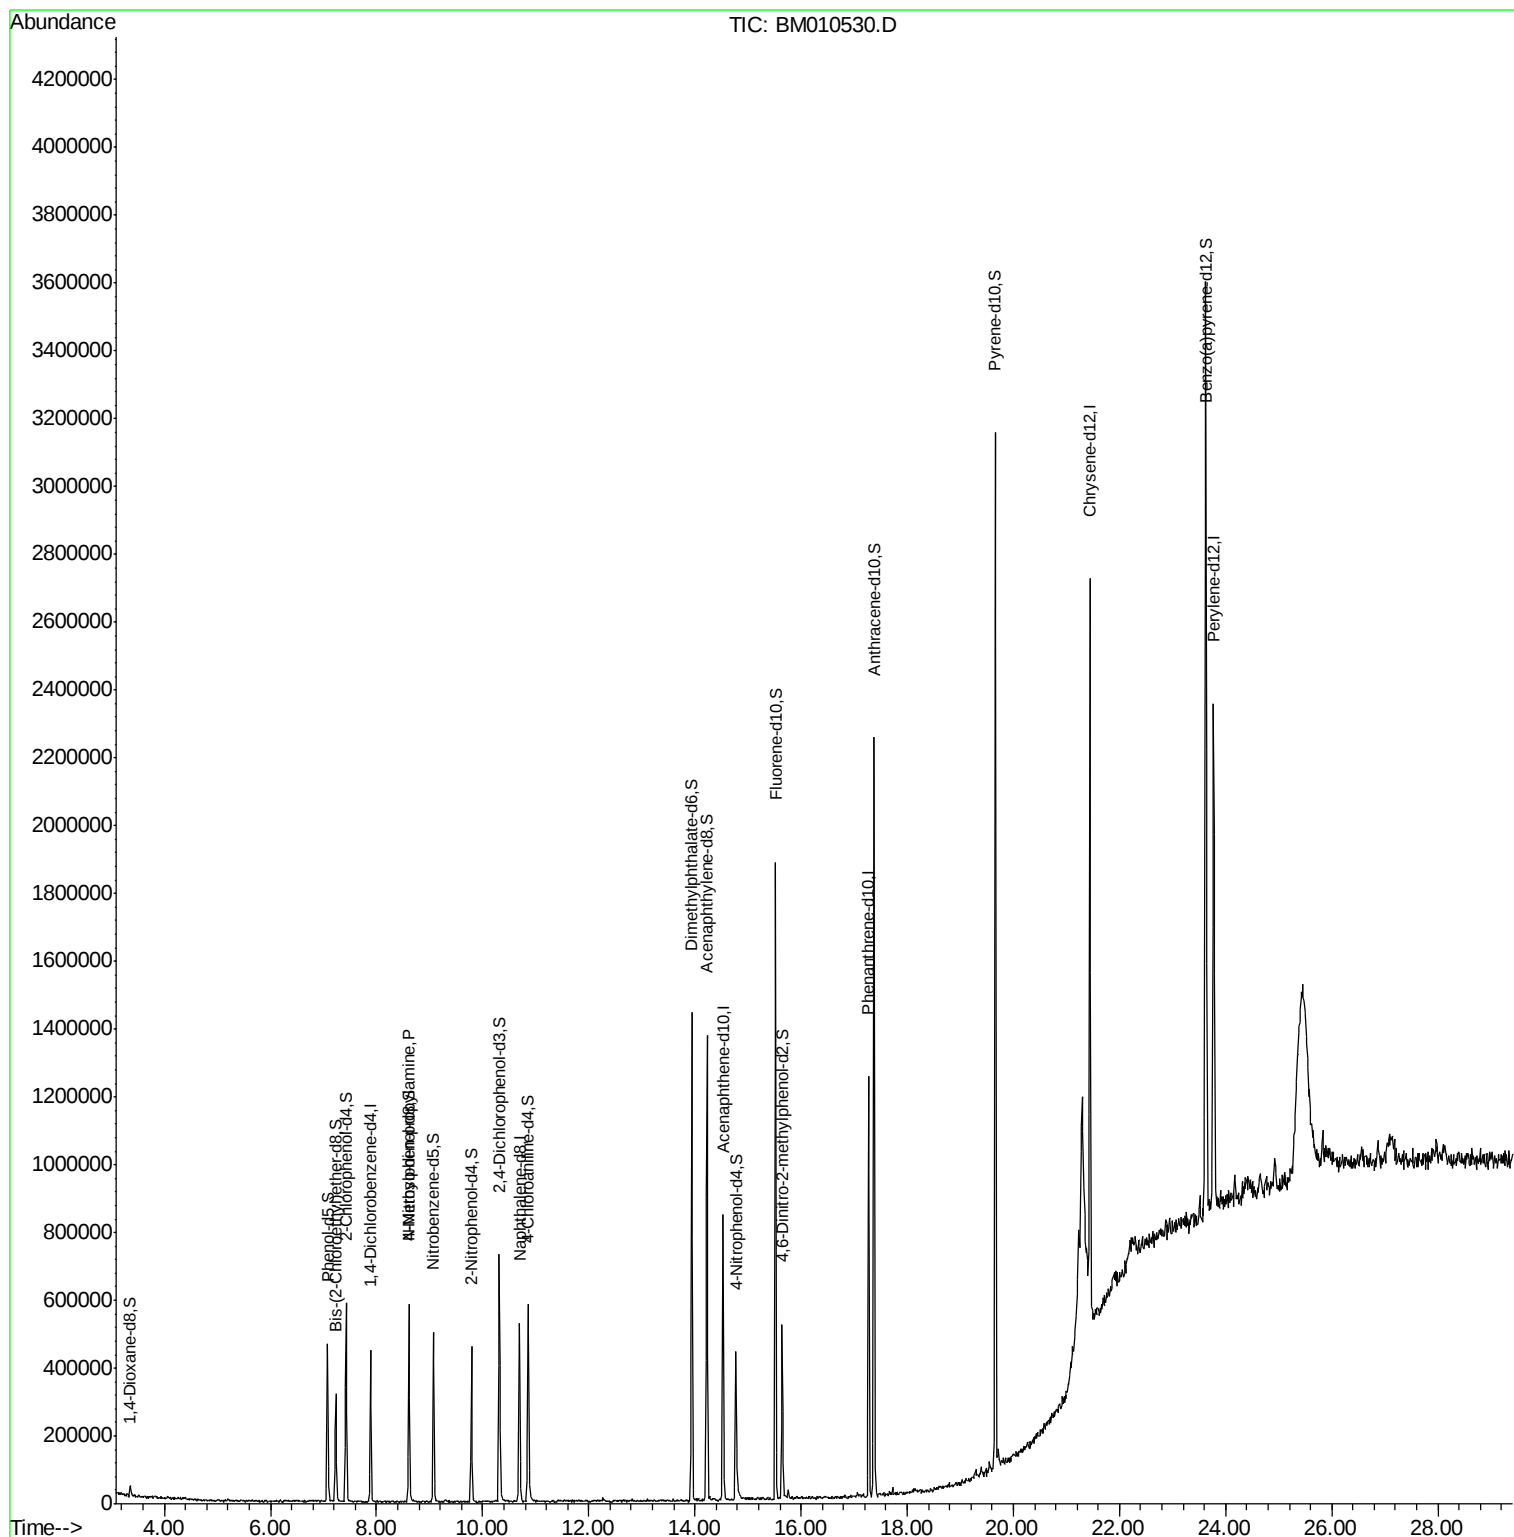

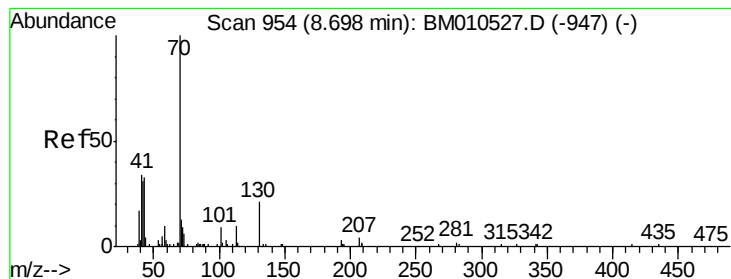

#15

N-Nitroso-di-n-propylamine

Concen: 1.61 ng/ul

RT: 8.61 min Scan# 939

Delta R.T. -0.09 min

Lab File: BM010530.D

Acq: 12 Jun 2017 12:06

Tgt Ion: 70 Resp: 7793



Ion Ratio Lower Upper

70 100

42 193.9 41.1 61.7#

101 0.0 6.7 10.1#

130 0.0 14.6 22.0#

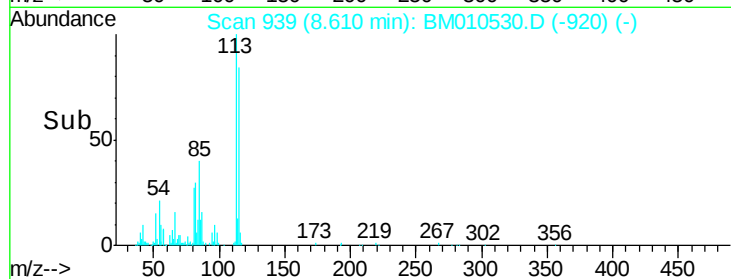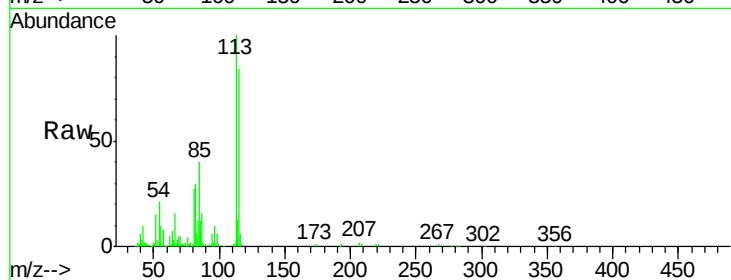

Abundance Ion 70.00 (69.70 to 70.70): BM0

Ion 42.00 (41.70 to 42.70): BM0

Ion 101.00 (100.70 to 101.70): E

Ion 130.00 (129.70 to 130.70): E

