

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061217\
 Data File : BM010528.D
 Acq On : 12 Jun 2017 10:20
 Operator : SJ/MA
 Sample : PB99659BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK59

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	7.075	670	678	694	rBV	530653	846952	18.78%	2.042%
2	7.234	698	705	717	rBV	355450	571491	12.67%	1.378%
3	7.428	730	738	747	rBV	628964	1000985	22.20%	2.414%
4	7.886	809	816	824	rBV	615520	983858	21.82%	2.372%
5	8.610	933	939	949	rBV2	699204	1105031	24.51%	2.665%
6	9.075	1009	1018	1027	rBV	555991	916898	20.33%	2.211%
7	9.786	1130	1139	1148	rBV2	535815	888071	19.69%	2.141%
8	10.316	1222	1229	1240	rBV	820399	1409042	31.25%	3.398%
9	10.692	1283	1293	1303	rVB	733364	1248599	27.69%	3.011%
10	10.857	1313	1321	1331	rBV	688626	1196720	26.54%	2.886%
11	13.939	1840	1845	1854	rVB	1690801	2381027	52.80%	5.742%
12	14.227	1887	1894	1901	rBV	1642225	2365184	52.45%	5.703%
13	14.527	1938	1945	1955	rVB2	1168615	1777110	39.41%	4.285%
14	14.768	1980	1986	1998	rBV	496374	902284	20.01%	2.176%
15	15.515	2107	2113	2121	rBV	2161925	3107765	68.92%	7.494%
16	15.645	2129	2135	2145	rBV	586271	858014	19.03%	2.069%
17	15.751	2149	2153	2159	rVB5	30592	46026	1.02%	0.111%
18	17.274	2404	2412	2420	rBV	1603316	2232043	49.50%	5.382%
19	17.374	2422	2429	2441	rVB	2587265	3559805	78.94%	8.584%
20	19.550	2796	2799	2805	rVB8	39673	46376	1.03%	0.112%
21	19.662	2812	2818	2824	rBV	3173188	4081793	90.52%	9.843%
22	21.438	3116	3120	3127	rBV	2278561	2694963	59.77%	6.499%
23	23.627	3485	3492	3499	rBV	2428340	4509238	100.00%	10.874%
24	23.774	3511	3517	3525	rVB2	1401712	2740400	60.77%	6.608%


Sum of corrected areas: 41469675

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061217\
Data File : BM010528.D
Acq On : 12 Jun 2017 10:20
Operator : SJ/MA
Sample : PB99659BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
SBLK59

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

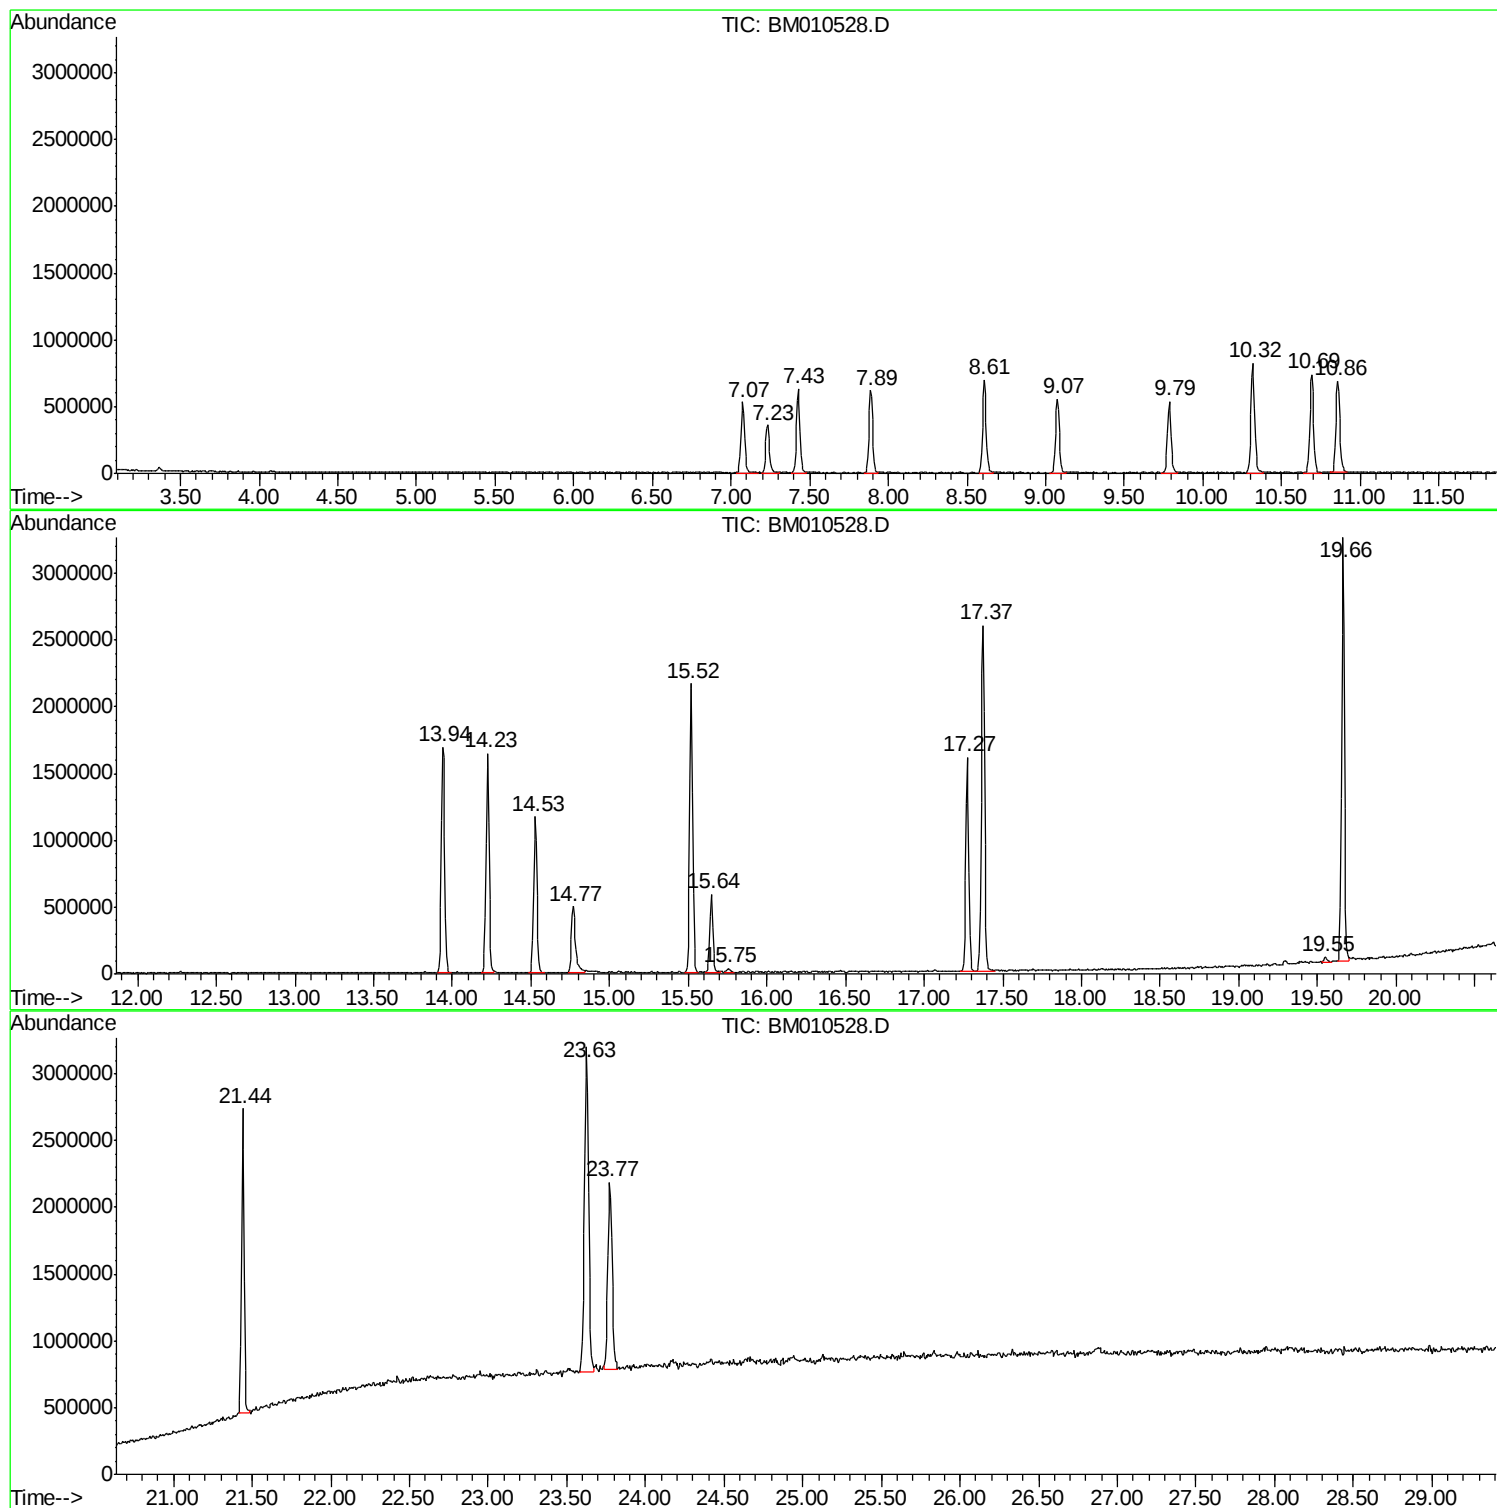

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061217\
Data File : BM010528.D
Acq On : 12 Jun 2017 10:20
Operator : SJ/MA
Sample : PB99659BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK59

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061217\
Data File : BM010528.D
Acq On : 12 Jun 2017 10:20
Operator : SJ/MA
Sample : PB99659BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK59

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc