

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061217\
 Data File : BM010530.D
 Acq On : 12 Jun 2017 12:06
 Operator : SJ/MA
 Sample : PB99650BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK50

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	42	46	53	rBV2	31670	55011	1.08%	0.145%
2	7.075	672	678	687	rBV	463657	734204	14.36%	1.931%
3	7.234	699	705	711	rBV	317263	492858	9.64%	1.296%
4	7.428	732	738	746	rBV	584424	905256	17.71%	2.381%
5	7.887	810	816	825	rVB	447746	717251	14.03%	1.887%
6	8.610	931	939	951	rBV2	584320	963451	18.84%	2.534%
7	9.075	1011	1018	1026	rVB	499884	796642	15.58%	2.095%
8	9.787	1133	1139	1147	rBV2	461158	763716	14.94%	2.009%
9	10.316	1221	1229	1241	rBV	730783	1239928	24.25%	3.261%
10	10.692	1286	1293	1302	rBV	528060	897312	17.55%	2.360%
11	10.857	1314	1321	1331	rBV	579526	1026993	20.09%	2.701%
12	13.939	1838	1845	1856	rBV	1442030	1985674	38.84%	5.223%
13	14.227	1886	1894	1901	rBV	1371507	2045332	40.00%	5.380%
14	14.527	1938	1945	1953	rVB2	841601	1291336	25.26%	3.397%
15	14.769	1980	1986	1997	rBV	435838	812210	15.89%	2.136%
16	15.516	2107	2113	2120	rBV	1880905	2681758	52.45%	7.054%
17	15.645	2129	2135	2142	rBV	513521	747947	14.63%	1.967%
18	17.274	2406	2412	2421	rVB2	1242227	1766965	34.56%	4.648%
19	17.374	2421	2429	2440	rVB2	2242409	3224446	63.07%	8.481%
20	19.392	2770	2772	2780	rVB9	29730	53281	1.04%	0.140%
21	19.662	2812	2818	2823	rBV	3052632	3944540	77.15%	10.375%
22	21.221	3080	3083	3084	rBV	186815	188321	3.68%	0.495%
23	21.439	3116	3120	3126	rVB	2176884	2739707	53.58%	7.206%
24	23.627	3485	3492	3500	rBV2	2743814	5112870	100.00%	13.448%
25	23.774	3512	3517	3526	rVB	1480442	2831852	55.39%	7.449%


Sum of corrected areas: 38018861

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061217\
Data File : BM010530.D
Acq On : 12 Jun 2017 12:06
Operator : SJ/MA
Sample : PB99650BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK50

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

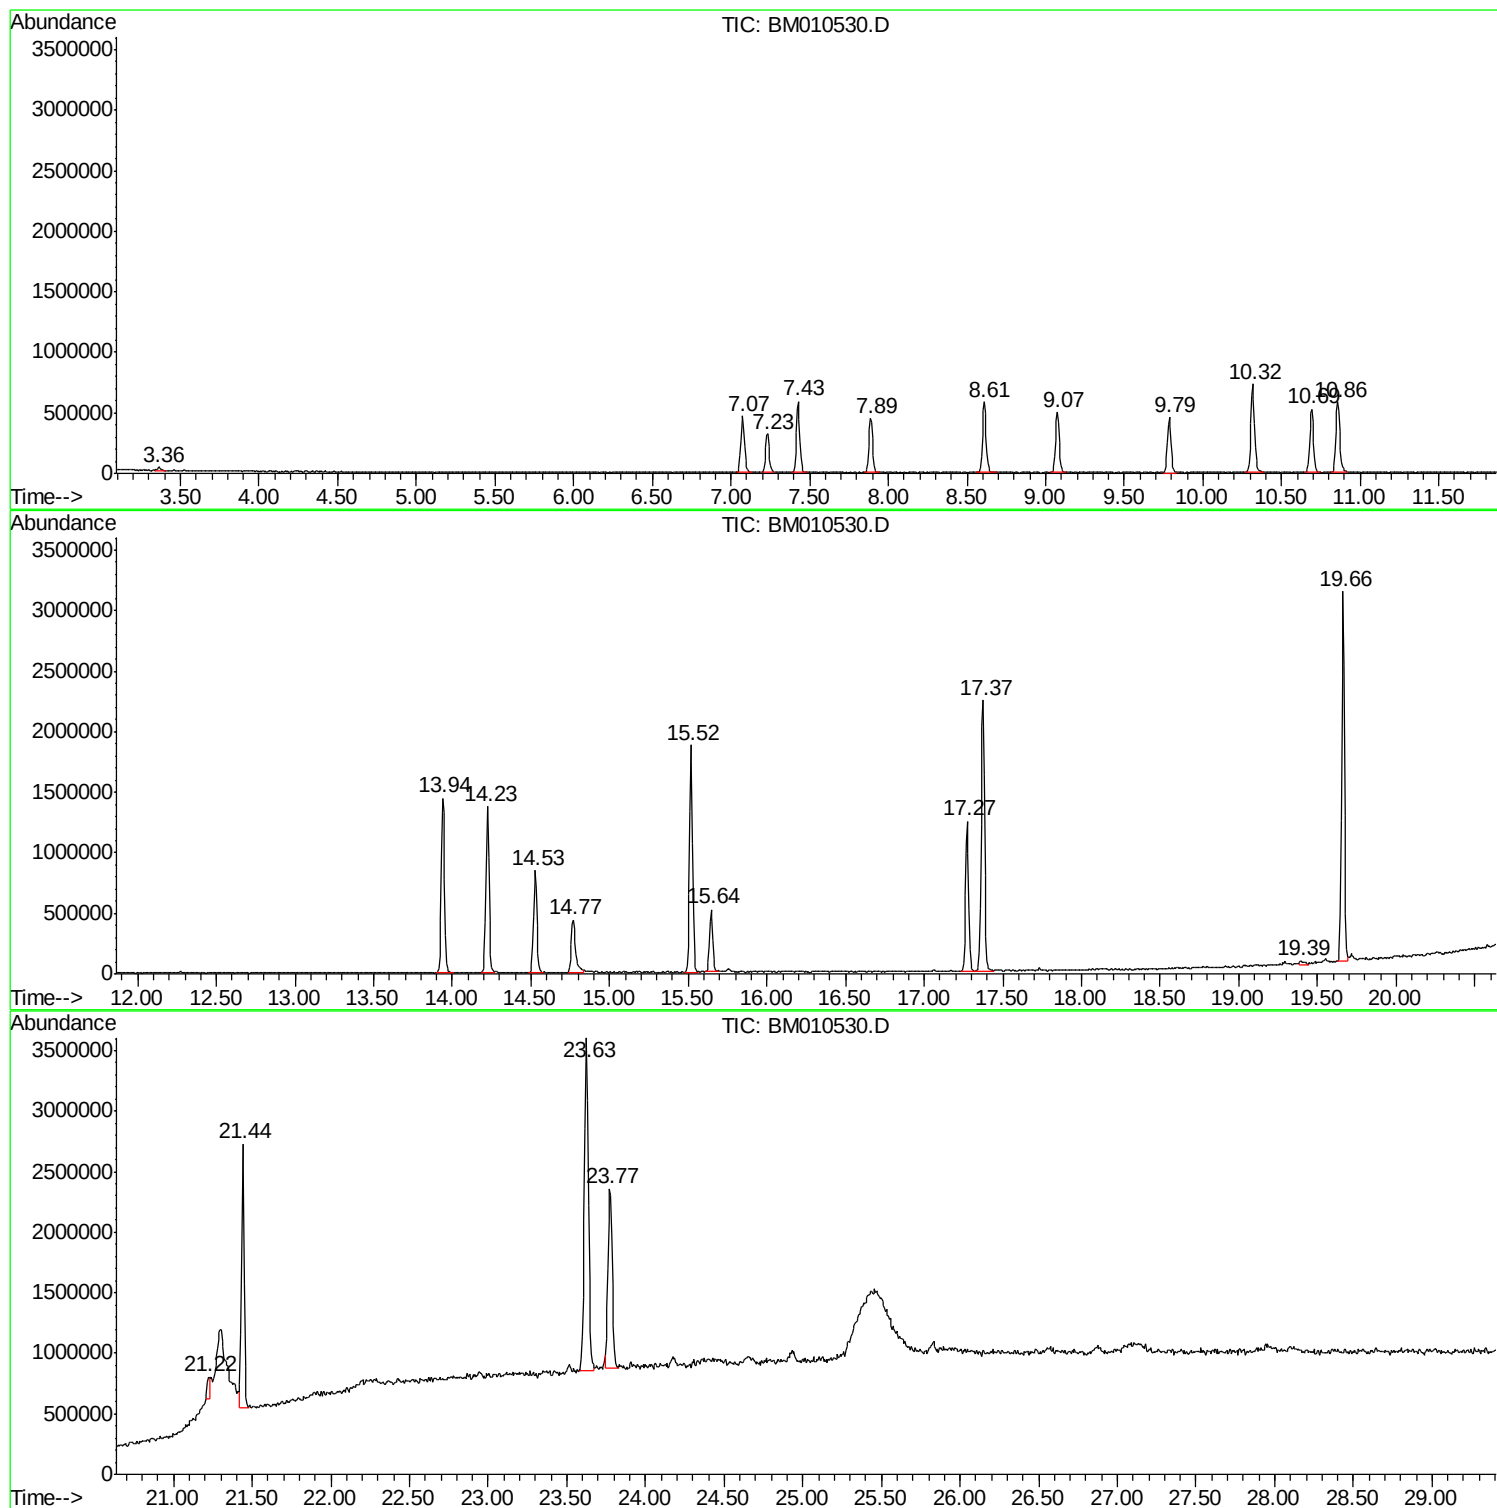

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061217\
Data File : BM010530.D
Acq On : 12 Jun 2017 12:06
Operator : SJ/MA
Sample : PB99650BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK50

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061217\
Data File : BM010530.D
Acq On : 12 Jun 2017 12:06
Operator : SJ/MA
Sample : PB99650BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK50

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc