

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061217\
 Data File : BM010536.D
 Acq On : 12 Jun 2017 15:43
 Operator : SJ/MA
 Sample : I3493-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDC68

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.316	34	39	44	rBV2	136855	189183	3.78%	0.501%
2	7.075	673	678	691	rVB2	95867	166425	3.32%	0.441%
3	7.234	698	705	714	rBV	350532	575503	11.49%	1.525%
4	7.428	730	738	747	rBV	525301	817601	16.32%	2.167%
5	7.887	810	816	825	rBV	555413	896512	17.89%	2.376%
6	8.610	932	939	951	rBV2	320141	533802	10.65%	1.414%
7	9.075	1009	1018	1026	rBV	554313	925416	18.47%	2.452%
8	9.786	1132	1139	1150	rBV	531315	886696	17.70%	2.350%
9	10.316	1221	1229	1243	rBV	781002	1359111	27.13%	3.601%
10	10.692	1285	1293	1300	rBV	638856	1100993	21.98%	2.917%
11	13.939	1839	1845	1854	rBV	1606268	2228071	44.47%	5.904%
12	14.221	1885	1893	1903	rBV	1575090	2348426	46.88%	6.223%
13	14.527	1936	1945	1952	rBV2	986017	1514807	30.24%	4.014%
14	14.780	1983	1988	2000	rBV5	54315	143816	2.87%	0.381%
15	15.515	2107	2113	2122	rBV	2144605	3061046	61.10%	8.111%
16	15.645	2129	2135	2145	rBV	549687	758985	15.15%	2.011%
17	17.274	2405	2412	2422	rBV	1383008	1949979	38.92%	5.167%
18	17.374	2422	2429	2437	rBV	2418674	3459498	69.05%	9.167%
19	19.074	2711	2718	2721	rBV9	21659	51041	1.02%	0.135%
20	19.392	2769	2772	2777	rBV6	39615	60200	1.20%	0.160%
21	19.662	2812	2818	2825	rBV	3191091	4261222	85.05%	11.292%
22	21.439	3116	3120	3127	rBV	2070791	2672029	53.33%	7.080%
23	23.627	3486	3492	3501	rVB	2751146	5009966	100.00%	13.276%
24	23.774	3511	3517	3525	rBV	1393981	2767947	55.25%	7.335%


Sum of corrected areas: 37738275

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061217\
Data File : BM010536.D
Acq On : 12 Jun 2017 15:43
Operator : SJ/MA
Sample : I3493-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDC68

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

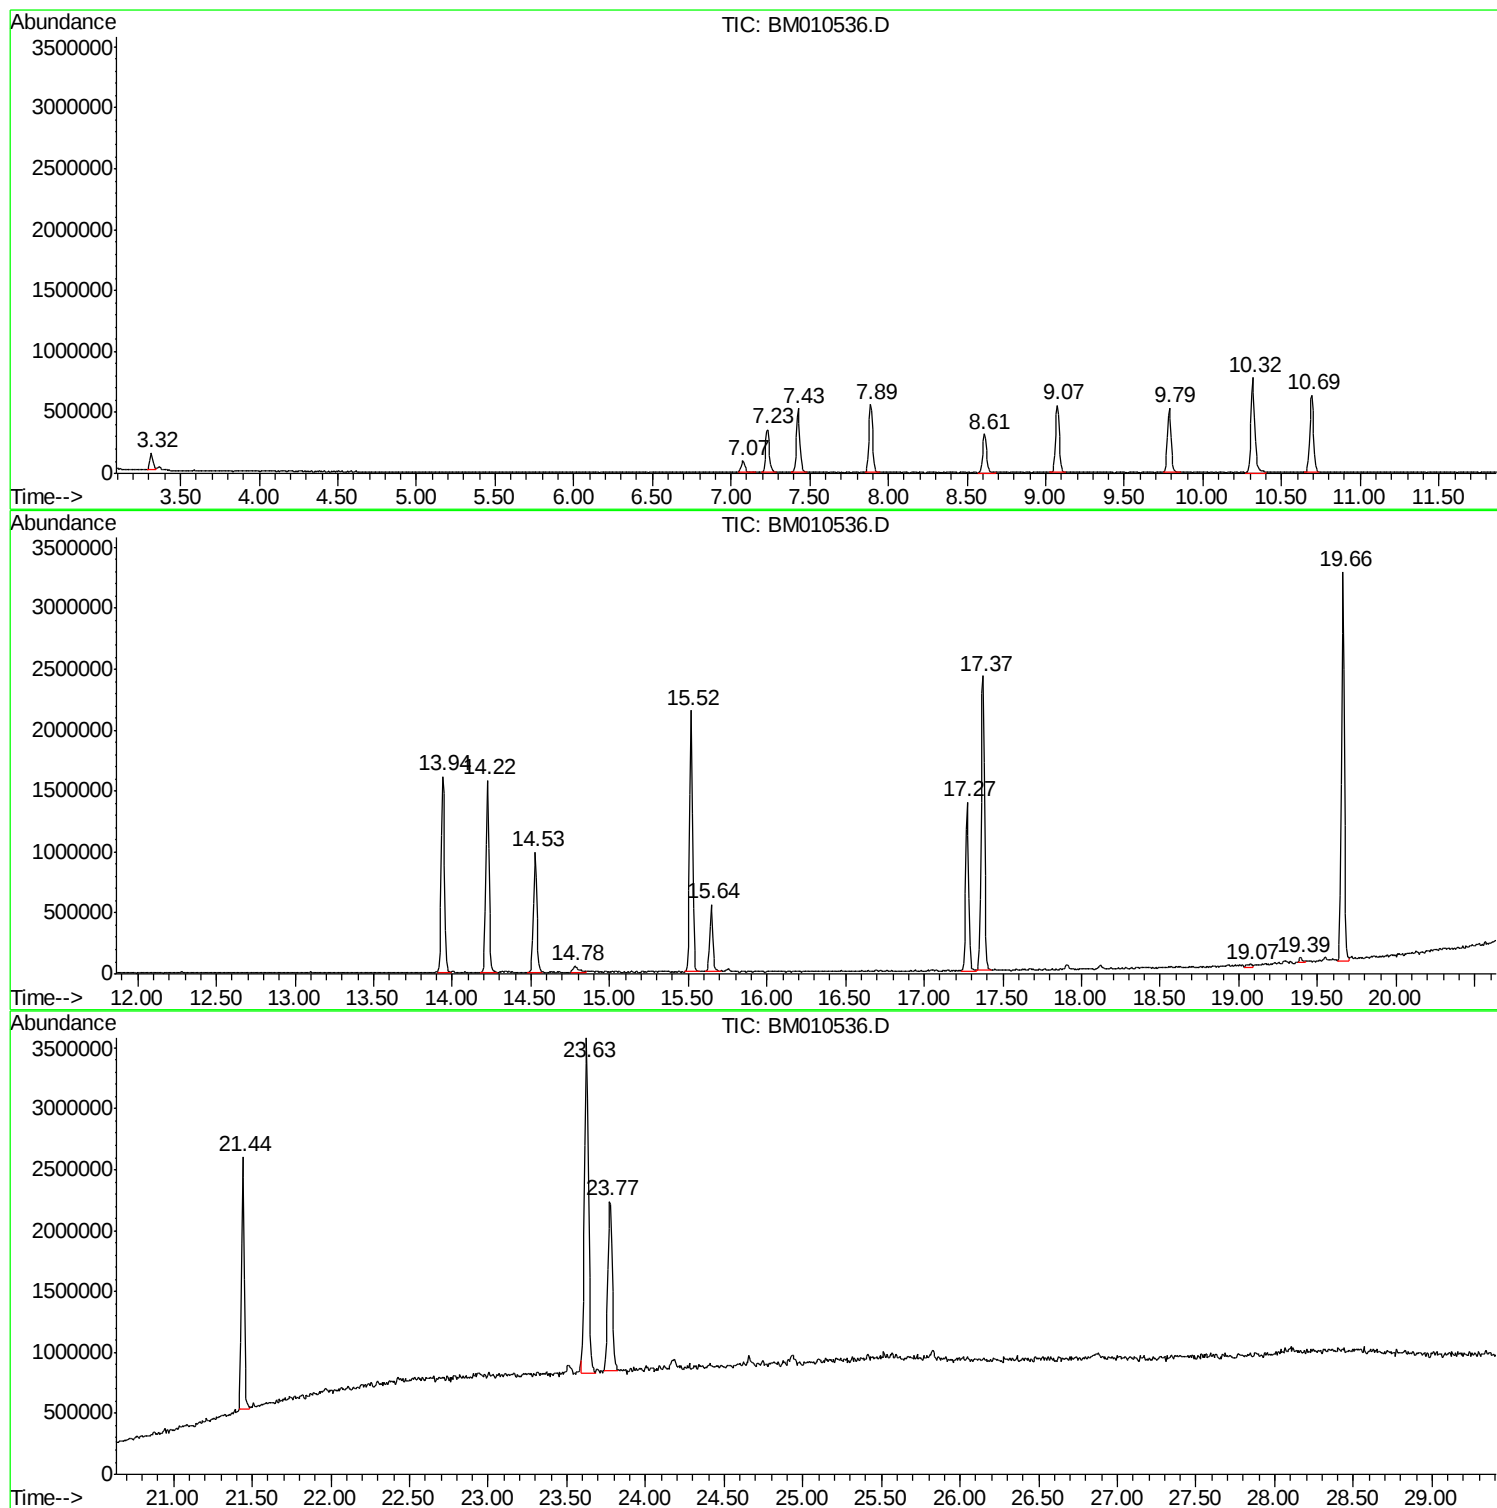

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061217\
Data File : BM010536.D
Acq On : 12 Jun 2017 15:43
Operator : SJ/MA
Sample : I3493-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDC68

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061217\
Data File : BM010536.D
Acq On : 12 Jun 2017 15:43
Operator : SJ/MA
Sample : I3493-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDC68

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc