

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061217\
 Data File : BM010539.D
 Acq On : 12 Jun 2017 17:31
 Operator : SJ/MA
 Sample : I3493-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDC52

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.316	34	39	45	rBV	215490	315140	6.80%	0.881%
2	4.593	251	256	265	rBV	136978	201773	4.35%	0.564%
3	7.069	670	677	685	rBV2	94369	167629	3.62%	0.468%
4	7.228	699	704	714	rBV	304162	498733	10.76%	1.394%
5	7.428	729	738	748	rBV	451624	738468	15.94%	2.063%
6	7.887	807	816	825	rBV	515639	816592	17.62%	2.282%
7	8.610	933	939	948	rBV	295917	489606	10.57%	1.368%
8	9.075	1011	1018	1028	rBV	468871	801798	17.30%	2.240%
9	9.786	1132	1139	1147	rBV	460133	774016	16.70%	2.163%
10	10.316	1222	1229	1240	rBV2	709933	1233636	26.62%	3.447%
11	10.692	1285	1293	1300	rBV	576648	1005717	21.70%	2.810%
12	10.863	1317	1322	1330	rBV6	27548	61416	1.33%	0.172%
13	13.939	1839	1845	1853	rBV	1481219	2017025	43.53%	5.636%
14	14.221	1887	1893	1901	rBV	1403665	2100317	45.32%	5.869%
15	14.527	1935	1945	1953	rBV2	878338	1395166	30.11%	3.898%
16	14.774	1982	1987	1995	rBV4	61783	131263	2.83%	0.367%
17	15.515	2103	2113	2122	rBV	1986583	2808230	60.60%	7.847%
18	15.645	2129	2135	2145	rBV	570159	786225	16.97%	2.197%
19	17.274	2406	2412	2417	rBV	1266440	1813554	39.13%	5.068%
20	17.374	2422	2429	2439	rVB	2176194	3136055	67.67%	8.763%
21	19.292	2752	2755	2759	rVB4	32750	55345	1.19%	0.155%
22	19.398	2767	2773	2778	rBV10	59564	138095	2.98%	0.386%
23	19.539	2793	2797	2804	rVB2	171708	239194	5.16%	0.668%
24	19.662	2812	2818	2824	rBV	3087155	4006390	86.45%	11.195%
25	21.439	3116	3120	3128	rBV	2196059	2664507	57.50%	7.445%
26	23.627	3486	3492	3499	rVB2	2502817	4634149	100.00%	12.949%
27	23.774	3512	3517	3525	rVB	1518047	2757668	59.51%	7.706%


Sum of corrected areas: 35787707

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061217\
Data File : BM010539.D
Acq On : 12 Jun 2017 17:31
Operator : SJ/MA
Sample : I3493-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDC52

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

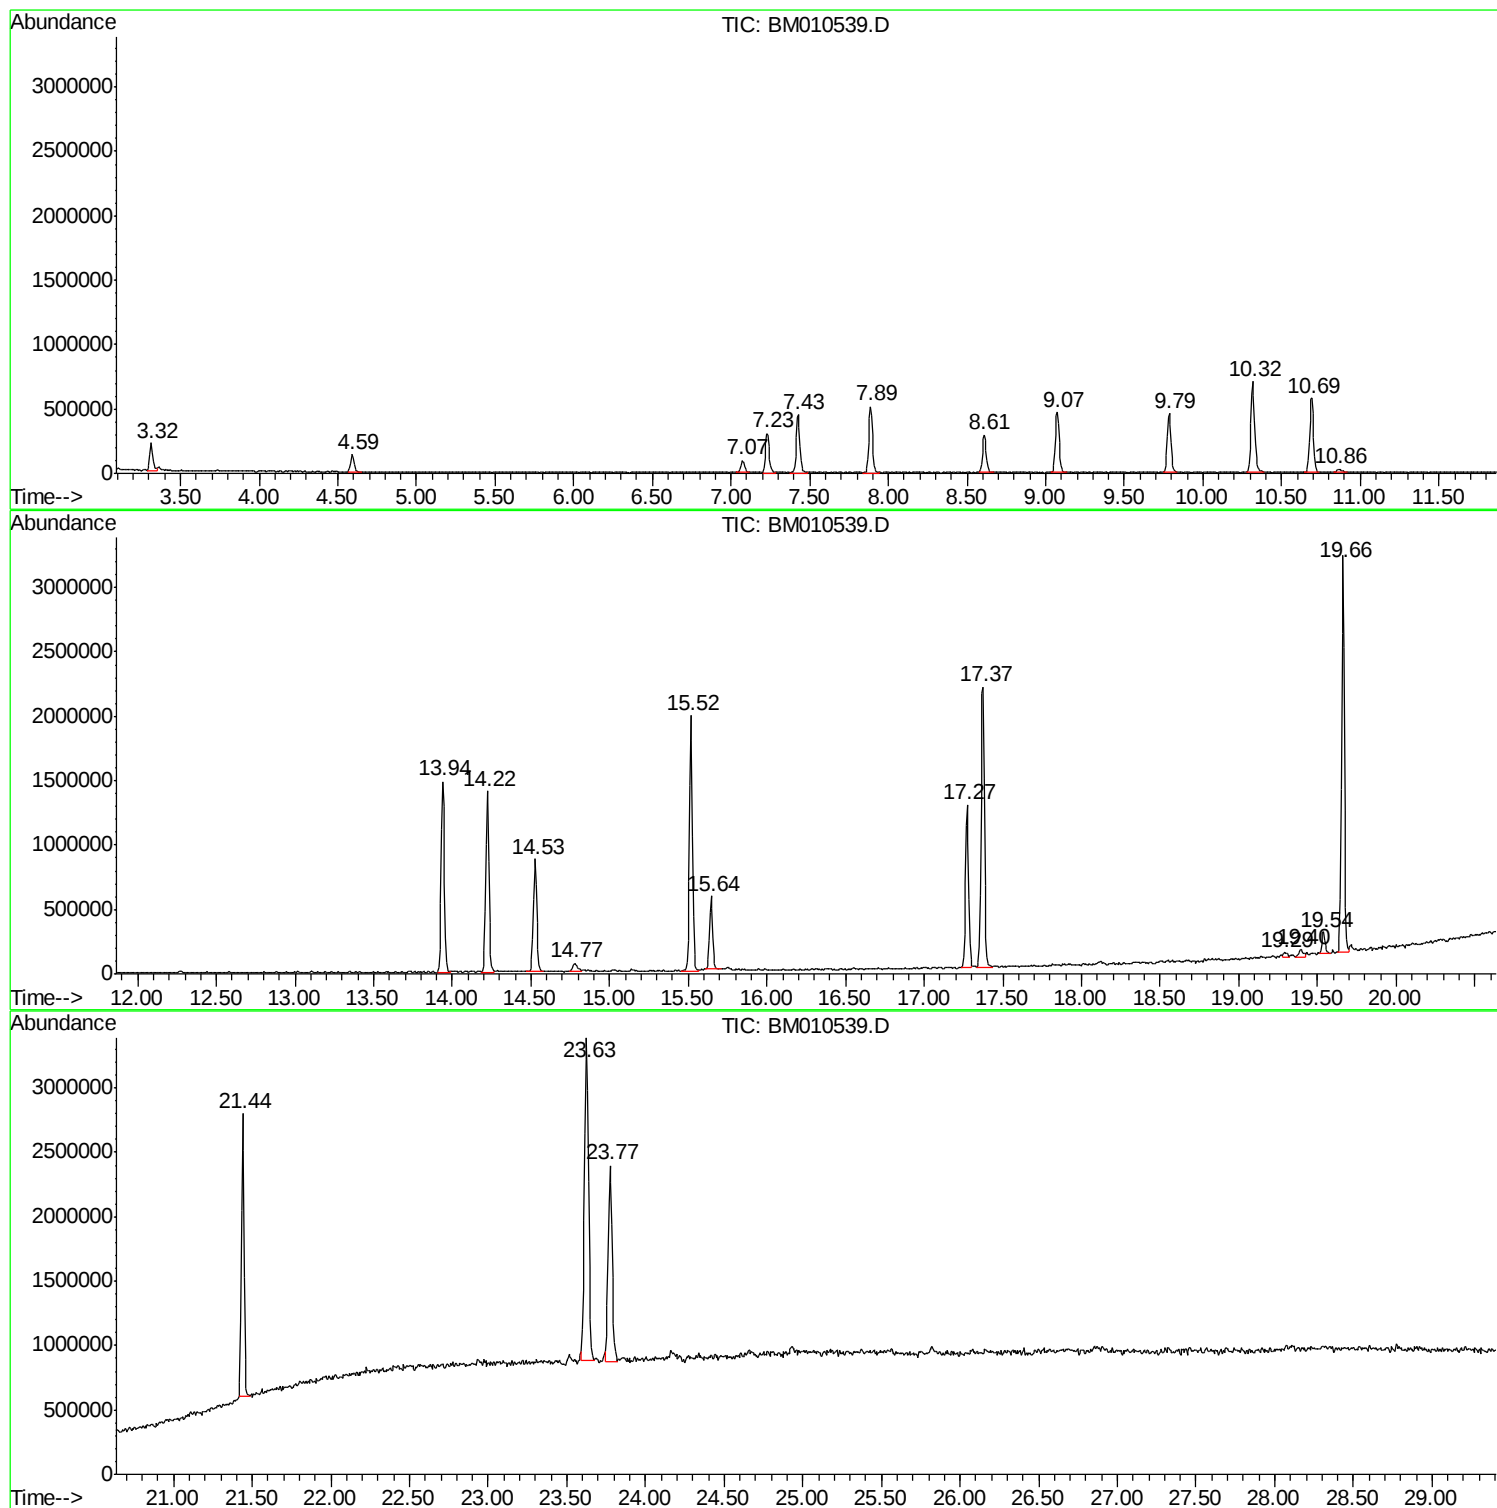

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061217\
Data File : BM010539.D
Acq On : 12 Jun 2017 17:31
Operator : SJ/MA
Sample : I3493-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDC52

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061217\
Data File : BM010539.D
Acq On : 12 Jun 2017 17:31
Operator : SJ/MA
Sample : I3493-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDC52

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc