

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061217\
 Data File : BM010543.D
 Acq On : 12 Jun 2017 19:56
 Operator : SJ/MA
 Sample : I3493-11
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDC82

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	7.075	672	678	686	rVB2	111346	190732	3.17%	0.462%
2	7.228	698	704	714	rBV	323851	537942	8.94%	1.304%
3	7.428	731	738	748	rBV	498599	797027	13.25%	1.932%
4	7.887	808	816	825	rBV	527818	822142	13.67%	1.993%
5	8.610	933	939	948	rVB3	323350	549238	9.13%	1.331%
6	9.075	1011	1018	1026	rBV	526471	887296	14.75%	2.151%
7	9.787	1131	1139	1151	rBV	516396	871107	14.48%	2.111%
8	10.316	1221	1229	1239	rBV	773730	1336454	22.22%	3.239%
9	10.692	1286	1293	1300	rBV	601406	1023899	17.02%	2.482%
10	13.939	1838	1845	1853	rBV	1629035	2196694	36.52%	5.325%
11	14.222	1885	1893	1901	rBV	1536012	2302567	38.28%	5.581%
12	14.527	1937	1945	1952	rBV2	985784	1524579	25.35%	3.695%
13	14.774	1983	1987	1994	rBV2	86011	171121	2.84%	0.415%
14	15.516	2107	2113	2119	rBV	2202323	3034003	50.44%	7.354%
15	15.645	2128	2135	2146	rBV	692114	993853	16.52%	2.409%
16	17.274	2405	2412	2420	rBV	1519859	2074546	34.49%	5.029%
17	17.374	2422	2429	2437	rVV	2492015	3608206	59.99%	8.746%
18	17.821	2501	2505	2508	rBV6	73595	108653	1.81%	0.263%
19	17.892	2508	2517	2530	rVB6	71945	229830	3.82%	0.557%
20	19.386	2769	2771	2778	rBV7	61320	94193	1.57%	0.228%
21	19.539	2794	2797	2802	rVB2	76114	96772	1.61%	0.235%
22	19.662	2812	2818	2823	rBV	3800061	4914277	81.70%	11.912%
23	21.439	3116	3120	3127	rVB	2833179	3319799	55.19%	8.047%
24	23.627	3485	3492	3500	rVB2	3128177	6014802	100.00%	14.579%
25	23.774	3511	3517	3526	rVB	1821511	3555682	59.12%	8.619%


Sum of corrected areas: 41255414

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061217\
Data File : BM010543.D
Acq On : 12 Jun 2017 19:56
Operator : SJ/MA
Sample : I3493-11
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
BDC82

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

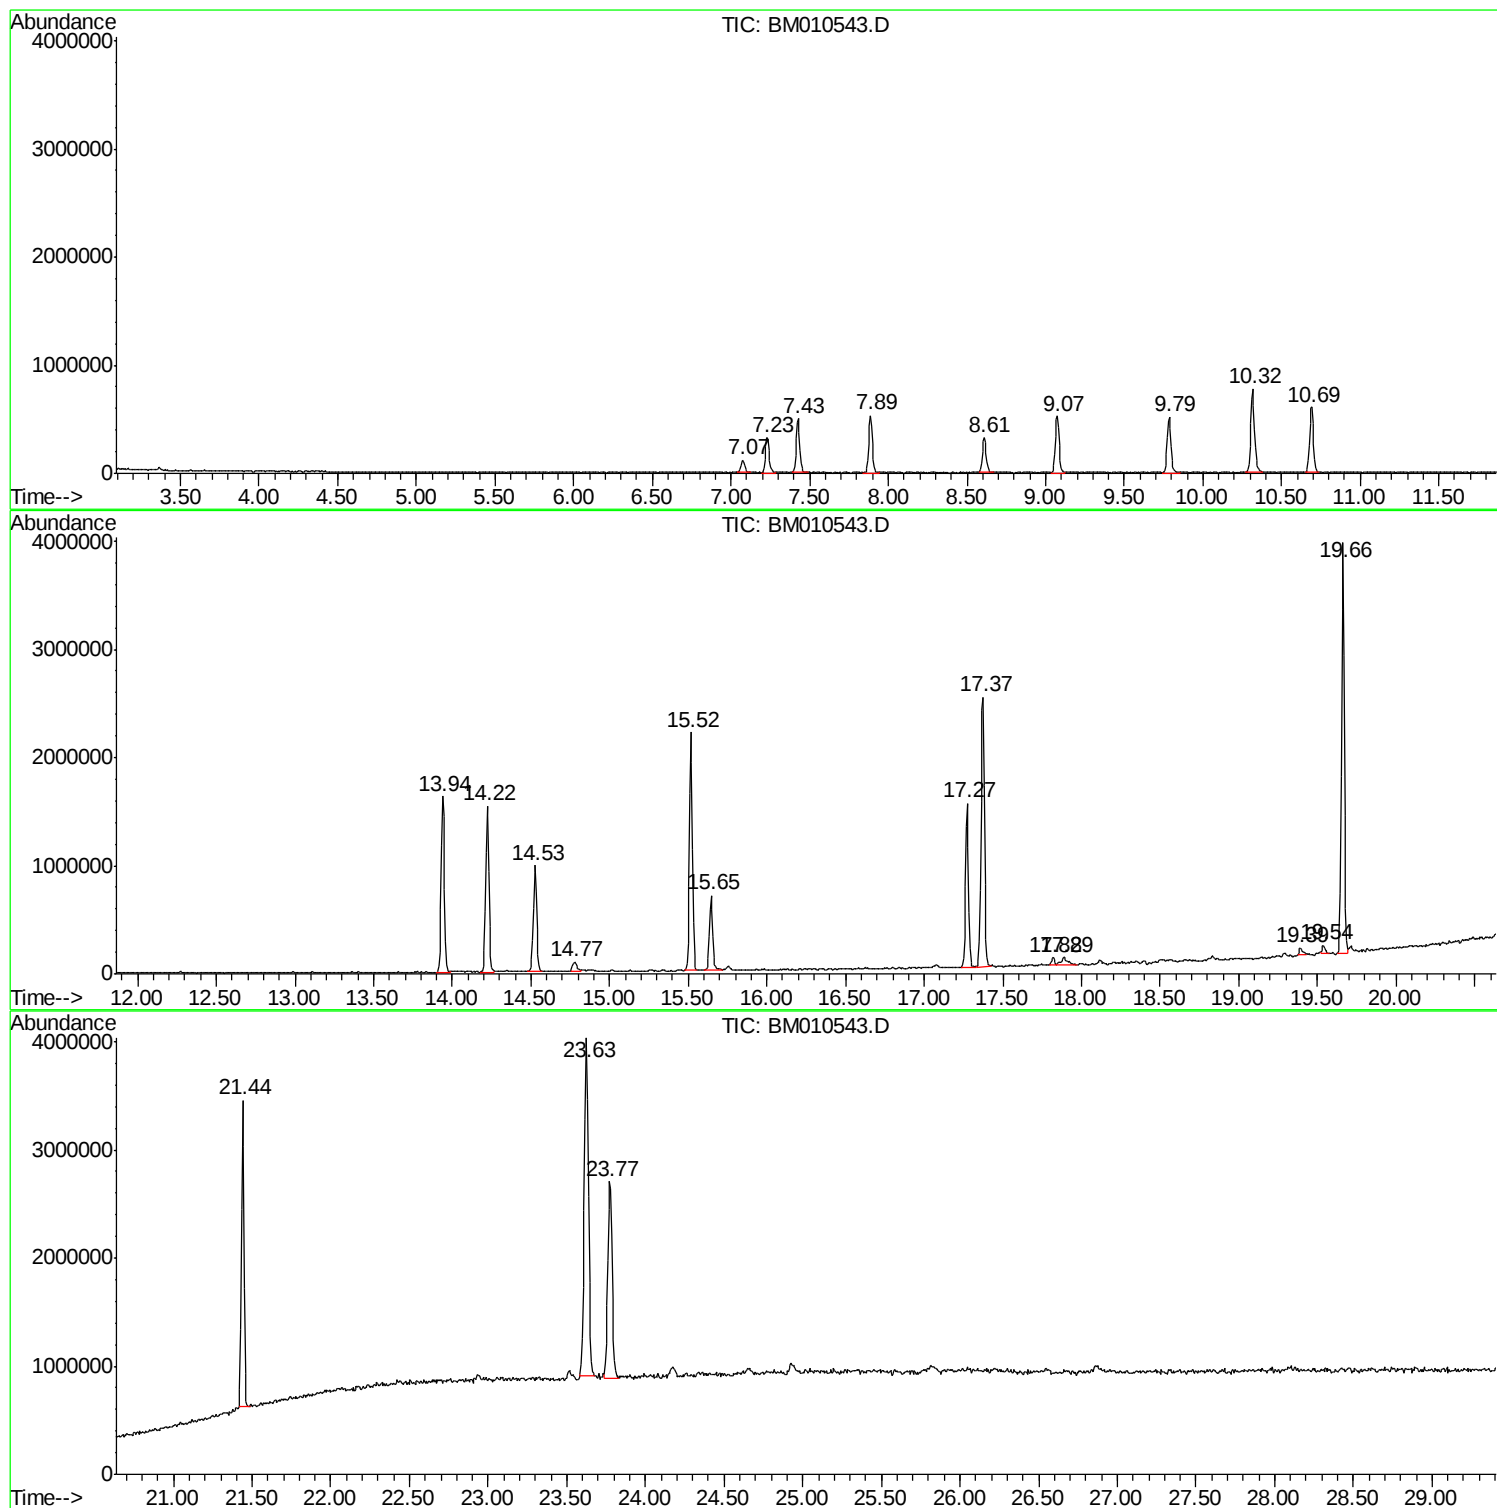

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061217\
Data File : BM010543.D
Acq On : 12 Jun 2017 19:56
Operator : SJ/MA
Sample : I3493-11
Misc :
ALS Vial : 17 Sample Multiplier: 1










Instrument :
BNA_M
ClientSampleId :
BDC82

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
17.89	2.22 ng/ul	229830	Phenanthrene-d10	17.27
Hit# of	5	Tentative ID	MW MolForm	CAS# Qual
1		1,2-Dehydro-as-hydrindacene	170 C13H14	096508-75-7 22
2		Cyclopropanecarboxylic acid, 2-(...	216 C14H16O2	090909-49-2 18
3		1,4-Methanonaphthalene, 1,4-dihy...	142 C11H10	004453-90-1 18
4		3-Fluoro-para-anisaldehyde	154 C8H7FO2	000351-54-2 18
5		Naphthalene, 1-methyl-	142 C11H10	000090-12-0 18

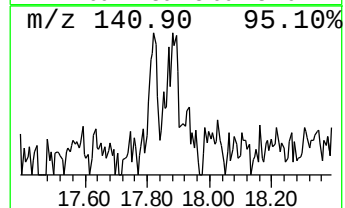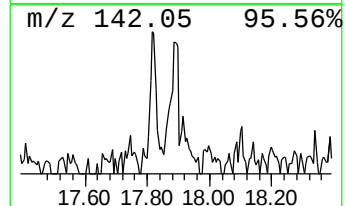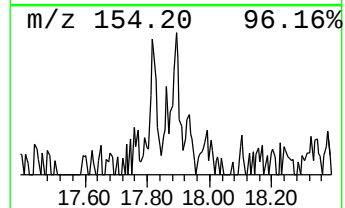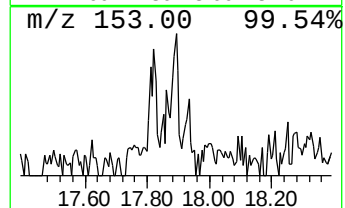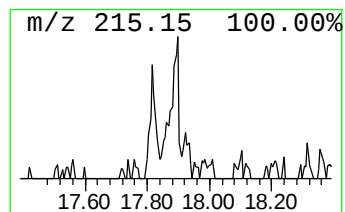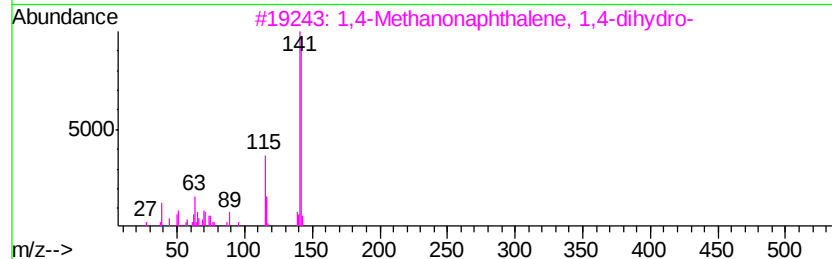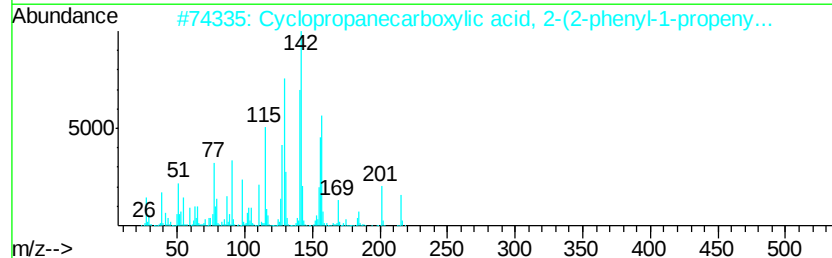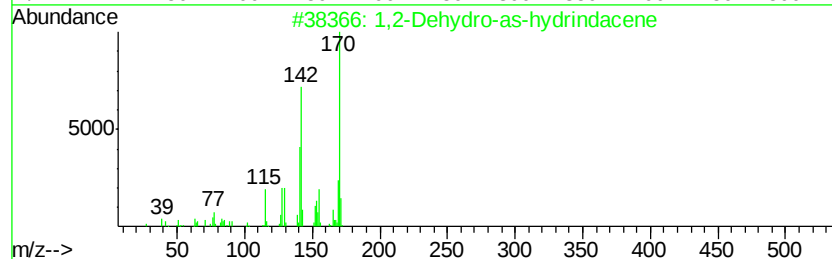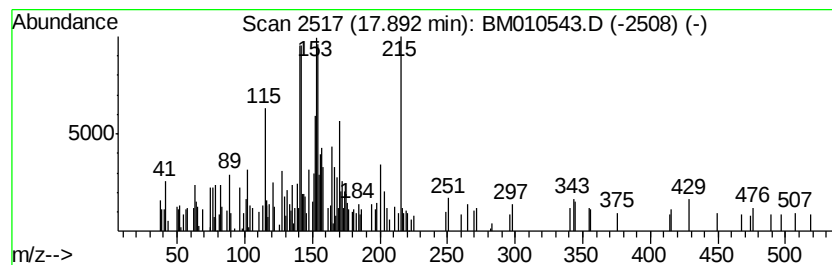

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061217\
Data File : BM010543.D
Acq On : 12 Jun 2017 19:56
Operator : SJ/MA
Sample : I3493-11
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDC82

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	17.89	2.2	ng/ul	229830	4	17.27	2074550	20.0