

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061217\
 Data File : BM010544.D
 Acq On : 12 Jun 2017 20:32
 Operator : SJ/MA
 Sample : I3493-12
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDC85

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	7.069	670	677	685	rBV2	91951	172941	3.13%	0.427%
2	7.228	697	704	715	rBV	354827	569240	10.30%	1.404%
3	7.428	731	738	744	rBV	481506	777707	14.07%	1.919%
4	7.887	809	816	823	rBV	577832	900025	16.28%	2.220%
5	8.610	932	939	951	rBV2	318212	526216	9.52%	1.298%
6	9.069	1010	1017	1028	rBV	542757	933702	16.89%	2.303%
7	9.786	1130	1139	1153	rBV	537170	903202	16.34%	2.228%
8	10.316	1220	1229	1243	rBV	763391	1382947	25.02%	3.412%
9	10.686	1286	1292	1299	rBV	688808	1173526	21.23%	2.895%
10	13.939	1839	1845	1854	rBV	1653655	2249883	40.70%	5.550%
11	14.221	1887	1893	1899	rBV	1590805	2366171	42.81%	5.837%
12	14.527	1937	1945	1953	rVB2	1032653	1675760	30.32%	4.134%
13	14.780	1983	1988	1994	rBV4	67207	134045	2.43%	0.331%
14	15.516	2106	2113	2120	rBV	2182968	3129464	56.62%	7.720%
15	15.645	2128	2135	2142	rBV	707532	982759	17.78%	2.424%
16	17.274	2406	2412	2418	rBV	1490643	2156392	39.01%	5.320%
17	17.368	2422	2428	2436	rBV2	2463132	3609292	65.30%	8.904%
18	17.815	2500	2504	2509	rBV8	74680	103738	1.88%	0.256%
19	19.392	2769	2772	2779	rVB9	59562	91916	1.66%	0.227%
20	19.539	2794	2797	2803	rVB3	71987	112860	2.04%	0.278%
21	19.662	2812	2818	2824	rBV	3629023	4687618	84.81%	11.564%
22	21.439	3116	3120	3126	rVB	2527030	3145889	56.91%	7.761%
23	23.627	3485	3492	3500	rVB2	2933696	5527481	100.00%	13.636%
24	23.780	3511	3518	3526	rVB	1698687	3224395	58.33%	7.954%


Sum of corrected areas: 40537169

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061217\
Data File : BM010544.D
Acq On : 12 Jun 2017 20:32
Operator : SJ/MA
Sample : I3493-12
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDC85

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

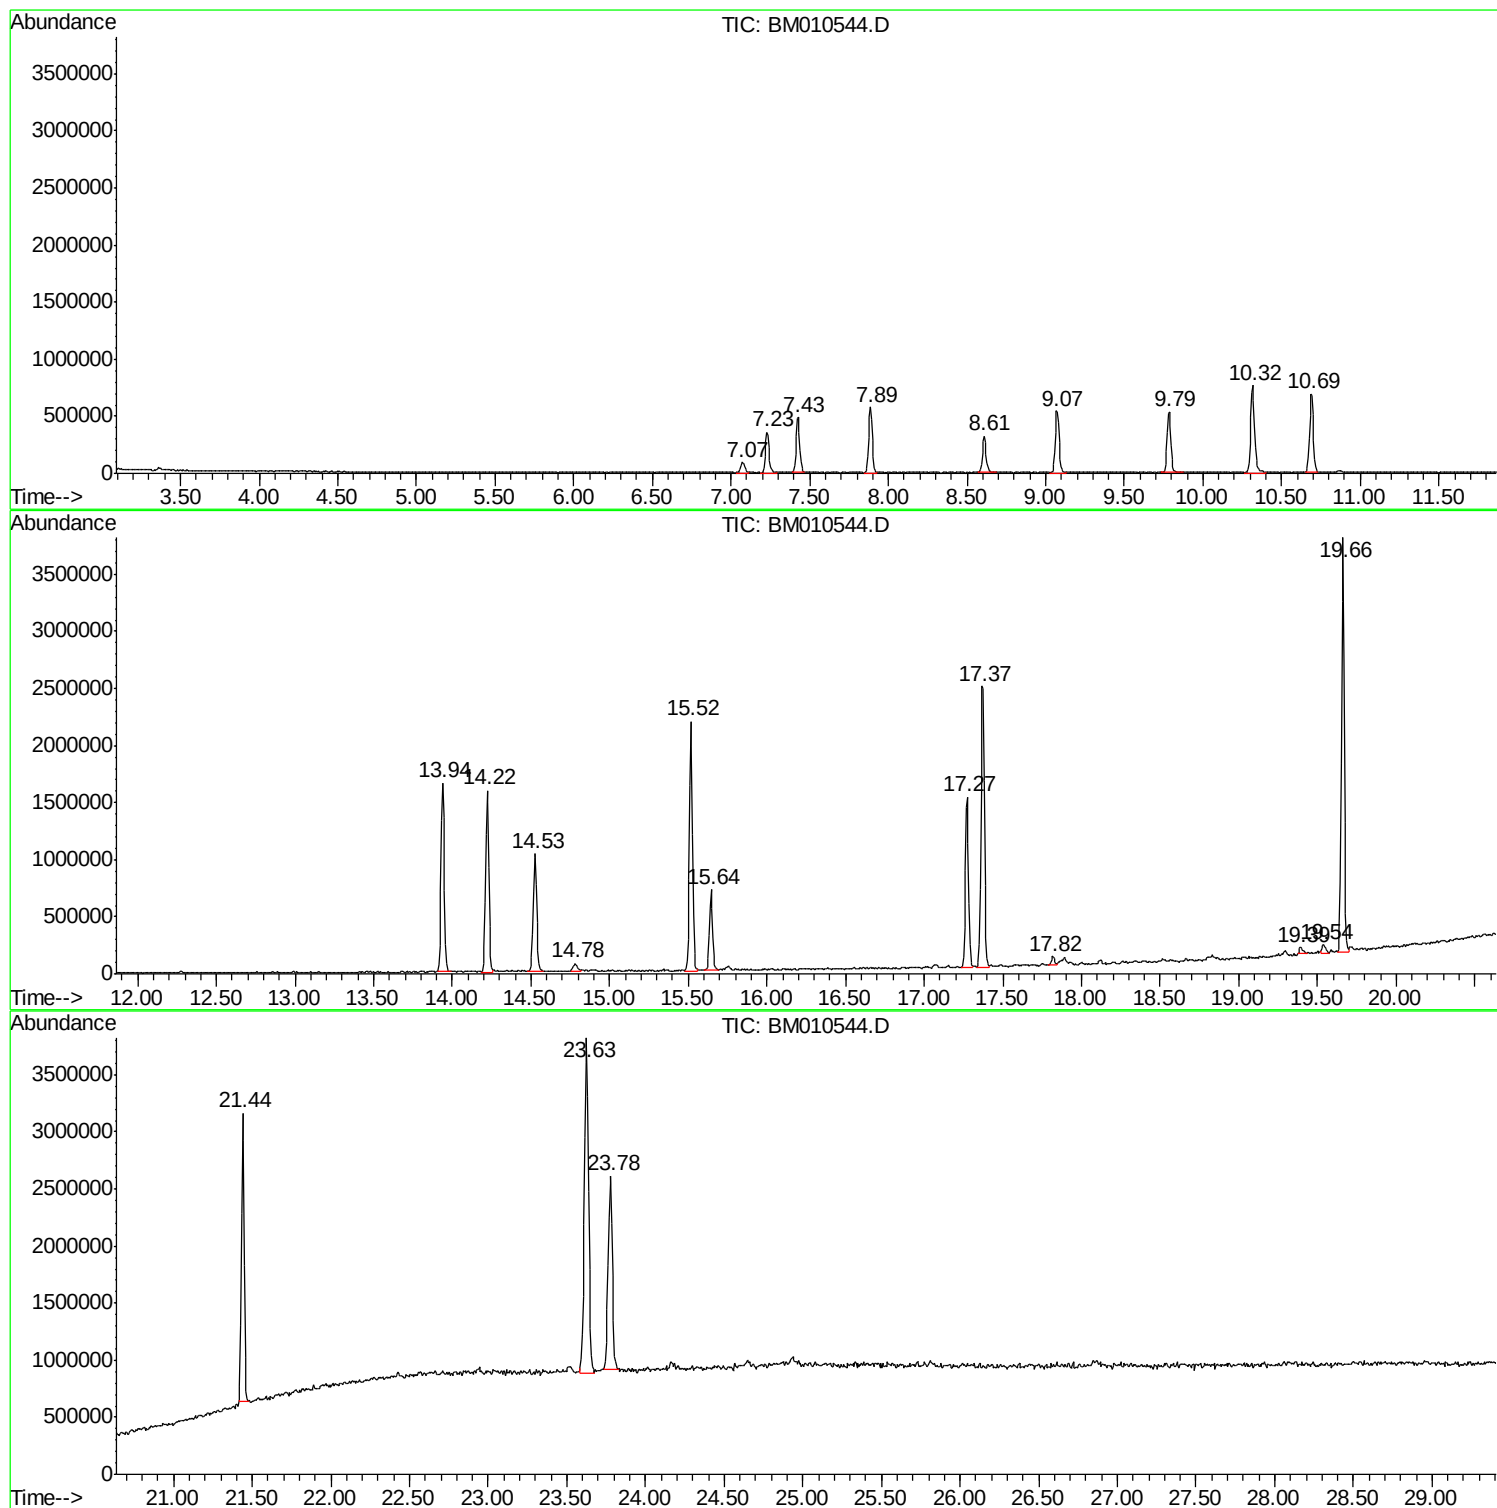

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061217\
Data File : BM010544.D
Acq On : 12 Jun 2017 20:32
Operator : SJ/MA
Sample : I3493-12
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDC85

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061217\
Data File : BM010544.D
Acq On : 12 Jun 2017 20:32
Operator : SJ/MA
Sample : I3493-12
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDC85

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc