

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061220\
 Data File : BM026379.D
 Acq On : 12 Jun 2020 16:18
 Operator : JU/CG
 Sample : L2850-05
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ETTX1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.222	54	57	65	rVB2	20557	23701	1.67%	0.332%
2	3.528	107	109	110	rBV2	3656	2427	0.17%	0.034%
3	3.651	128	130	131	rBV2	2370	1912	0.13%	0.027%
4	3.681	132	135	139	rVB2	8966	10122	0.71%	0.142%
5	3.851	162	164	166	rBV3	1707	1571	0.11%	0.022%
6	4.222	223	227	228	rBV3	1582	1426	0.10%	0.020%
7	4.310	239	242	248	rVB3	5687	8833	0.62%	0.124%
8	4.740	314	315	318	rBV3	1741	2035	0.14%	0.029%
9	4.828	327	330	334	rVB7	2097	3396	0.24%	0.048%
10	4.893	340	341	343	rBV2	1879	1947	0.14%	0.027%
11	4.963	350	353	355	rBV3	1427	1662	0.12%	0.023%
12	5.310	411	412	415	rVB3	1562	1444	0.10%	0.020%
13	5.345	415	418	422	rBV6	2394	3661	0.26%	0.051%
14	5.898	509	512	515	rVB5	1485	2065	0.15%	0.029%
15	6.281	574	577	580	rBV5	1513	2282	0.16%	0.032%
16	6.475	608	610	612	rBV2	1850	1952	0.14%	0.027%
17	6.592	625	630	632	rBV4	3047	4380	0.31%	0.061%
18	6.628	634	636	639	rVB4	2226	2203	0.15%	0.031%
19	6.663	639	642	645	rBV5	1774	2468	0.17%	0.035%
20	6.745	653	656	659	rBV4	1452	2297	0.16%	0.032%
21	6.828	667	670	671	rBV3	1887	1841	0.13%	0.026%
22	7.116	715	719	722	rBV5	1605	2034	0.14%	0.028%
23	7.304	750	751	756	rVB4	1963	1693	0.12%	0.024%
24	7.404	762	768	783	rBV	391604	616921	43.40%	8.642%
25	8.398	935	937	942	rBV4	1164	1615	0.11%	0.023%
26	8.533	956	960	962	rVB4	1511	1979	0.14%	0.028%
27	9.186	1068	1071	1073	rBV4	1272	1444	0.10%	0.020%
28	10.169	1231	1238	1251	rBV	483853	806721	56.76%	11.301%
29	10.310	1259	1262	1266	rBV5	1142	1638	0.12%	0.023%
30	10.516	1295	1297	1300	rVB3	1473	1681	0.12%	0.024%
31	10.810	1343	1347	1352	rBV4	1094	1665	0.12%	0.023%
32	11.163	1406	1407	1412	rBV3	1272	1610	0.11%	0.023%
33	11.227	1415	1418	1419	rBV2	1859	1422	0.10%	0.020%
34	11.374	1439	1443	1448	rBV4	785	1435	0.10%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061220\
 Data File : BM026379.D
 Acq On : 12 Jun 2020 16:18
 Operator : JU/CG
 Sample : L2850-05
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ETTX1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
 Title : SVOA CALIBRATION

35	11.733	1501	1504	1508	rBV5	1513	2125	0.15%	0.030%
36	12.651	1658	1660	1664	rBV2	1210	1672	0.12%	0.023%
37	13.151	1744	1745	1751	rVB3	1484	2033	0.14%	0.028%
38	13.739	1840	1845	1847	rBV2	1434	1875	0.13%	0.026%
39	13.892	1867	1871	1873	rVB5	1225	1765	0.12%	0.025%
40	14.063	1894	1900	1914	rBV2	677759	994353	69.96%	13.929%
41	14.204	1920	1924	1929	rVB6	4558	7511	0.53%	0.105%
42	14.968	2050	2054	2057	rBV5	1847	3400	0.24%	0.048%
43	15.210	2092	2095	2098	rBV3	1272	1713	0.12%	0.024%
44	15.339	2111	2117	2123	rBV	56337	77838	5.48%	1.090%
45	15.780	2189	2192	2195	rBV3	2138	2464	0.17%	0.035%
46	15.951	2216	2221	2226	rVB	7941	9906	0.70%	0.139%
47	15.992	2226	2228	2231	rBV3	1450	1816	0.13%	0.025%
48	16.062	2236	2240	2246	rVB2	13921	18305	1.29%	0.256%
49	16.204	2261	2264	2267	rBV4	1961	2608	0.18%	0.037%
50	16.356	2286	2290	2295	rBV3	10594	13834	0.97%	0.194%
51	16.451	2303	2306	2311	rVB4	1933	3597	0.25%	0.050%
52	16.498	2311	2314	2316	rBV3	2366	2595	0.18%	0.036%
53	16.527	2316	2319	2322	rBV4	1485	1615	0.11%	0.023%
54	16.609	2329	2333	2338	rVB5	2615	3619	0.25%	0.051%
55	16.709	2345	2350	2353	rBV2	56085	72470	5.10%	1.015%
56	16.745	2353	2356	2362	rVB3	18189	23874	1.68%	0.334%
57	16.821	2362	2369	2380	rBV	843121	1216561	85.59%	17.042%
58	16.921	2384	2386	2390	rVB3	2787	3398	0.24%	0.048%
59	17.003	2395	2400	2405	rVB2	28374	43393	3.05%	0.608%
60	17.251	2440	2442	2445	rVB2	2358	1779	0.13%	0.025%
61	17.286	2445	2448	2451	rBV4	3697	4348	0.31%	0.061%
62	17.433	2467	2473	2480	rVB3	34719	64079	4.51%	0.898%
63	17.551	2485	2493	2500	rBV8	10579	22841	1.61%	0.320%
64	17.680	2510	2515	2519	rBV4	8848	12262	0.86%	0.172%
65	17.727	2521	2523	2528	rVB5	4931	6464	0.45%	0.091%
66	17.809	2535	2537	2538	rBV2	2702	1921	0.14%	0.027%
67	17.839	2538	2542	2546	rVV6	2734	4714	0.33%	0.066%
68	17.898	2548	2552	2558	rBV4	19042	26621	1.87%	0.373%
69	17.956	2559	2562	2566	rVV5	10740	14194	1.00%	0.199%
70	18.003	2566	2570	2575	rVV5	6556	8109	0.57%	0.114%
71	18.186	2595	2601	2605	rBV3	19012	24268	1.71%	0.340%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061220\
 Data File : BM026379.D
 Acq On : 12 Jun 2020 16:18
 Operator : JU/CG
 Sample : L2850-05
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ETTX1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
 Title : SVOA CALIBRATION

72	18.233	2607	2609	2615	rVB7	4973	7768	0.55%	0.109%
73	18.292	2615	2619	2620	rBV4	3203	4359	0.31%	0.061%
74	18.327	2623	2625	2628	rVV4	4360	5100	0.36%	0.071%
75	18.362	2628	2631	2635	rVB4	8460	10858	0.76%	0.152%
76	18.462	2646	2648	2651	rVB4	3489	3616	0.25%	0.051%
77	18.580	2666	2668	2671	rVB4	2221	1739	0.12%	0.024%
78	18.692	2683	2687	2689	rBV4	4412	6914	0.49%	0.097%
79	18.727	2692	2693	2697	rVV4	5908	7360	0.52%	0.103%
80	18.774	2698	2701	2705	rVB5	6927	8842	0.62%	0.124%
81	18.845	2711	2713	2715	rBV3	2797	3091	0.22%	0.043%
82	18.986	2735	2737	2742	rVB5	4878	6032	0.42%	0.084%
83	19.197	2771	2773	2775	rVB3	6960	5422	0.38%	0.076%
84	21.027	3079	3084	3092	rBV	1147345	1421317	100.00%	19.910%
85	23.127	3435	3441	3451	rVB	811721	1414950	99.55%	19.821%


Sum of corrected areas: 7138791

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061220\
Data File : BM026379.D
Acq On : 12 Jun 2020 16:18
Operator : JU/CG
Sample : L2850-05
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ETTX1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

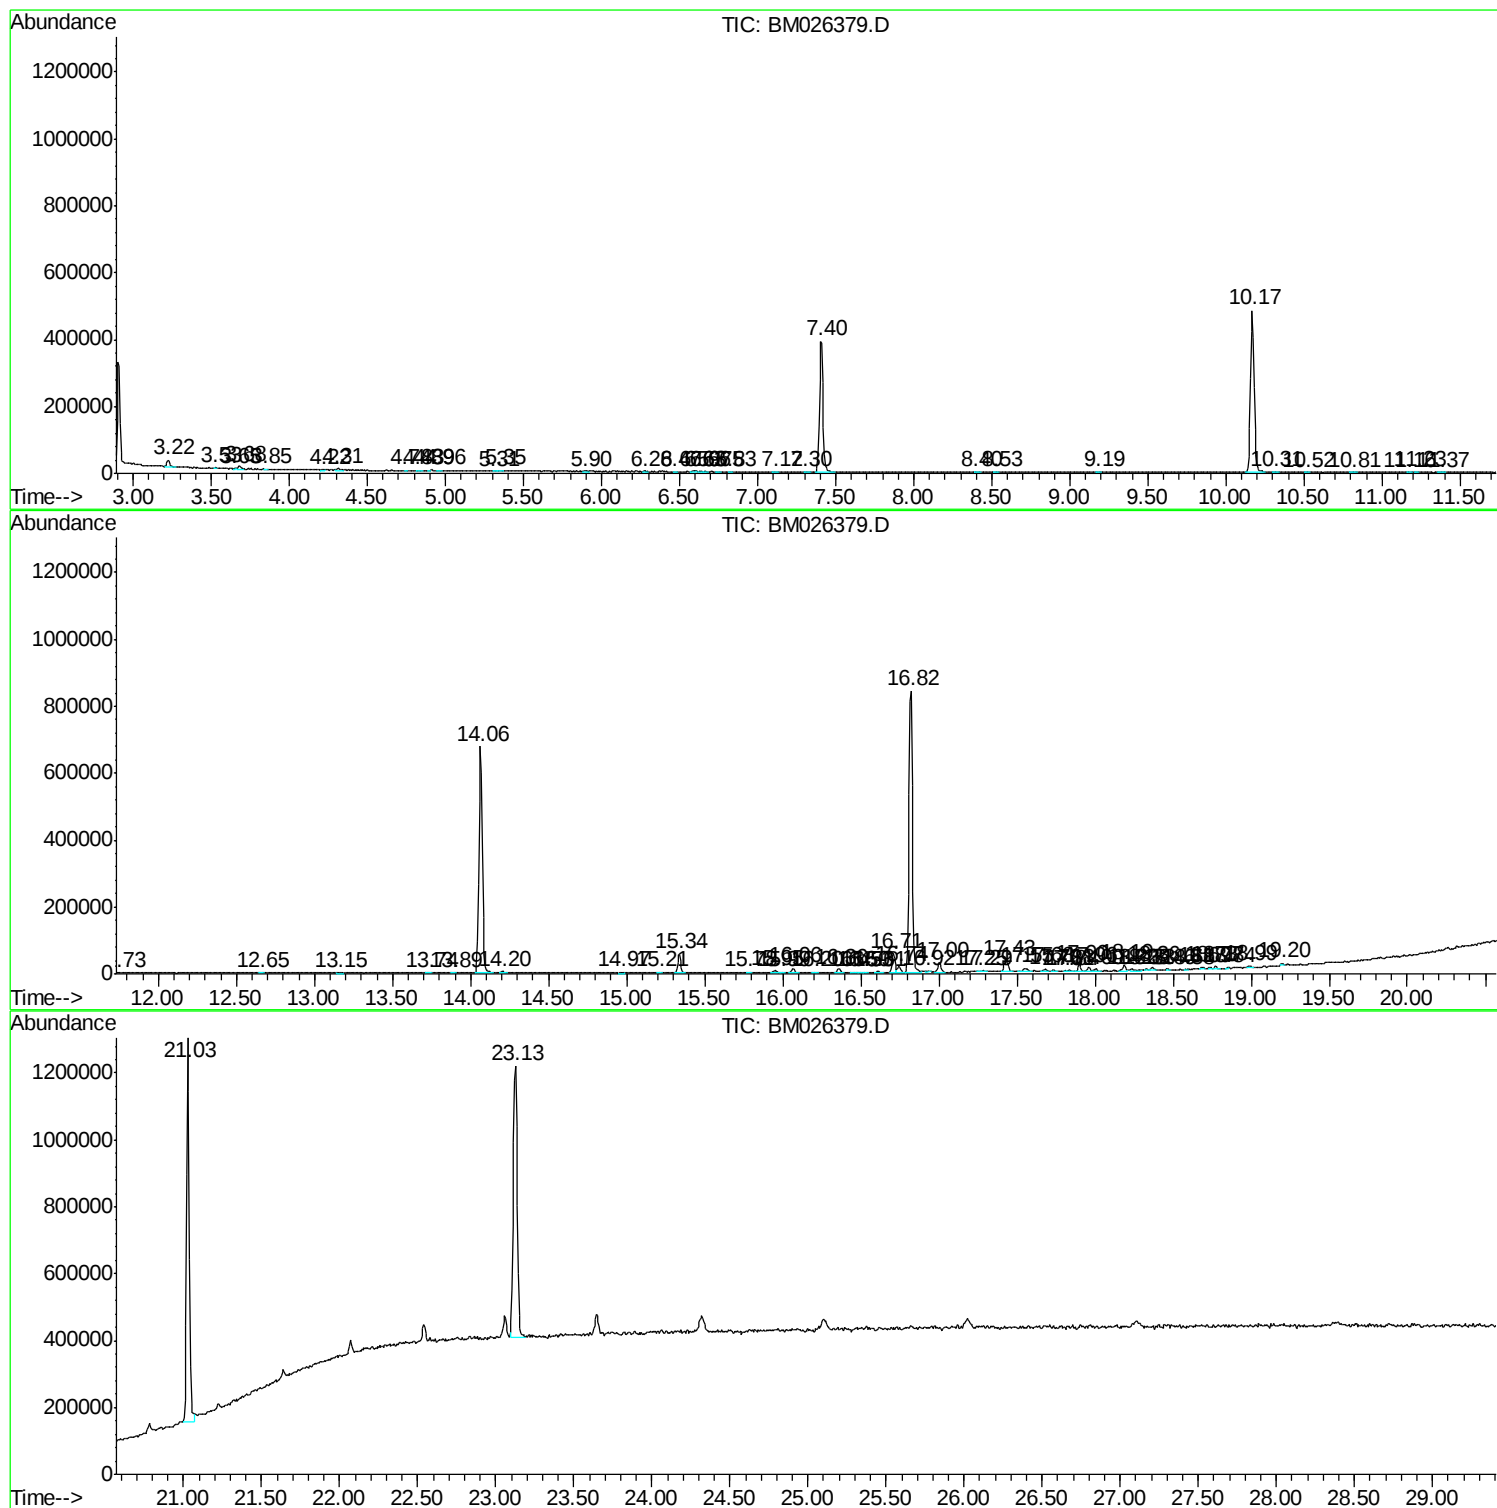

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061220\
Data File : BM026379.D
Acq On : 12 Jun 2020 16:18
Operator : JU/CG
Sample : L2850-05
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ETTX1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061220\
Data File : BM026379.D
Acq On : 12 Jun 2020 16:18
Operator : JU/CG
Sample : L2850-05
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ETTX1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc