

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061224\
 Data File : BM045993.D
 Acq On : 12 Jun 2024 11:26
 Operator : MA/JU
 Sample : PB161249BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK249

Quant Time: Jun 13 00:07:17 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM060624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 13 00:05:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.442	152	3270	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.211	136	11631	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.090	164	7003	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.930	188	1090150	0.400	ng/ul	0.08
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.04
23) Perylene-d12	23.133	264	16829	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.042	96	23532	6.318	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	11.838	152	5172	0.309	ng/ul	0.00
18) Fluoranthene-d10	18.867	212	12541	0.000	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.085	166	1987	0.076	ng/ul#	15
26) Benzo(a)pyrene	22.998	252	4004	0.072	ng/ul#	55


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061224\
Data File : BM045993.D
Acq On : 12 Jun 2024 11:26
Operator : MA/JU
Sample : PB161249BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK249

Quant Time: Jun 13 00:07:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM060624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 13 00:05:38 2024
Response via : Initial Calibration




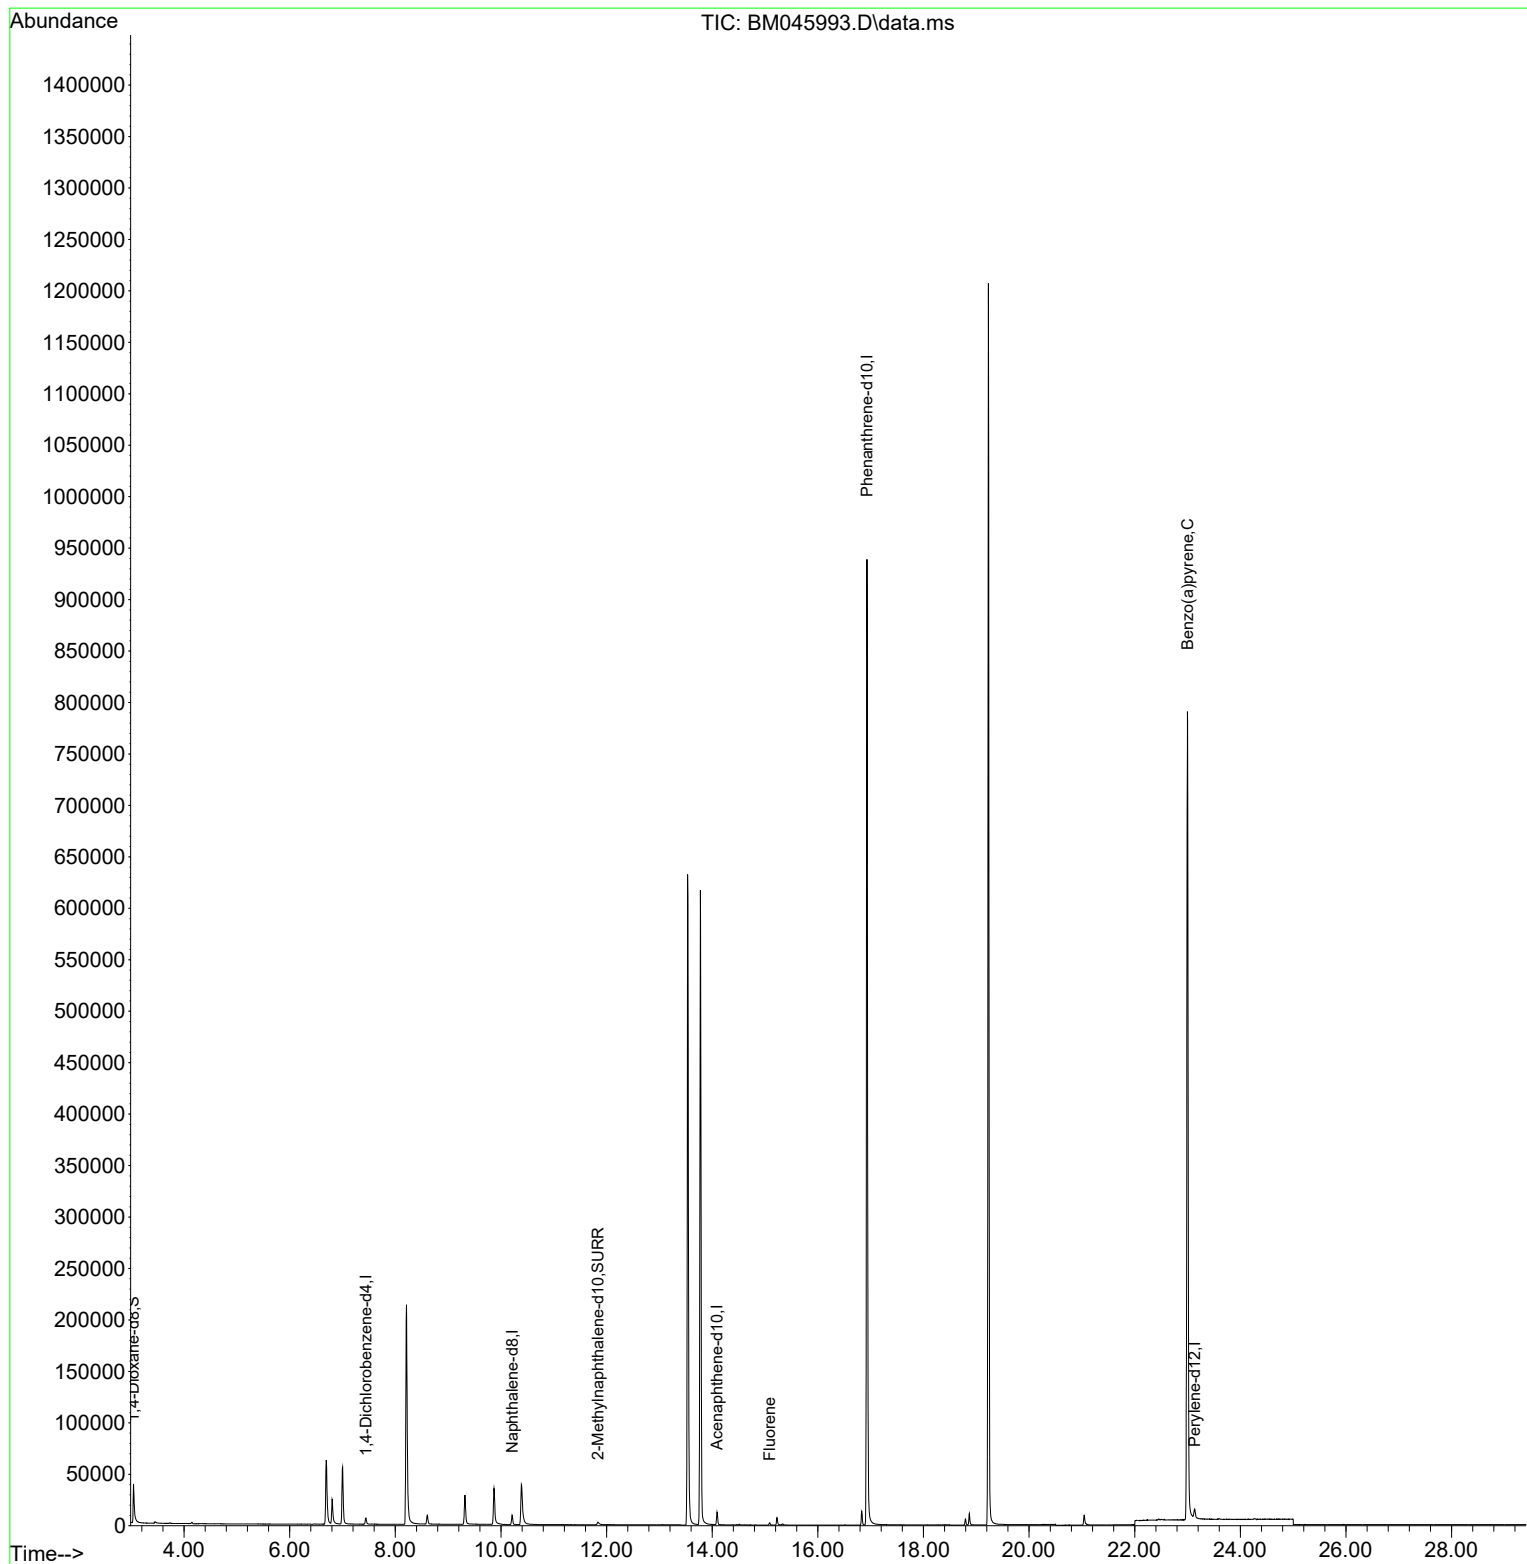


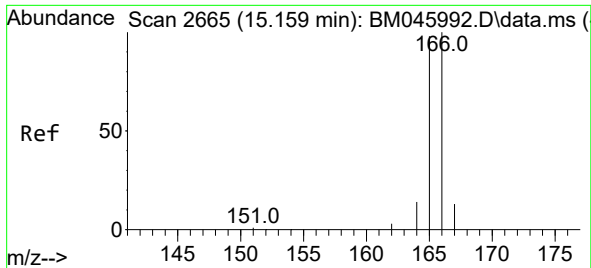

#12
Fluorene
Concen: 0.076 ng/ul
RT: 15.085 min Scan# 2649
Delta R.T. -0.074 min
Lab File: BM045993.D
Acq: 12 Jun 2024 11:26

Instrument :
BNA_M
ClientSampleId :
SBLK249

Tgt Ion:166 Resp: 1987
Ion Ratio Lower Upper
166 100
165 9.4 79.7 119.5#
167 32.5 11.3 16.9#

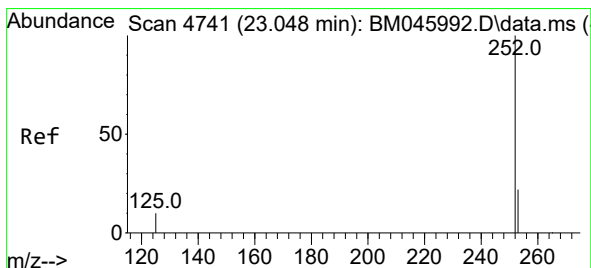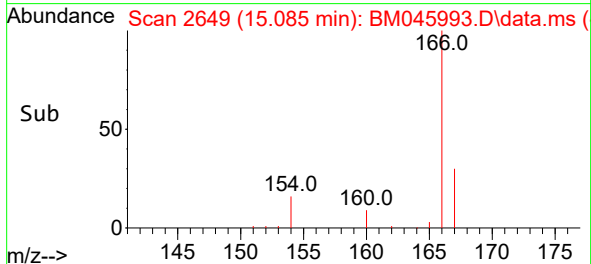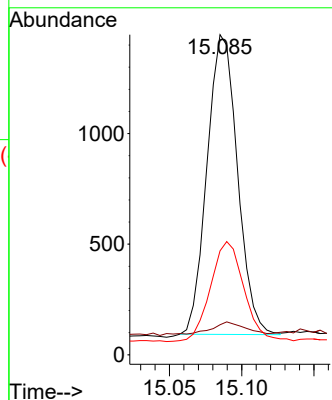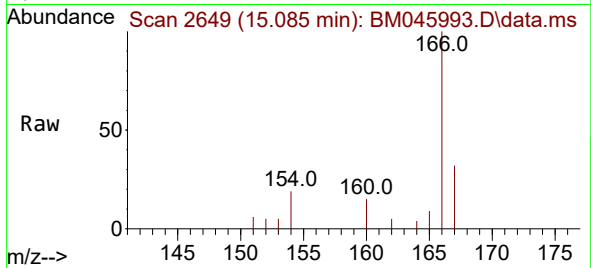

#26
Benzo(a)pyrene
Concen: 0.072 ng/ul
RT: 22.998 min Scan# 4724
Delta R.T. -0.050 min
Lab File: BM045993.D
Acq: 12 Jun 2024 11:26

Tgt Ion:252 Resp: 4004
Ion Ratio Lower Upper
252 100
253 58.1 28.8 43.2#
125 48.3 17.3 25.9#

