


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061315\
 Data File : BM001676.D
 Acq On : 12 Jun 2015 19:05
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\SIM-BM061315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 15 16:37:00 2015

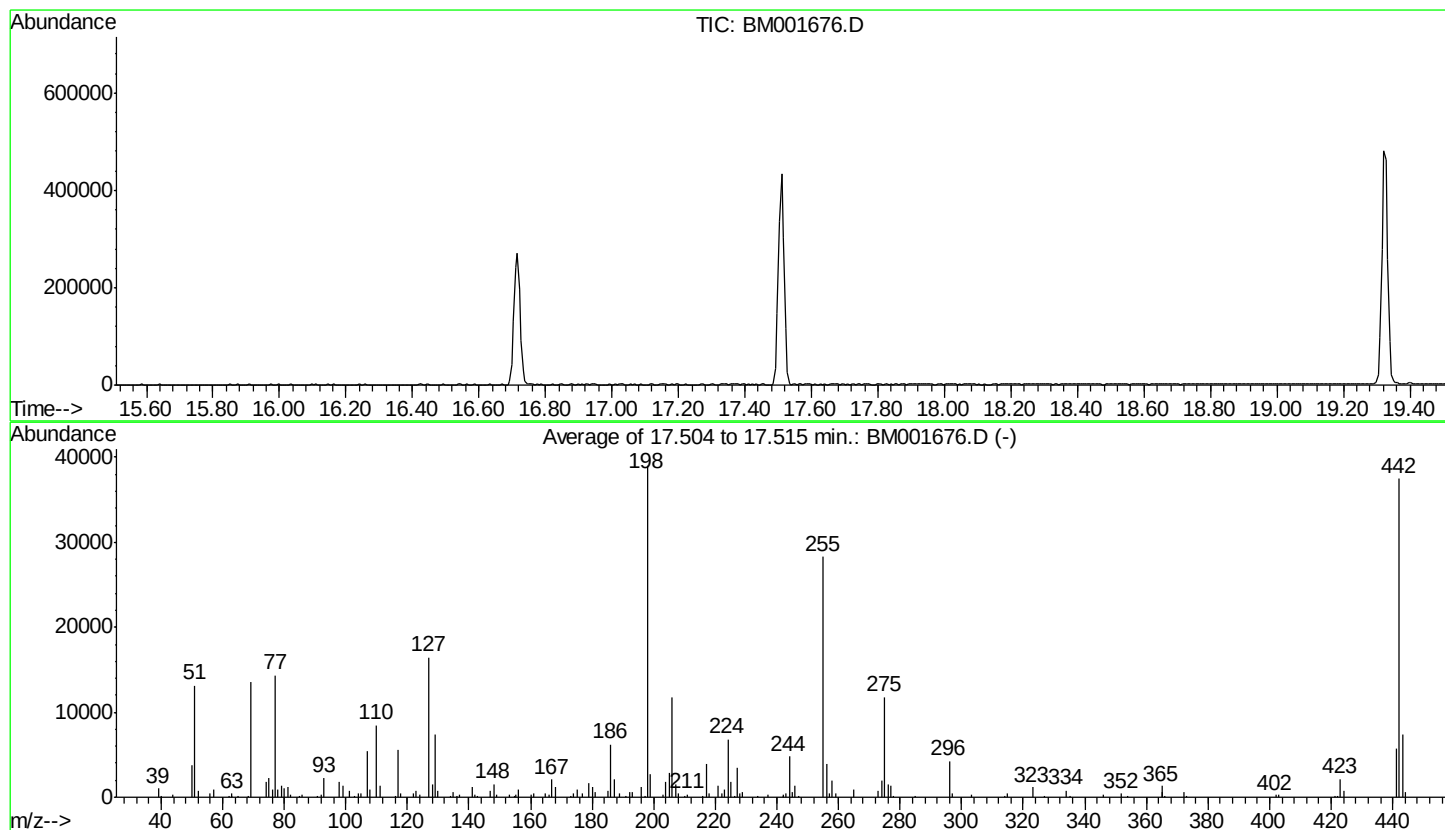

AutoFind: Scans 2519, 2520, 2521; Background Corrected with Scan 2513

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.7	13153	PASS
68	69	0.00	2	0.8	104	PASS
69	198	0.00	100	34.8	13566	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.1	16417	PASS
197	198	0.00	2	0.3	106	PASS
198	198	100	100	100.0	39013	PASS
199	198	5	9	6.9	2689	PASS
275	198	10	60	30.2	11771	PASS
365	198	1	100	3.3	1292	PASS
441	442	0.01	24	15.2	5695	PASS
442	198	50	100	96.0	37434	PASS
443	442	15	24	19.7	7367	PASS