

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061317\
 Data File : BM010562.D
 Acq On : 13 Jun 2017 16:16
 Operator : SJ/MA
 Sample : PB99725BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK25

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	7.063	670	676	683	rBV	409804	663626	14.86%	1.900%
2	7.222	696	703	711	rBV	277156	432588	9.69%	1.239%
3	7.416	730	736	746	rBV	502687	805829	18.05%	2.308%
4	7.881	807	815	821	rBV	468306	736543	16.50%	2.109%
5	8.598	929	937	947	rBV	525994	885011	19.82%	2.534%
6	9.063	1010	1016	1027	rVB	421825	695950	15.59%	1.993%
7	9.775	1129	1137	1148	rVB	406458	708554	15.87%	2.029%
8	10.304	1221	1227	1239	rBV	644627	1109357	24.84%	3.177%
9	10.681	1283	1291	1301	rVB	546859	899146	20.14%	2.575%
10	10.845	1312	1319	1329	rBV	504289	908062	20.34%	2.600%
11	13.933	1836	1844	1852	rBV	1430573	1893737	42.41%	5.423%
12	14.216	1887	1892	1900	rVB	1232262	1774225	39.73%	5.081%
13	14.421	1922	1927	1932	rBV5	27197	51006	1.14%	0.146%
14	14.521	1935	1944	1951	rVB2	795793	1265662	28.34%	3.624%
15	14.757	1978	1984	1997	rBV	544100	930582	20.84%	2.665%
16	15.510	2106	2112	2119	rVB	1693076	2400428	53.76%	6.874%
17	15.639	2128	2134	2140	rBV	609561	845304	18.93%	2.421%
18	17.268	2404	2411	2418	rVB	1205687	1736186	38.88%	4.972%
19	17.368	2421	2428	2436	rBV2	2047461	2936713	65.77%	8.410%
20	18.204	2566	2570	2575	rBV2	30750	50757	1.14%	0.145%
21	19.656	2811	2817	2823	rBV	2872627	3710608	83.10%	10.626%
22	21.439	3115	3120	3126	rVB	1873239	2449428	54.86%	7.014%
23	23.615	3484	3490	3500	rVB2	2336726	4465240	100.00%	12.787%
24	23.768	3510	3516	3525	rVB2	1359021	2566778	57.48%	7.350%


Sum of corrected areas: 34921320

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061317\
Data File : BM010562.D
Acq On : 13 Jun 2017 16:16
Operator : SJ/MA
Sample : PB99725BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
SBLK25

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

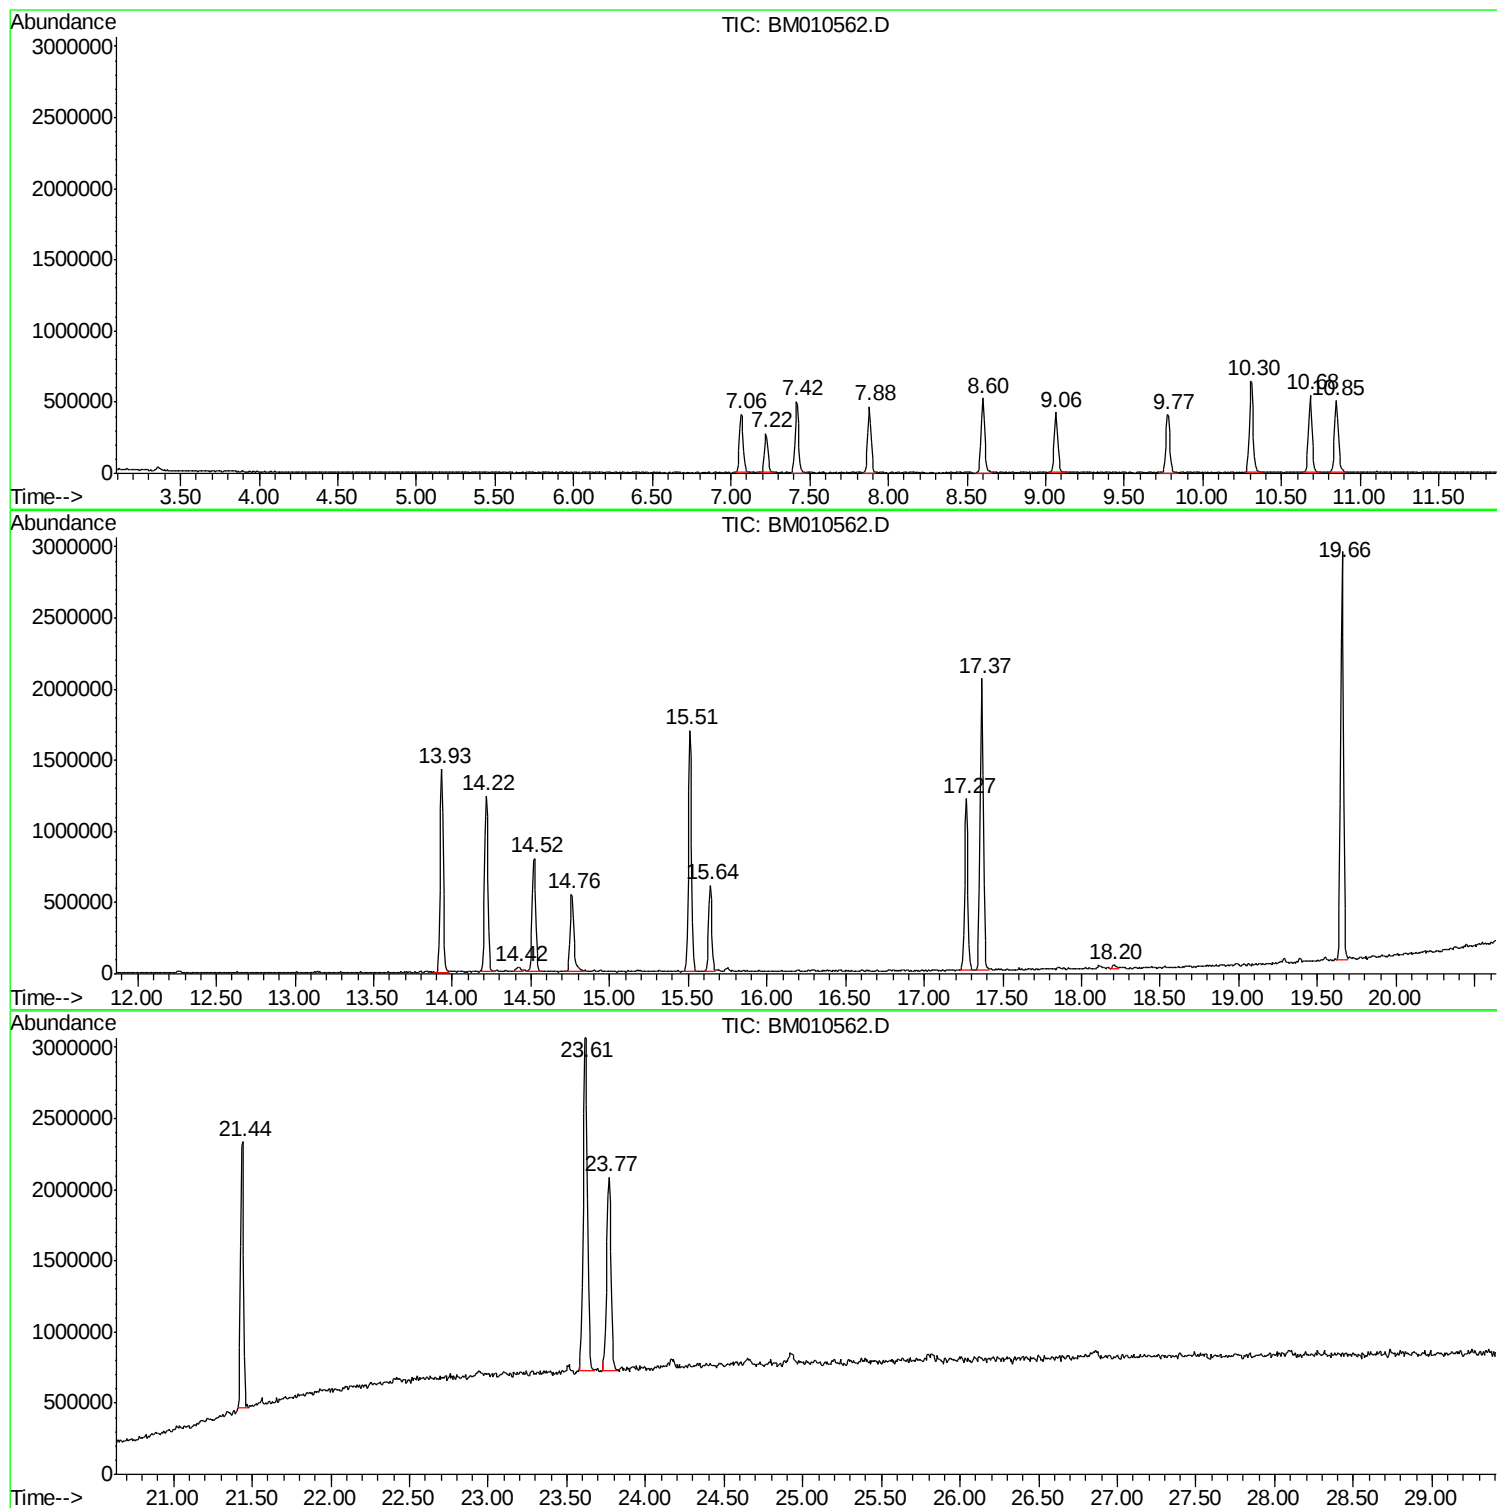

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061317\
Data File : BM010562.D
Acq On : 13 Jun 2017 16:16
Operator : SJ/MA
Sample : PB99725BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK25

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061317\
Data File : BM010562.D
Acq On : 13 Jun 2017 16:16
Operator : SJ/MA
Sample : PB99725BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK25

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc