

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061324\
 Data File : BM046003.D
 Acq On : 12 Jun 2024 19:20
 Operator : MA/JU
 Sample : PB161309BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK309

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM046003.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.040	5	9	18	rVB	35004	54271	1.49%	0.133%
2	3.446	75	78	114	rBV	388424	933043	25.58%	2.282%
3	4.146	193	197	205	rVB2	21653	34553	0.95%	0.085%
4	5.440	414	417	421	rBV5	1994	4012	0.11%	0.010%
5	6.587	609	612	614	rBV3	4577	3951	0.11%	0.010%
6	6.687	622	629	642	rBV	608948	1164952	31.93%	2.850%
7	6.798	643	648	671	rVV	432584	838233	22.98%	2.050%
8	6.993	674	681	699	rVB	645208	1121117	30.73%	2.742%
9	7.281	727	730	733	rBV3	3107	3733	0.10%	0.009%
10	7.434	749	756	773	rBV	536560	910031	24.95%	2.226%
11	8.204	880	887	903	rBV	743201	1348802	36.97%	3.299%
12	8.598	948	954	966	rBV	683767	1191016	32.65%	2.913%
13	9.222	1055	1060	1065	rBV8	4323	8762	0.24%	0.021%
14	9.310	1068	1075	1094	rVV	553731	980362	26.87%	2.398%
15	9.863	1162	1169	1194	rBV	658215	1361359	37.32%	3.330%
16	10.204	1220	1227	1241	rBV	768660	1317892	36.13%	3.224%
17	10.386	1251	1258	1281	rBV	571188	1422780	39.00%	3.480%
18	11.827	1497	1503	1510	rBV8	6988	18146	0.50%	0.044%
19	13.057	1705	1712	1714	rBV7	2291	4260	0.12%	0.010%
20	13.533	1786	1793	1809	rBV	1240050	1964513	53.85%	4.806%
21	13.769	1825	1833	1848	rBV	1481747	2323400	63.69%	5.683%
22	14.080	1879	1886	1894	rBV	1211635	1774037	48.63%	4.340%
23	14.380	1931	1937	1957	rBV	558256	1147542	31.46%	2.807%
24	15.080	2049	2056	2075	rBV	1900285	2797945	76.70%	6.844%
25	15.221	2075	2080	2094	rVV	648683	933450	25.59%	2.283%
26	15.327	2094	2098	2102	rVB6	8911	14011	0.38%	0.034%
27	16.621	2315	2318	2321	rVB4	4254	4709	0.13%	0.012%
28	16.827	2346	2353	2363	rBV	1629005	2173571	59.58%	5.317%
29	16.927	2363	2370	2387	rVV	2106646	3117850	85.47%	7.627%
30	18.380	2615	2617	2620	rVB4	4317	3707	0.10%	0.009%
31	18.792	2681	2687	2693	rBV4	27048	45143	1.24%	0.110%
32	18.862	2695	2699	2705	rVV	23187	34027	0.93%	0.083%
33	19.145	2745	2747	2749	rBV3	3931	3915	0.11%	0.010%
34	19.227	2751	2761	2770	rBV	2772998	3647917	100.00%	8.923%
35	21.039	3064	3069	3083	rBV	1588480	2382209	65.30%	5.827%
36	23.556	3489	3497	3513	rBV2	1516200	3312773	90.81%	8.104%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061324\
Data File : BM046003.D
Acq On : 12 Jun 2024 19:20
Operator : MA/JU
Sample : PB161309BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK309

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
Title : SVOA CALIBRATION

37	23.744	3521	3529	3544	rVB	1045937	2478245	67.94%	6.062%
----	--------	------	------	------	-----	---------	---------	--------	--------




Sum of corrected areas: 40880239

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061324\
Data File : BM046003.D
Acq On : 12 Jun 2024 19:20
Operator : MA/JU
Sample : PB161309BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK309

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

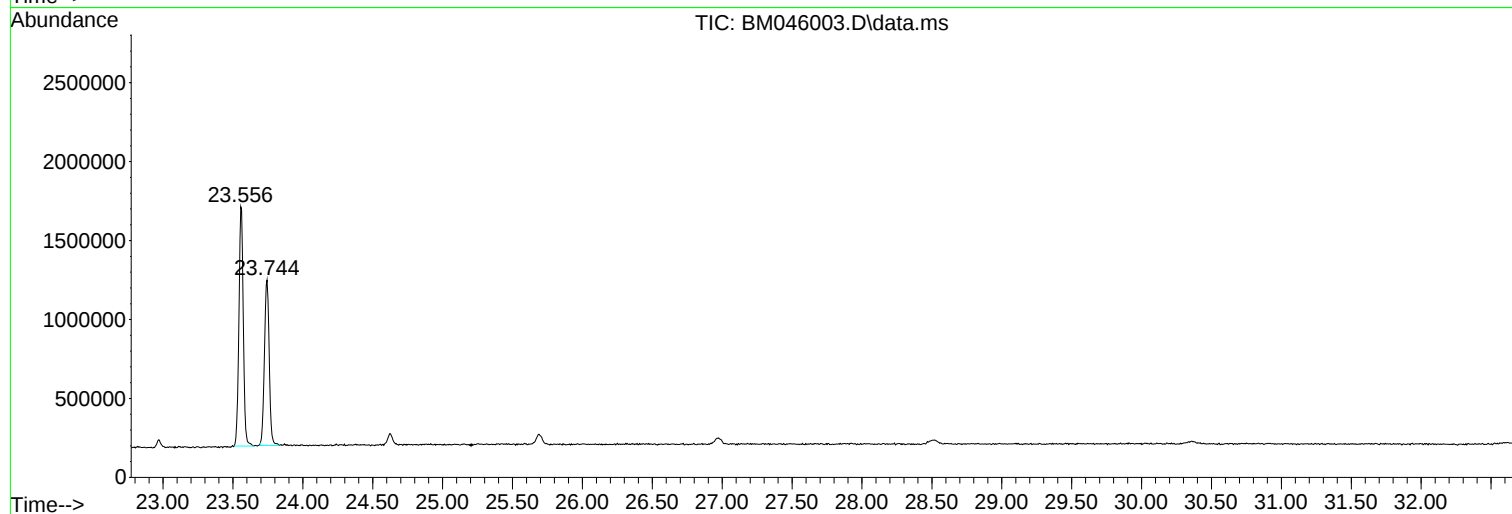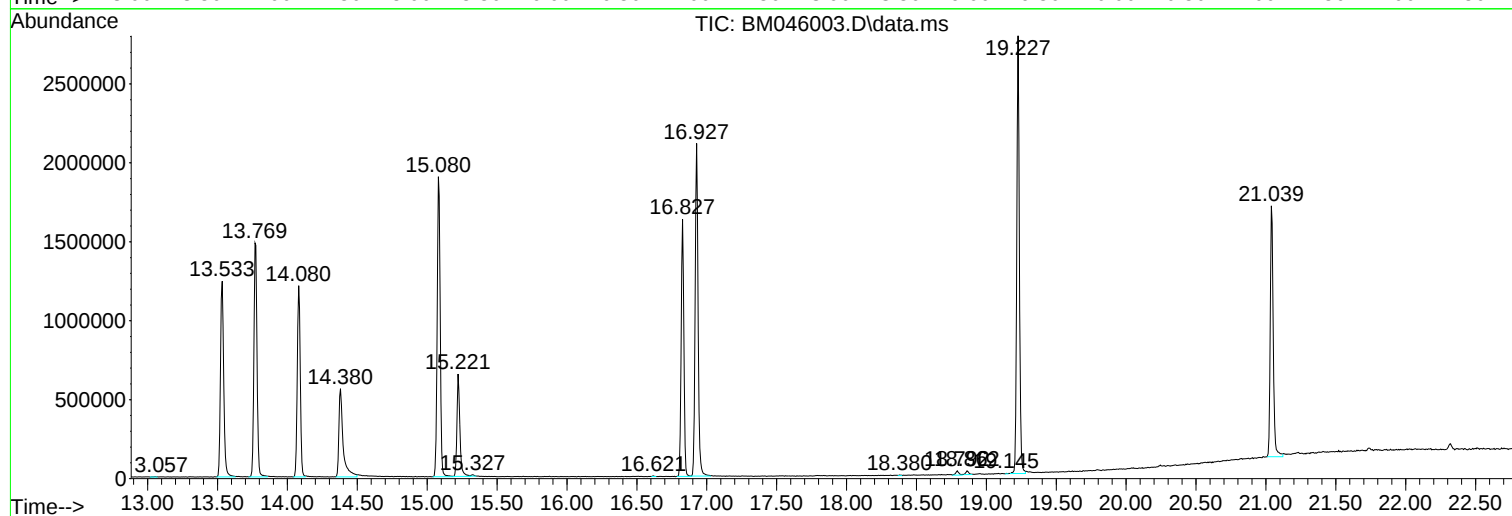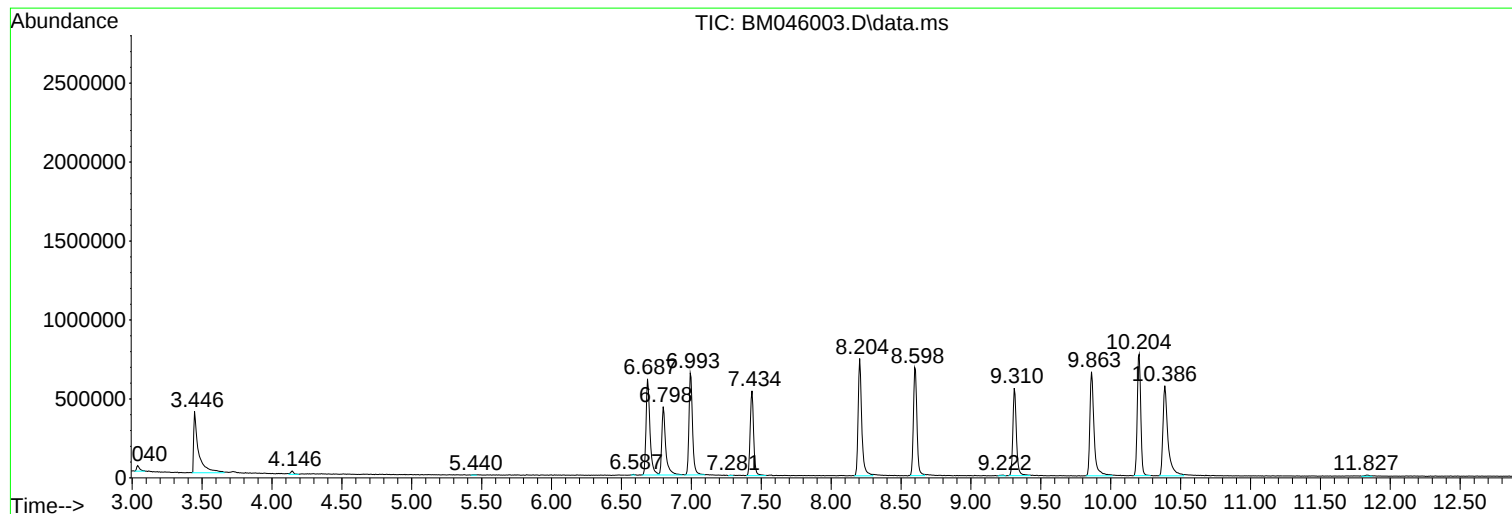

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061324\
Data File : BM046003.D
Acq On : 12 Jun 2024 19:20
Operator : MA/JU
Sample : PB161309BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK309

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061324\
Data File : BM046003.D
Acq On : 12 Jun 2024 19:20
Operator : MA/JU
Sample : PB161309BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK309

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc