

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061325\
 Data File : BM050312.D
 Acq On : 13 Jun 2025 23:03
 Operator : RC/JU
 Sample : Q2296-24
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 WC-6

Quant Time: Jun 14 00:41:20 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 09 11:54:38 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.763	152	352982	20.000	ng	0.00
21) Naphthalene-d8	10.546	136	1314559	20.000	ng	#-0.01
39) Acenaphthene-d10	14.392	164	678439	20.000	ng	0.00
64) Phenanthrene-d10	17.128	188	1295277	20.000	ng	-0.01
76) Chrysene-d12	21.357	240	1355341	20.000	ng	-0.02
86) Perylene-d12	24.327	264	855453	20.000	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.358	112	3009388	142.219	ng	0.00
7) Phenol-d6	6.928	99	3301050	118.507	ng	0.00
23) Nitrobenzene-d5	8.910	82	2580209	102.081	ng	0.00
42) 2,4,6-Tribromophenol	15.875	330	1130724	146.528	ng	0.00
45) 2-Fluorobiphenyl	13.016	172	4848170	96.747	ng	-0.01
79) Terphenyl-d14	19.757	244	6717832	93.928	ng	-0.01


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061325\
Data File : BM050312.D
Acq On : 13 Jun 2025 23:03
Operator : RC/JU
Sample : Q2296-24
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
WC-6


Quant Time: Jun 14 00:41:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

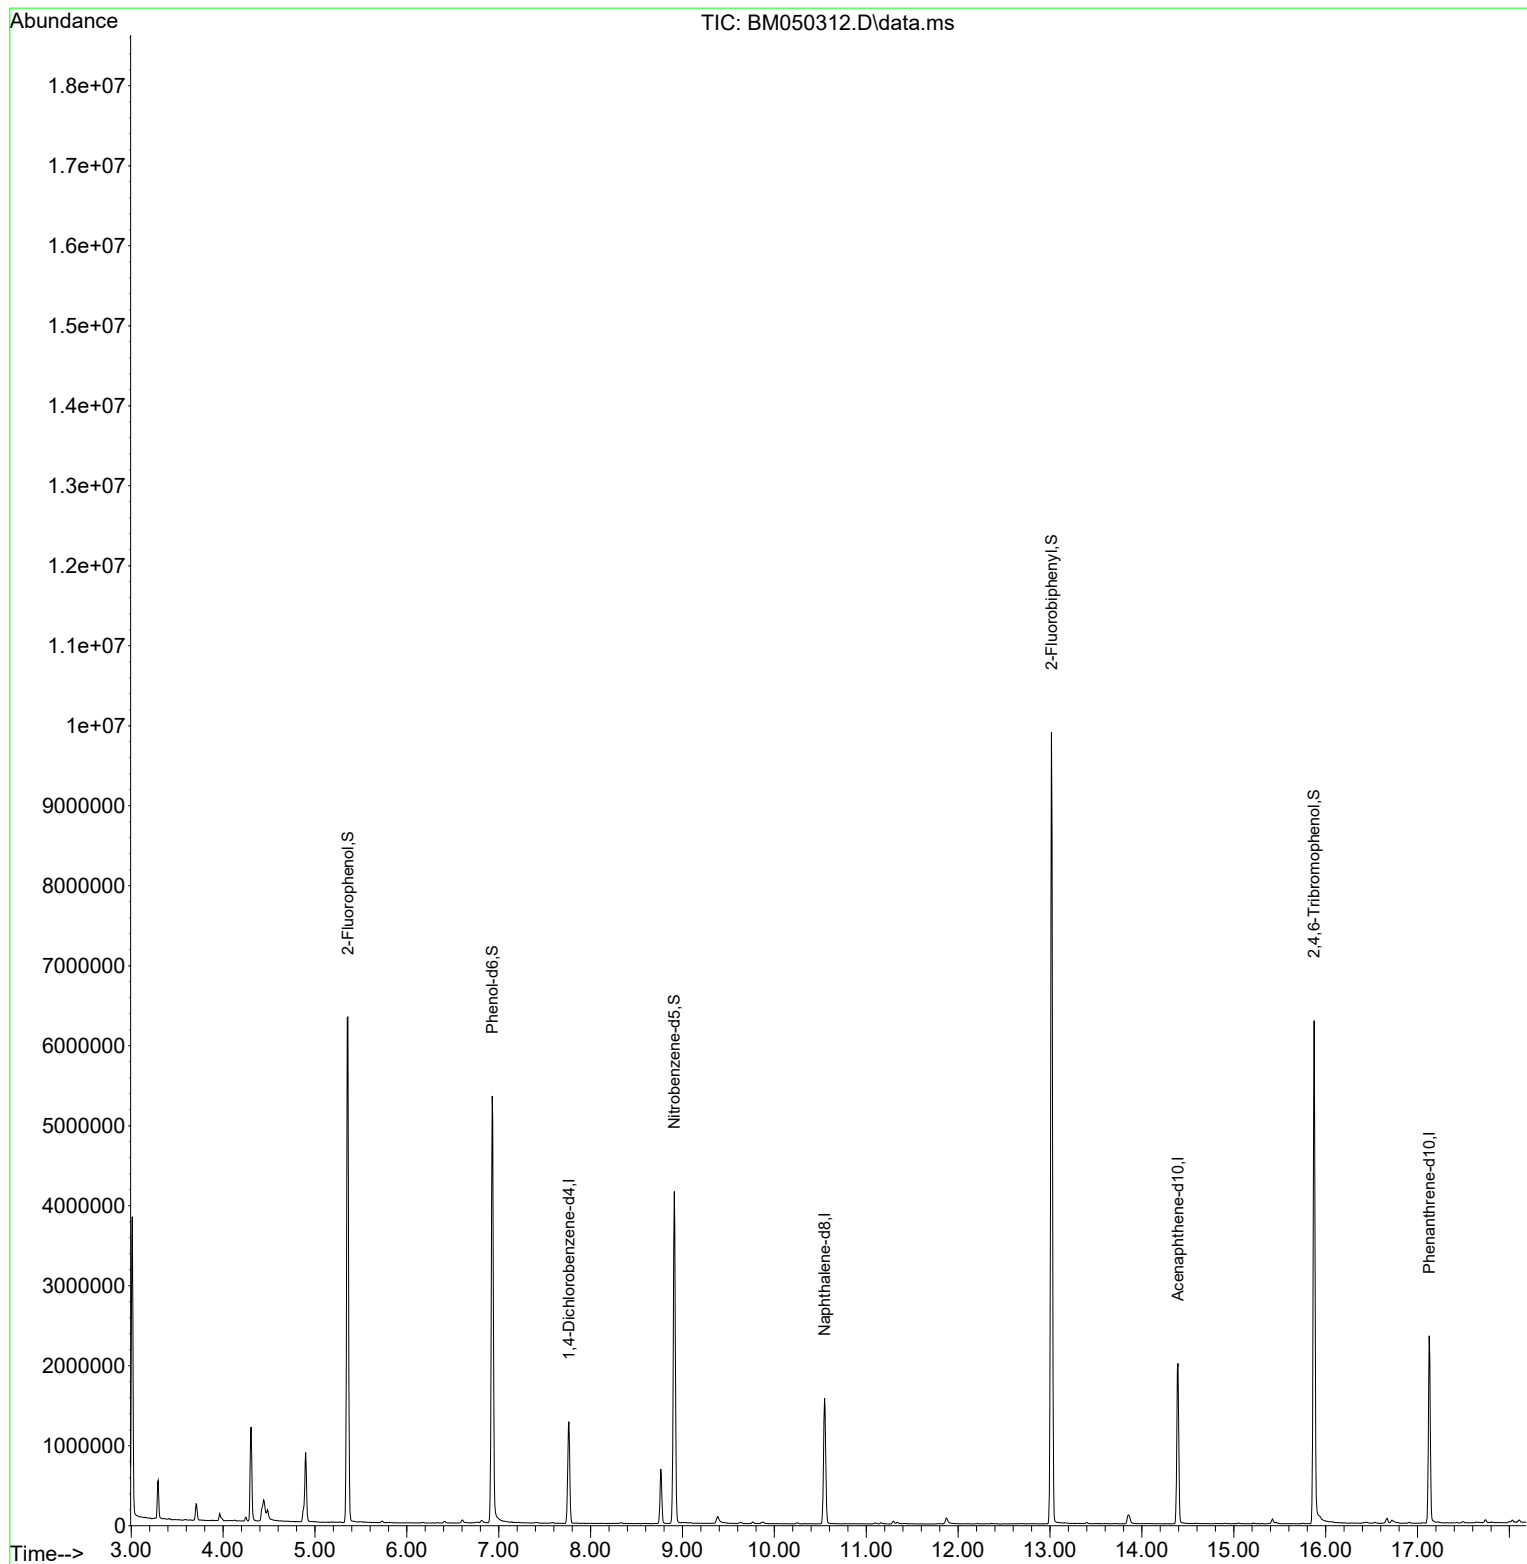


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061325\
Data File : BM050312.D
Acq On : 13 Jun 2025 23:03
Operator : RC/JU
Sample : Q2296-24
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
WC-6

Quant Time: Jun 14 00:41:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration




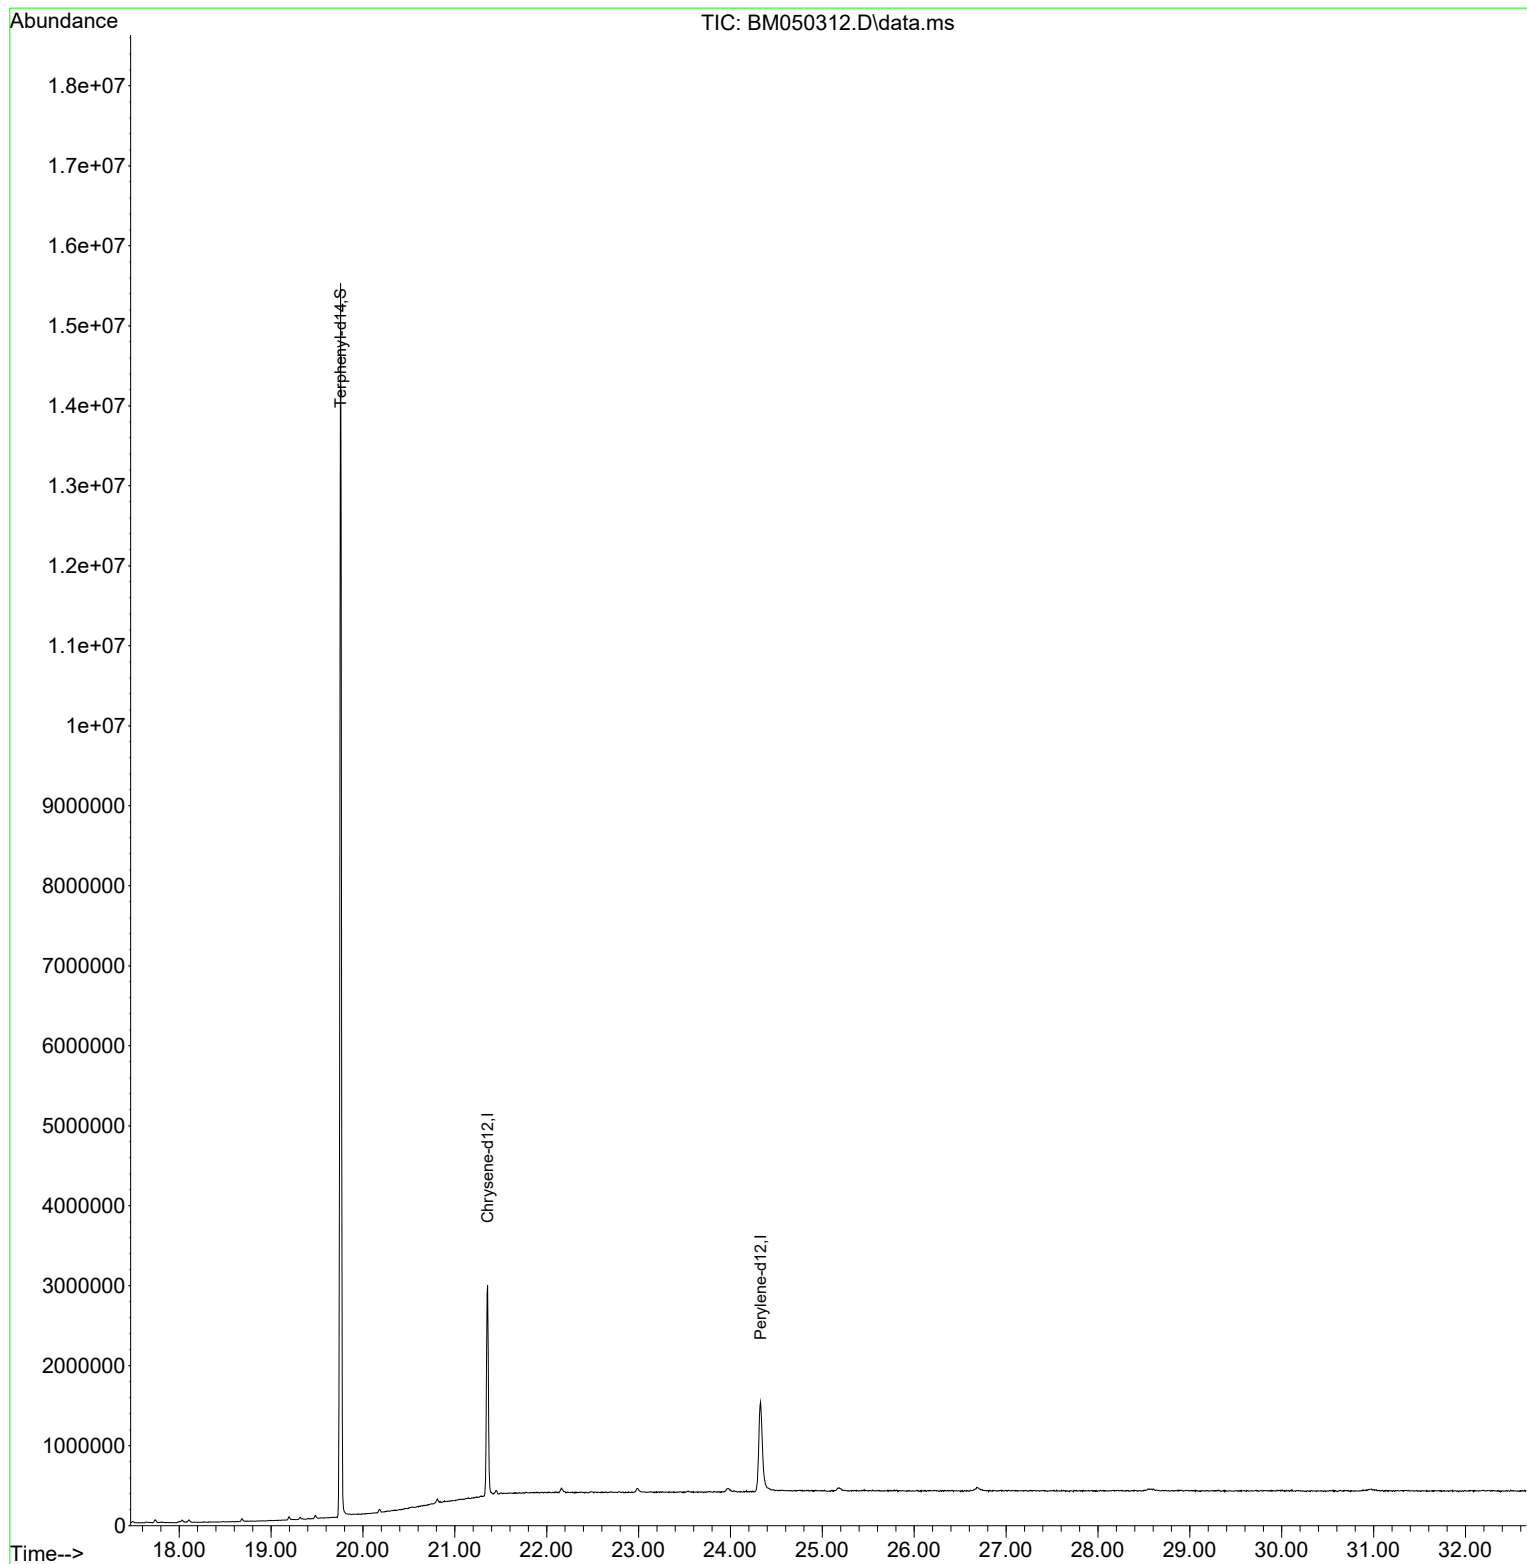


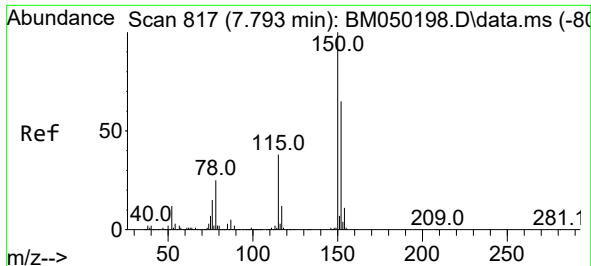

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.763 min Scan# 817
Delta R.T. -0.006 min
Lab File: BM050312.D
Acq: 13 Jun 2025 23:03




Instrument :
BNA_M
ClientSampleId :
WC-6


Tgt Ion:152 Resp: 352982
Ion Ratio Lower Upper
152 100
150 156.5 122.2 183.4
115 60.0 46.3 69.5

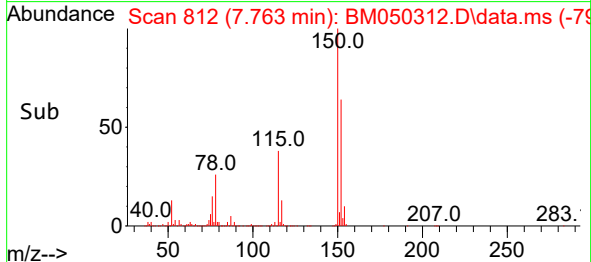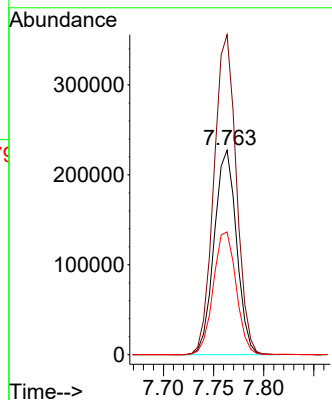

#5
2-Fluorophenol
Concen: 142.219 ng
RT: 5.358 min Scan# 403
Delta R.T. 0.000 min
Lab File: BM050312.D
Acq: 13 Jun 2025 23:03

Tgt Ion:112 Resp: 3009388
Ion Ratio Lower Upper
112 100
64 51.6 39.8 59.6
63 25.9 19.8 29.8


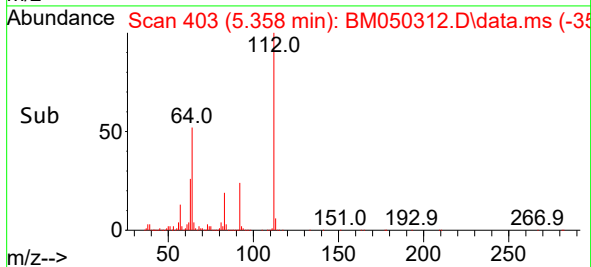
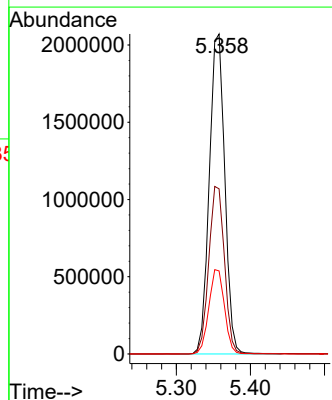
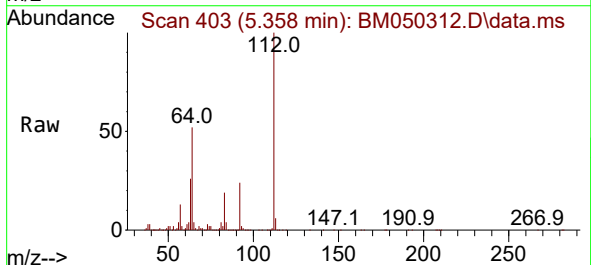


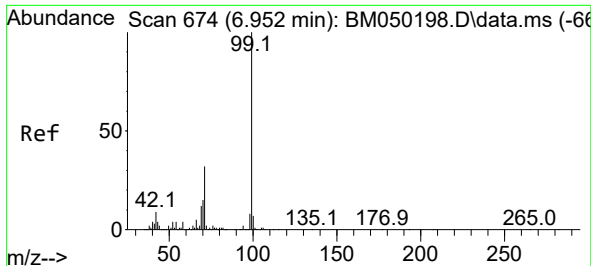

#7
Phenol-d6
Concen: 118.507 ng
RT: 6.928 min Scan# 61
Delta R.T. -0.005 min
Lab File: BM050312.D
Acq: 13 Jun 2025 23:03




Instrument :
BNA_M
ClientSampleId :
WC-6


Tgt Ion: 99 Resp: 3301050
Ion Ratio Lower Upper
99 100
42 9.0 6.9 10.3
71 33.4 25.3 37.9

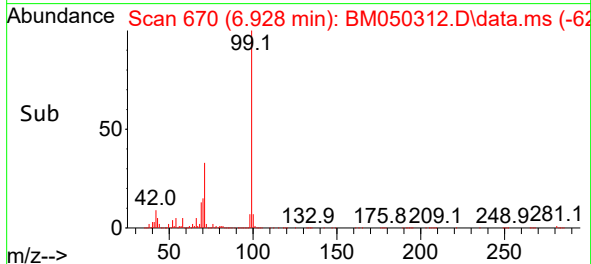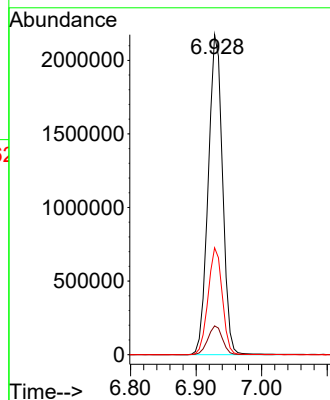

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.546 min Scan# 1285
Delta R.T. -0.011 min
Lab File: BM050312.D
Acq: 13 Jun 2025 23:03

Tgt Ion: 136 Resp: 1314559
Ion Ratio Lower Upper
136 100
137 10.6 8.6 13.0
54 5.8 3.8 5.8#
68 6.3 4.9 7.3


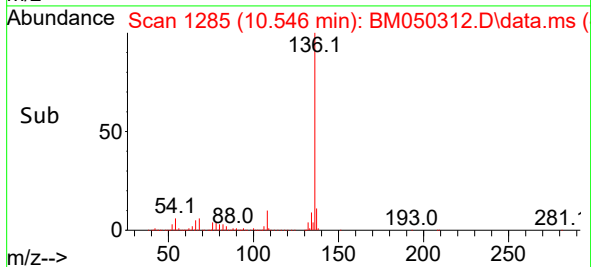
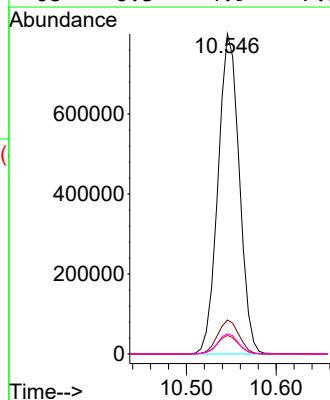
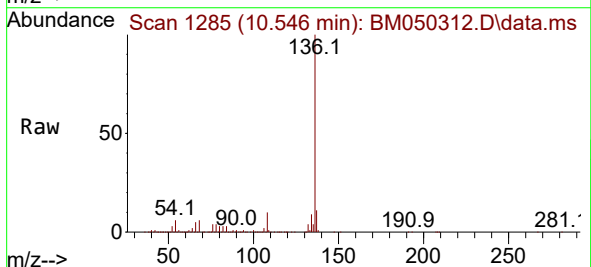




#23
 Nitrobenzene-d5
 Concen: 102.081 ng
 RT: 8.910 min Scan# 1012
 Delta R.T. -0.005 min
 Lab File: BM050312.D
 Acq: 13 Jun 2025 23:03




Instrument :
 BNA_M
 ClientSampleId :
 WC-6


Tgt Ion: 82 Resp: 2580209
 Ion Ratio Lower Upper
 82 100
 128 41.3 35.2 52.8
 54 32.4 24.5 36.7

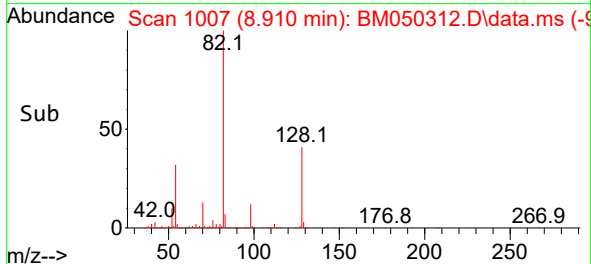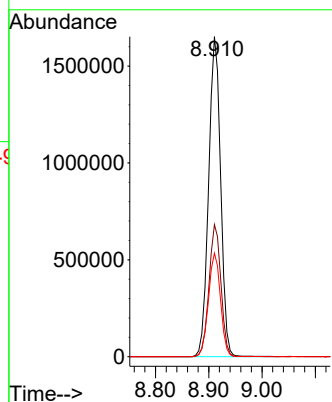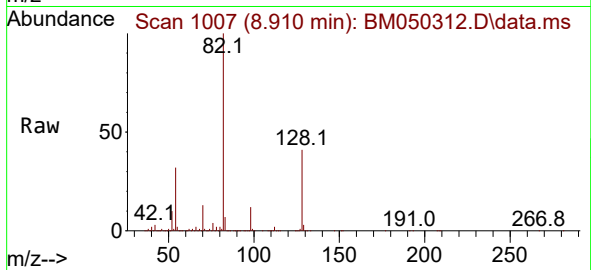

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.392 min Scan# 1939
 Delta R.T. -0.005 min
 Lab File: BM050312.D
 Acq: 13 Jun 2025 23:03

Tgt Ion:164 Resp: 678439
 Ion Ratio Lower Upper
 164 100
 162 101.5 80.2 120.4
 160 48.1 35.7 53.5


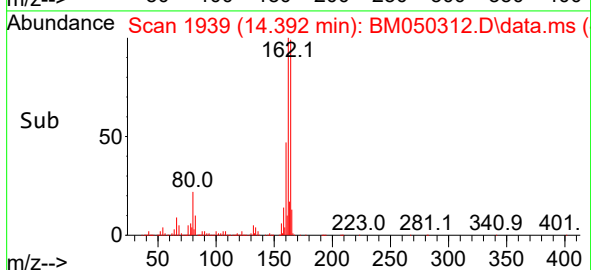
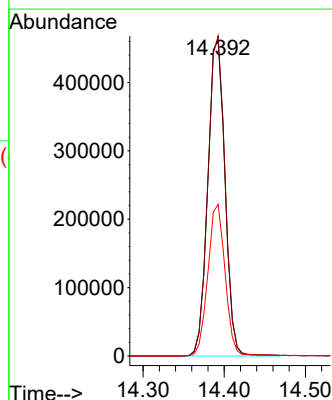
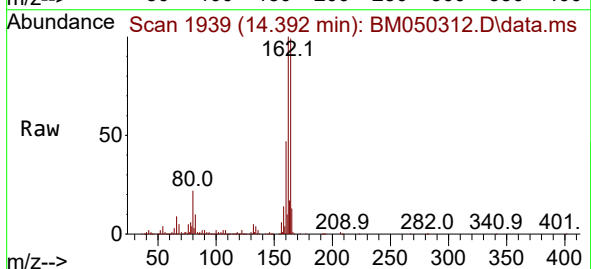


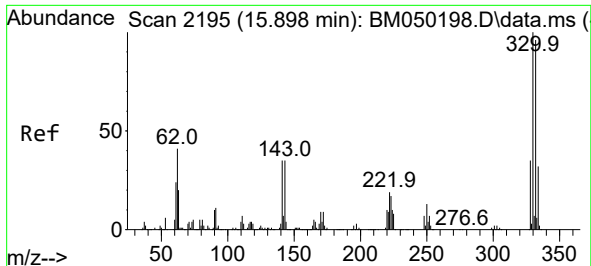

#42
 2,4,6-Tribromophenol
 Concen: 146.528 ng
 RT: 15.875 min Scan# 2191
 Delta R.T. -0.005 min
 Lab File: BM050312.D
 Acq: 13 Jun 2025 23:03




Instrument :
 BNA_M
 ClientSampleId :
 WC-6


Tgt Ion:330 Resp: 1130724
 Ion Ratio Lower Upper
 330 100
 332 96.6 77.5 116.3
 141 39.5 28.8 43.2

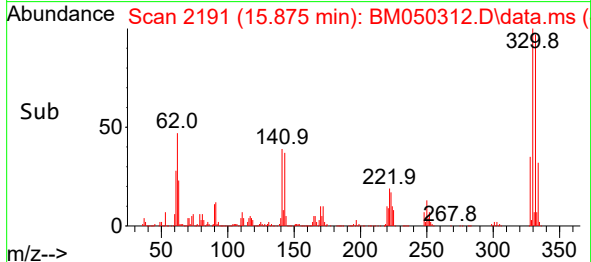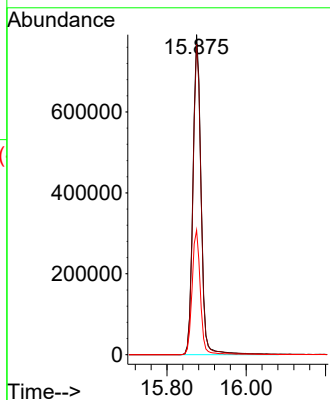

#45
 2-Fluorobiphenyl
 Concen: 96.747 ng
 RT: 13.016 min Scan# 1705
 Delta R.T. -0.011 min
 Lab File: BM050312.D
 Acq: 13 Jun 2025 23:03

Tgt Ion:172 Resp: 4848170
 Ion Ratio Lower Upper
 172 100
 171 34.6 27.8 41.6
 170 23.3 18.6 27.8


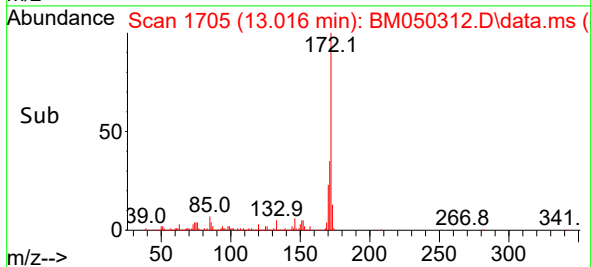
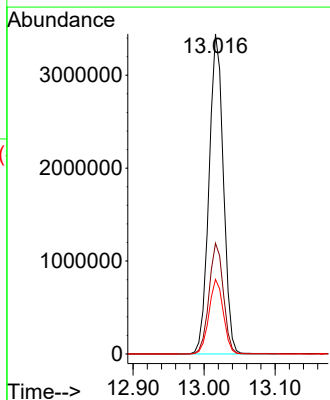
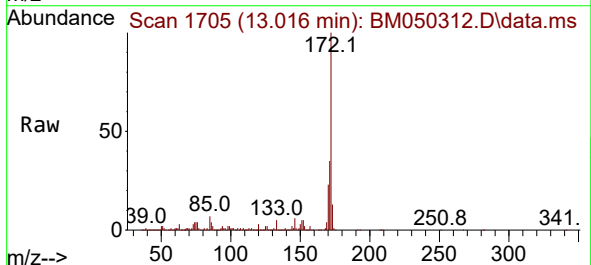


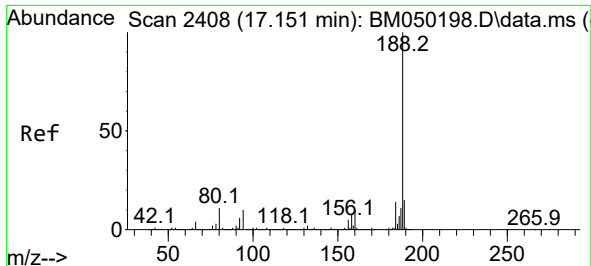

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.128 min Scan# 2404
Delta R.T. -0.011 min
Lab File: BM050312.D
Acq: 13 Jun 2025 23:03




Instrument :
BNA_M
ClientSampleId :
WC-6


Tgt Ion:188 Resp: 1295277
Ion Ratio Lower Upper
188 100
94 10.9 8.1 12.1
80 12.0 8.6 13.0

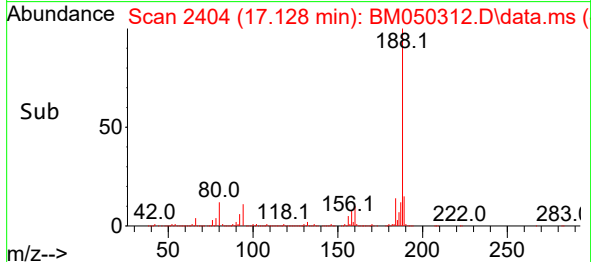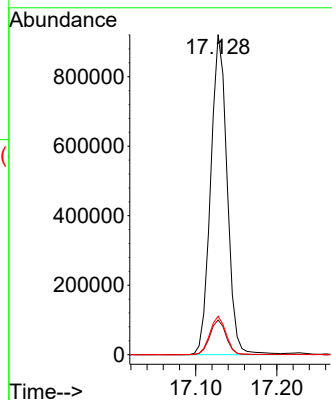

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.357 min Scan# 3123
Delta R.T. -0.017 min
Lab File: BM050312.D
Acq: 13 Jun 2025 23:03

Tgt Ion:240 Resp: 1355341
Ion Ratio Lower Upper
240 100
120 11.6 9.0 13.4
236 25.0 20.7 31.1


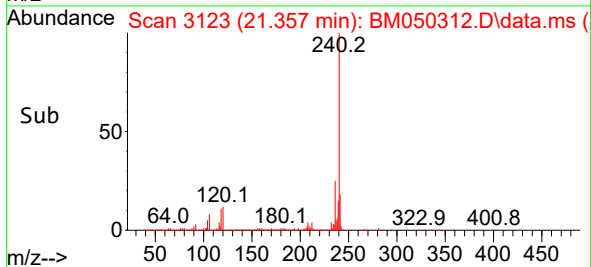
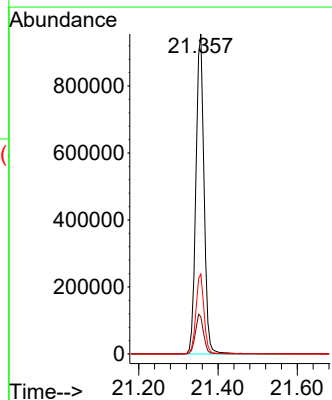
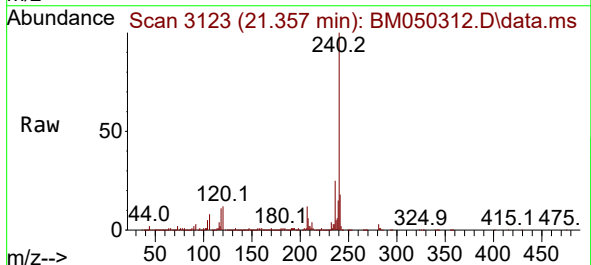




#79
 Terphenyl-d14
 Concen: 93.928 ng
 RT: 19.757 min Scan# 21
 Delta R.T. -0.011 min
 Lab File: BM050312.D
 Acq: 13 Jun 2025 23:03

Instrument :
 BNA_M
 ClientSampleId :
 WC-6

Tgt Ion:244 Resp: 6717832
 Ion Ratio Lower Upper
 244 100
 212 7.2 6.0 9.0
 122 11.5 8.6 12.8

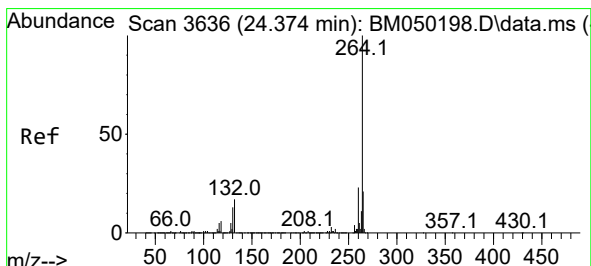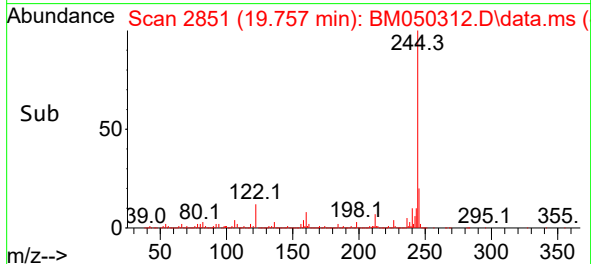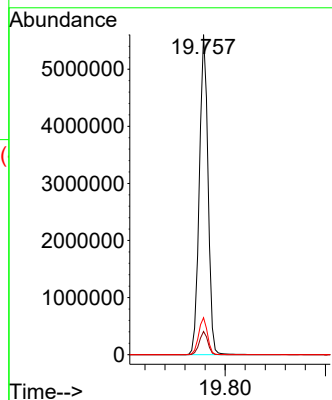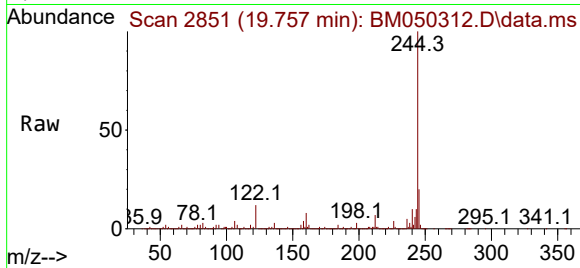

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 24.327 min Scan# 3628
 Delta R.T. -0.017 min
 Lab File: BM050312.D
 Acq: 13 Jun 2025 23:03

Tgt Ion:264 Resp: 855453
 Ion Ratio Lower Upper
 264 100
 260 25.6 18.6 28.0
 265 21.1 16.8 25.2

