

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061325\
 Data File : BM050302.D
 Acq On : 13 Jun 2025 16:31
 Operator : RC/JU
 Sample : Q2287-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CONCRETE-SLAB

Quant Time: Jun 13 18:05:11 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 09 11:54:38 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.763	152	448758	20.000	ng	0.00
21) Naphthalene-d8	10.545	136	1702322	20.000	ng	-0.01
39) Acenaphthene-d10	14.392	164	953364	20.000	ng	0.00
64) Phenanthrene-d10	17.133	188	1772941	20.000	ng	0.00
76) Chrysene-d12	21.362	240	1833717	20.000	ng	-0.01
86) Perylene-d12	24.333	264	1904952	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.357	112	3629051	134.901	ng	0.00
7) Phenol-d6	6.928	99	4193315	118.410	ng	0.00
23) Nitrobenzene-d5	8.910	82	2992541	91.426	ng	0.00
42) 2,4,6-Tribromophenol	15.880	330	1547586	142.716	ng	0.00
45) 2-Fluorobiphenyl	13.016	172	5920963	84.082	ng	-0.01
79) Terphenyl-d14	19.762	244	8321033	85.992	ng	0.00
Target Compounds						
32) Benzoic acid	9.851	122	581353	35.036	ng	Qvalue 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061325\
Data File : BM050302.D
Acq On : 13 Jun 2025 16:31
Operator : RC/JU
Sample : Q2287-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CONCRETE-SLAB

Quant Time: Jun 13 18:05:11 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

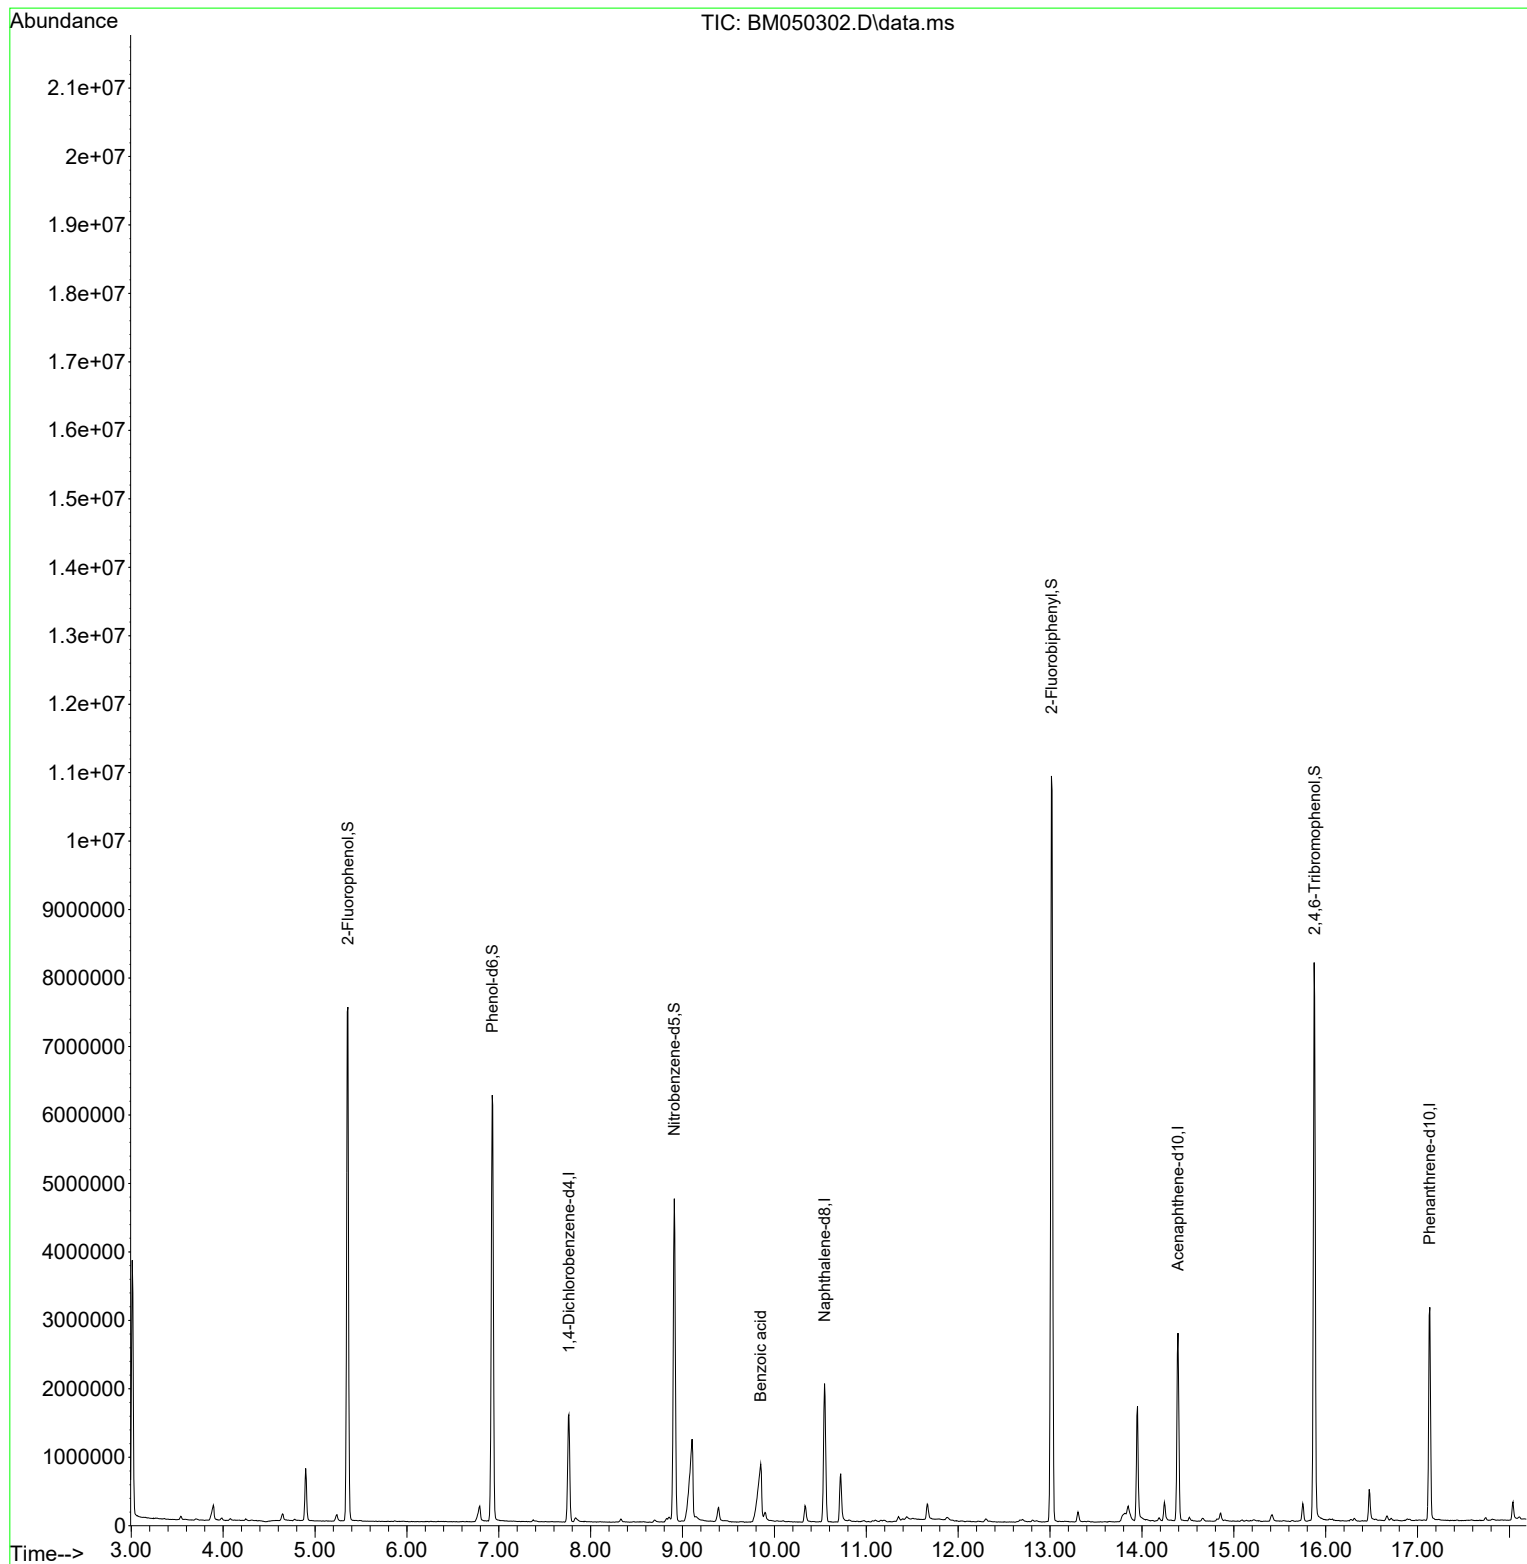

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061325\
Data File : BM050302.D
Acq On : 13 Jun 2025 16:31
Operator : RC/JU
Sample : Q2287-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CONCRETE-SLAB

Quant Time: Jun 13 18:05:11 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

