

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061325\
 Data File : BM050305.D
 Acq On : 13 Jun 2025 18:29
 Operator : RC/JU
 Sample : Q2295-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 TP01-MH1-WC

Quant Time: Jun 13 23:19:58 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 09 11:54:38 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.763	152	426179	20.000	ng	0.00
21) Naphthalene-d8	10.545	136	1570236	20.000	ng	-0.01
39) Acenaphthene-d10	14.392	164	848155	20.000	ng	0.00
64) Phenanthrene-d10	17.127	188	1649184	20.000	ng	-0.01
76) Chrysene-d12	21.356	240	1661619	20.000	ng	-0.02
86) Perylene-d12	24.327	264	990702	20.000	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.357	112	3570907	139.772	ng	0.00
7) Phenol-d6	6.934	99	4113999	122.325	ng	0.00
23) Nitrobenzene-d5	8.910	82	2875456	95.239	ng	0.00
42) 2,4,6-Tribromophenol	15.874	330	1521361	157.700	ng	0.00
45) 2-Fluorobiphenyl	13.016	172	5883405	93.913	ng	-0.01
79) Terphenyl-d14	19.756	244	7948761	90.653	ng	-0.01
Target Compounds						
50) Dimethylphthalate	13.851	163	172413	3.006	ng	Qvalue 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061325\
Data File : BM050305.D
Acq On : 13 Jun 2025 18:29
Operator : RC/JU
Sample : Q2295-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TP01-MH1-WC

Quant Time: Jun 13 23:19:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

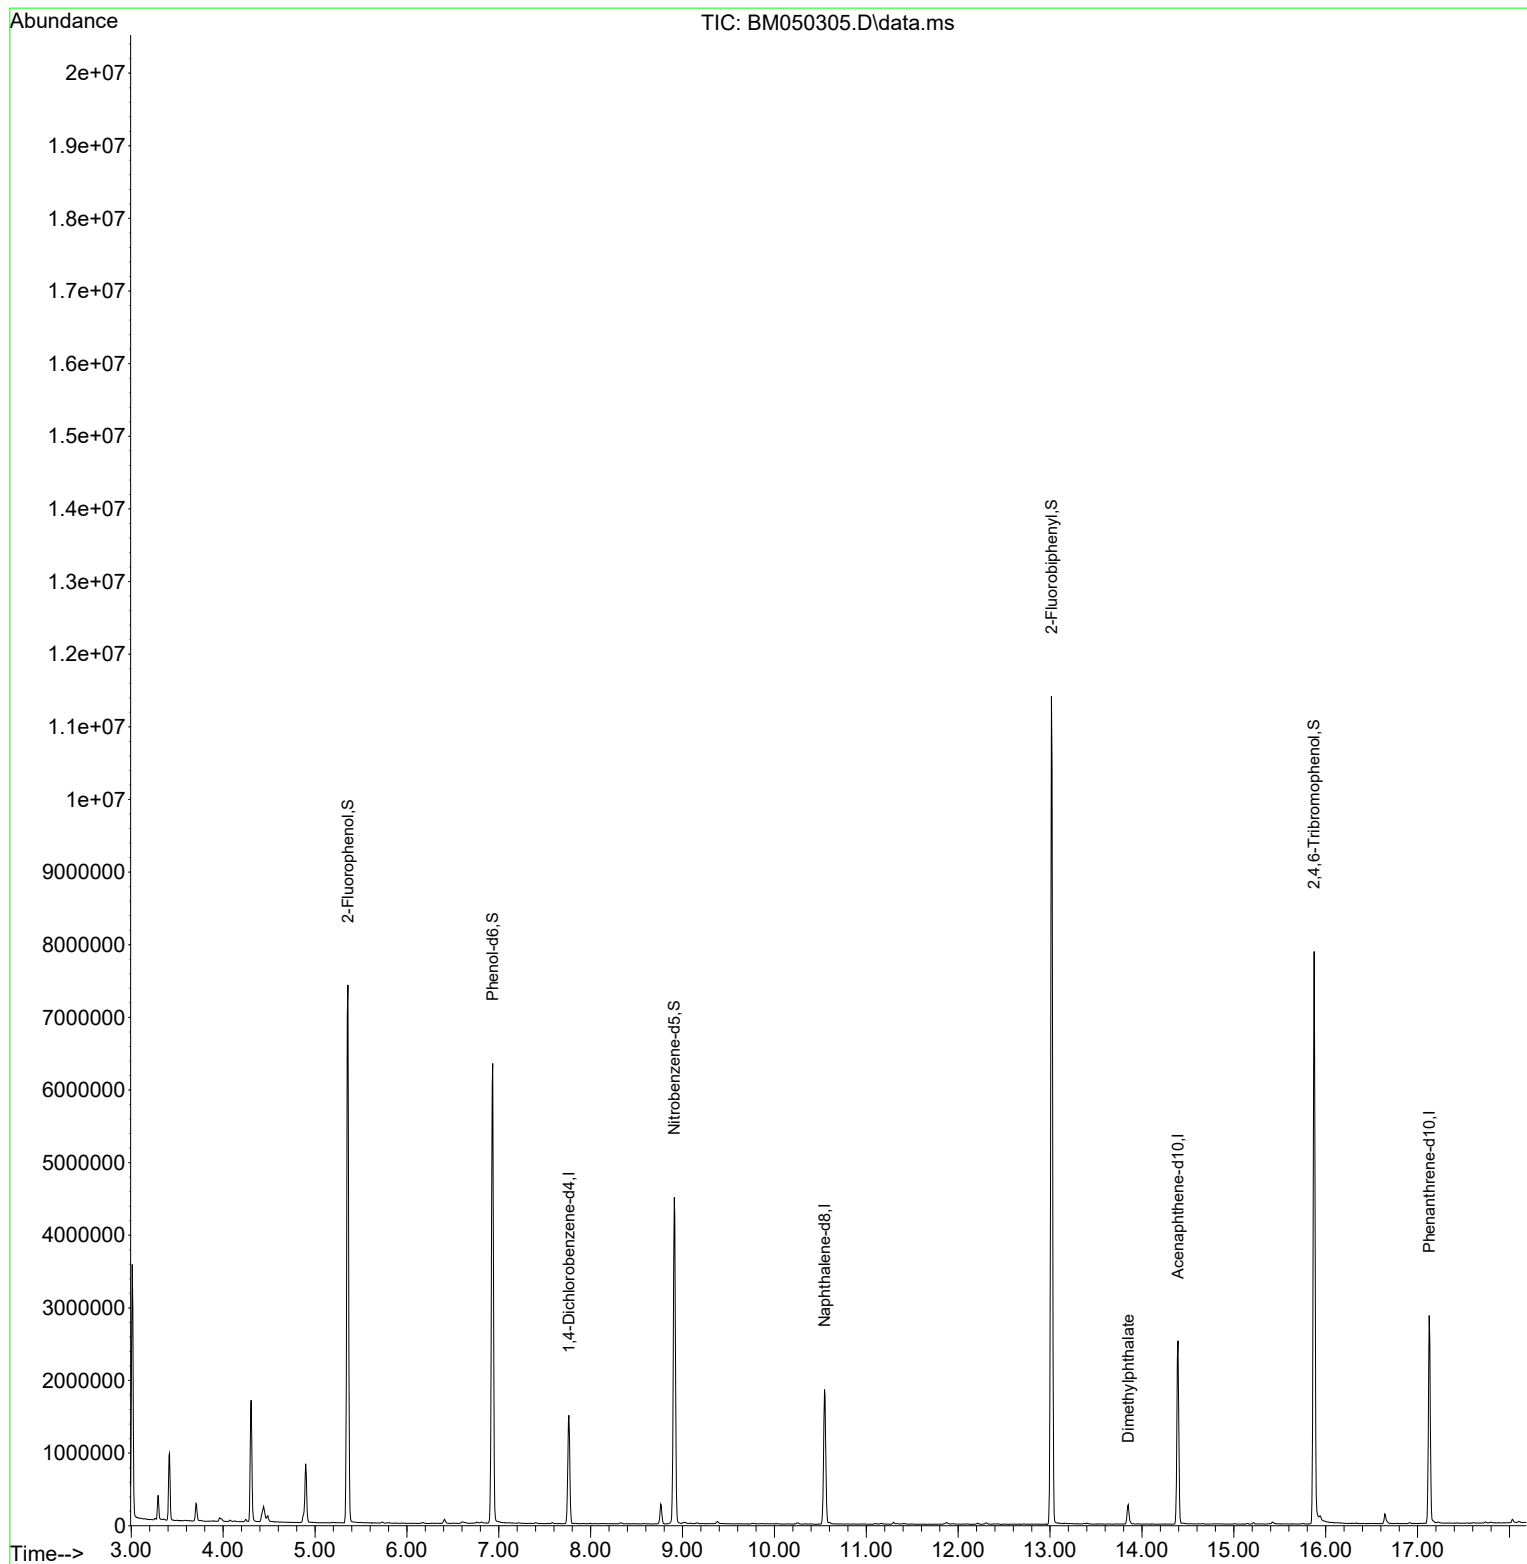

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061325\
Data File : BM050305.D
Acq On : 13 Jun 2025 18:29
Operator : RC/JU
Sample : Q2295-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TP01-MH1-WC

Quant Time: Jun 13 23:19:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

