

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061325\
Data File : BM050311.D
Acq On : 13 Jun 2025 22:24
Operator : RC/JU
Sample : Q2296-20
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
WC-5

Quant Time: Jun 14 00:41:06 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.763	152	374198	20.000	ng	0.00
21) Naphthalene-d8	10.545	136	1386931	20.000	ng	#-0.01
39) Acenaphthene-d10	14.392	164	729126	20.000	ng	0.00
64) Phenanthrene-d10	17.127	188	1344097	20.000	ng	-0.01
76) Chrysene-d12	21.356	240	1424977	20.000	ng	-0.02
86) Perylene-d12	24.327	264	1496511	20.000	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.357	112	3229031	143.947	ng	0.00
7) Phenol-d6	6.928	99	3589177	121.545	ng	0.00
23) Nitrobenzene-d5	8.910	82	2720170	102.003	ng	0.00
42) 2,4,6-Tribromophenol	15.874	330	1177559	141.989	ng	0.00
45) 2-Fluorobiphenyl	13.016	172	5113901	94.956	ng	-0.01
79) Terphenyl-d14	19.756	244	6281401	83.534	ng	-0.01


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061325\
Data File : BM050311.D
Acq On : 13 Jun 2025 22:24
Operator : RC/JU
Sample : Q2296-20
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
WC-5

Quant Time: Jun 14 00:41:06 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

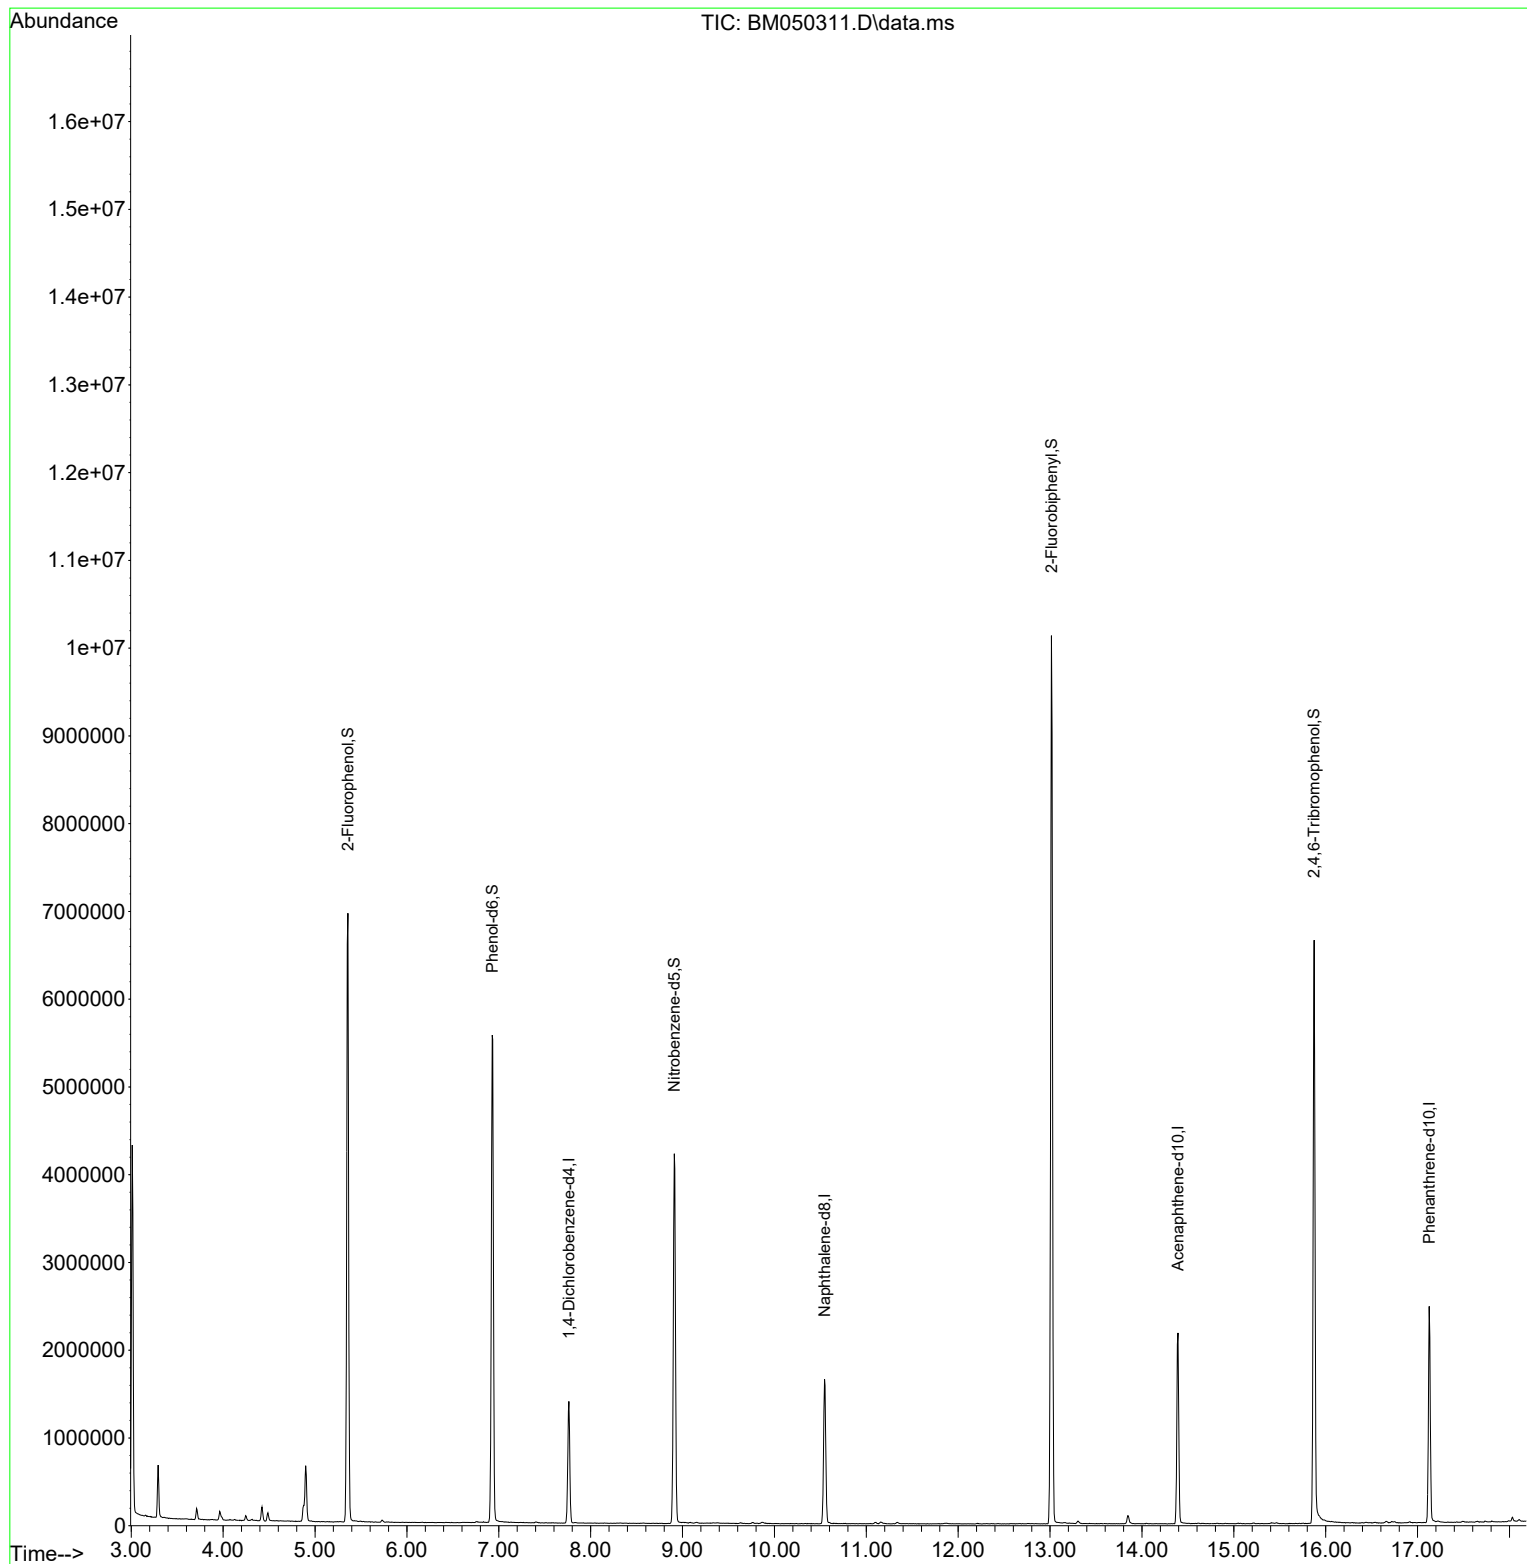

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061325\
Data File : BM050311.D
Acq On : 13 Jun 2025 22:24
Operator : RC/JU
Sample : Q2296-20
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
WC-5

Quant Time: Jun 14 00:41:06 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

