

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061325\
 Data File : BM050318.D
 Acq On : 14 Jun 2025 03:40
 Operator : RC/JU
 Sample : Q2301-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 WC-URBAN-FILL-C

Quant Time: Jun 14 04:28:15 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 09 11:54:38 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.763	152	365030	20.000	ng	0.00
21) Naphthalene-d8	10.545	136	1367333	20.000	ng	-0.01
39) Acenaphthene-d10	14.392	164	730437	20.000	ng	0.00
64) Phenanthrene-d10	17.127	188	1329061	20.000	ng	-0.01
76) Chrysene-d12	21.356	240	1333433	20.000	ng	-0.02
86) Perylene-d12	24.321	264	1403419	20.000	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.357	112	3510429	160.422	ng	0.00
7) Phenol-d6	6.934	99	4011894	139.272	ng	0.00
23) Nitrobenzene-d5	8.910	82	2810169	106.888	ng	0.00
42) 2,4,6-Tribromophenol	15.874	330	1350757	162.581	ng	0.00
45) 2-Fluorobiphenyl	13.016	172	5544528	102.767	ng	-0.01
79) Terphenyl-d14	19.756	244	7199245	102.313	ng	-0.01
Target Compounds						
						Qvalue
31) Naphthalene	10.598	128	241099	3.410	ng	99
52) Acenaphthene	14.451	154	88016	2.046	ng	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061325\
Data File : BM050318.D
Acq On : 14 Jun 2025 03:40
Operator : RC/JU
Sample : Q2301-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
WC-URBAN-FILL-C

Quant Time: Jun 14 04:28:15 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

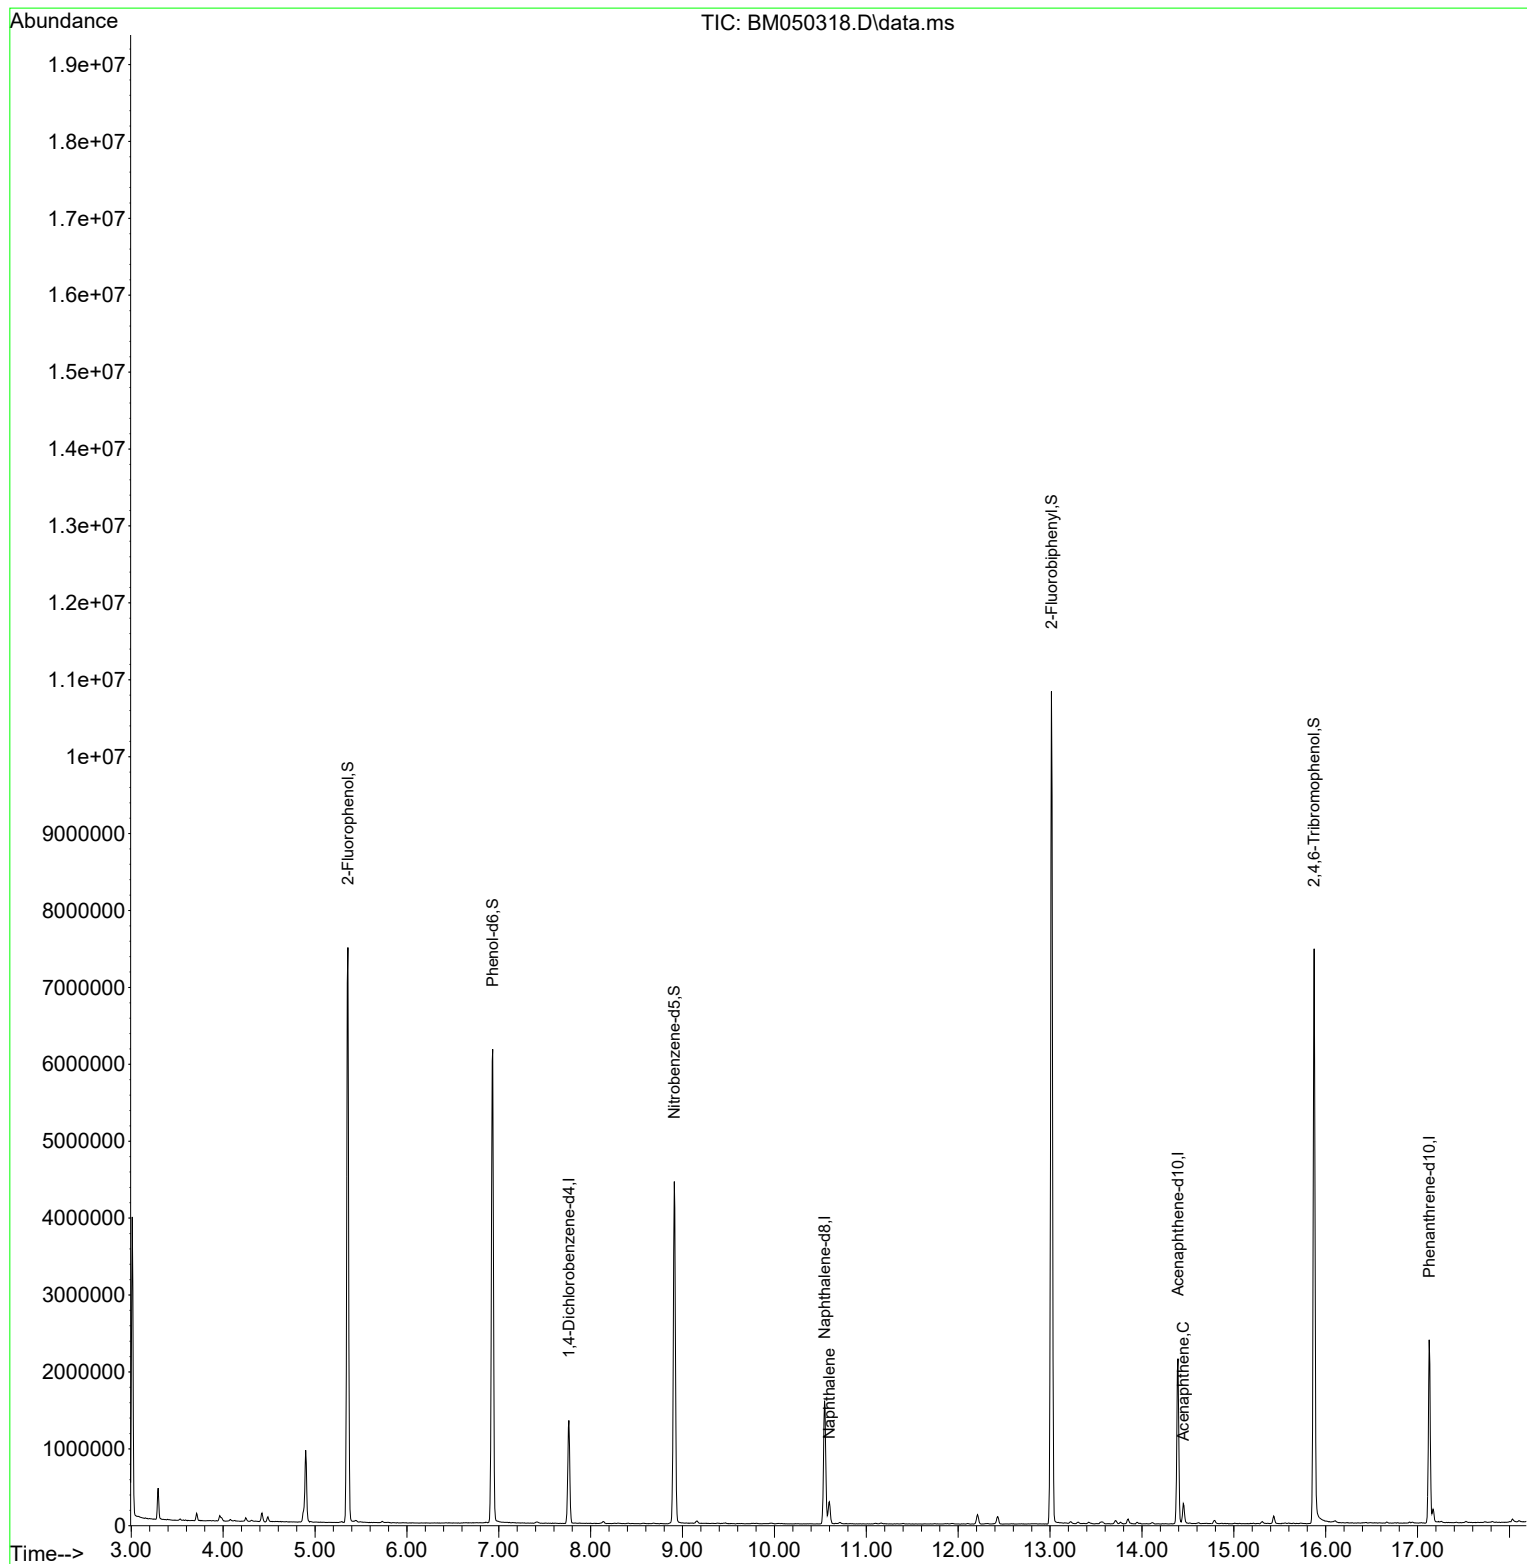

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061325\
Data File : BM050318.D
Acq On : 14 Jun 2025 03:40
Operator : RC/JU
Sample : Q2301-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
WC-URBAN-FILL-C

Quant Time: Jun 14 04:28:15 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

