
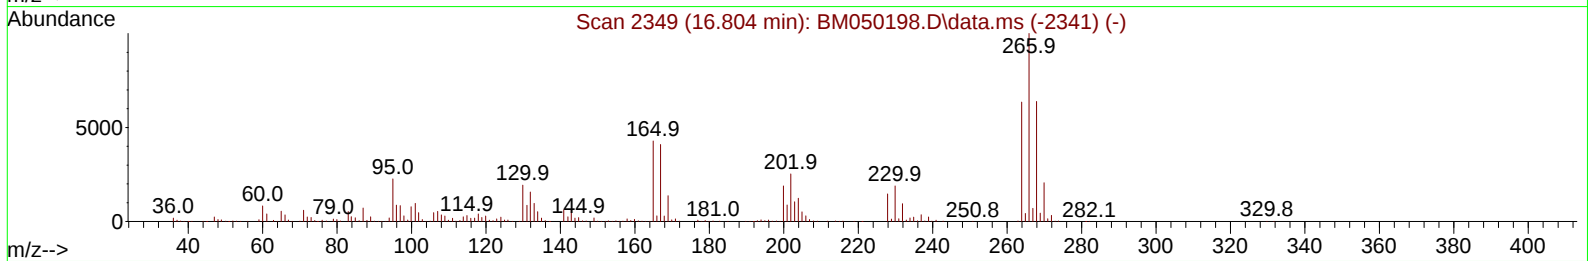
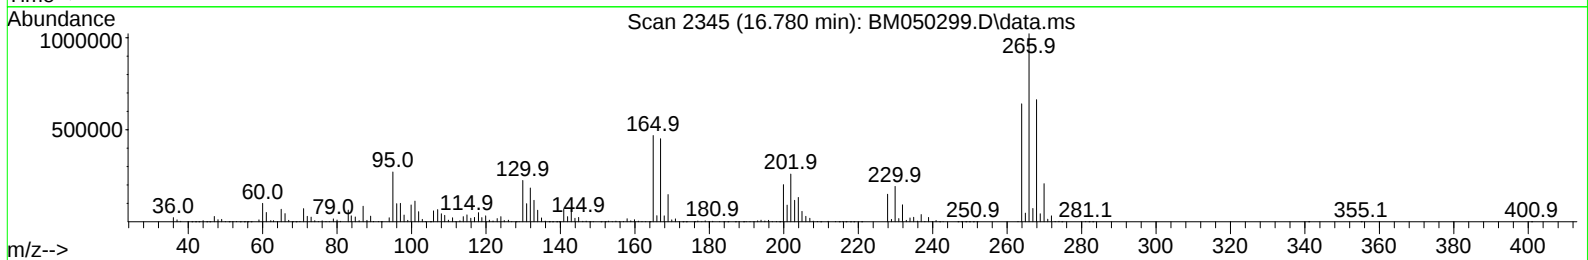


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061325\
Data File : BM050299.D
Acq On : 13 Jun 2025 13:06
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 13 14:03:31 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

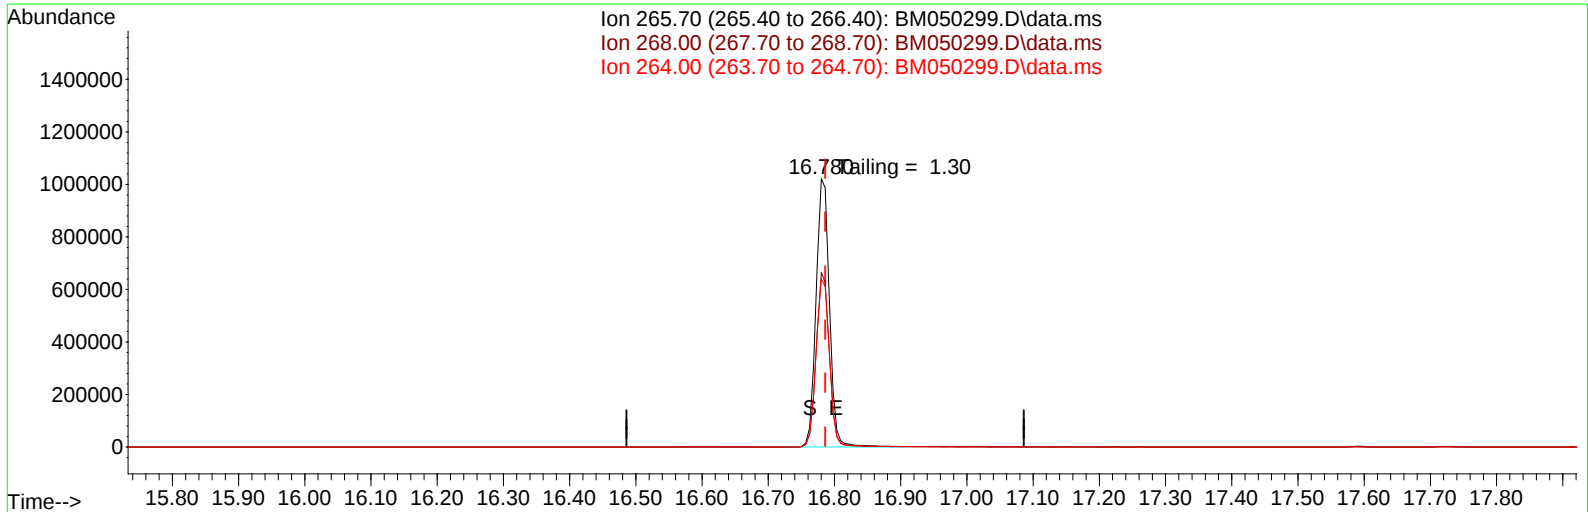




TIC: BM050299.D\data.ms

(70) Pentachlorophenol (C)**16.780min (-0.006) 1168905.43 ng****response 1439222**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.98
264.00	63.50	62.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061325\
Data File : BM050299.D
Acq On : 13 Jun 2025 13:06
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 13 14:03:31 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

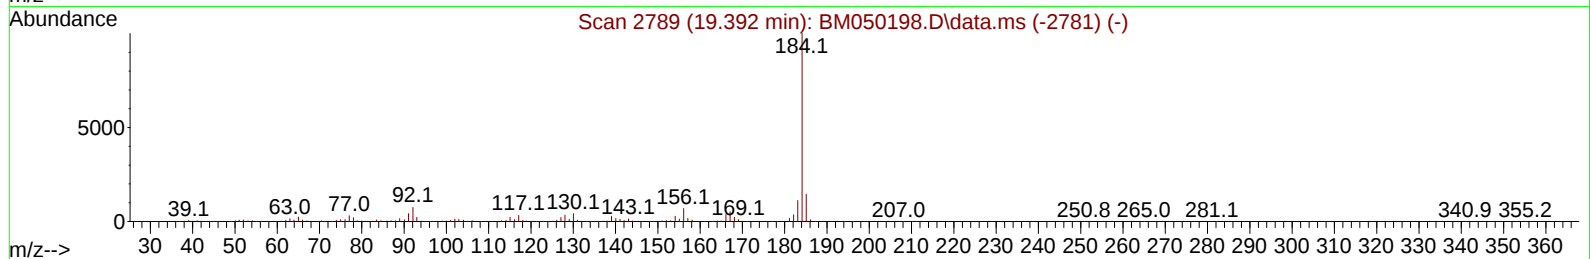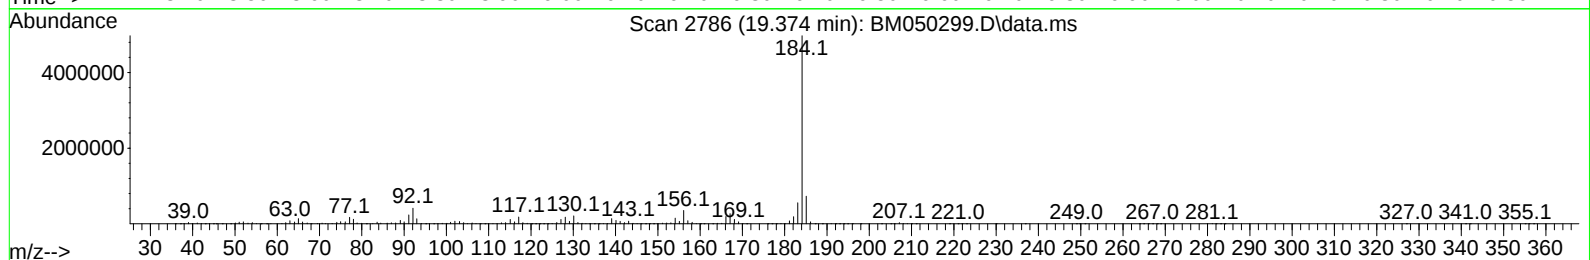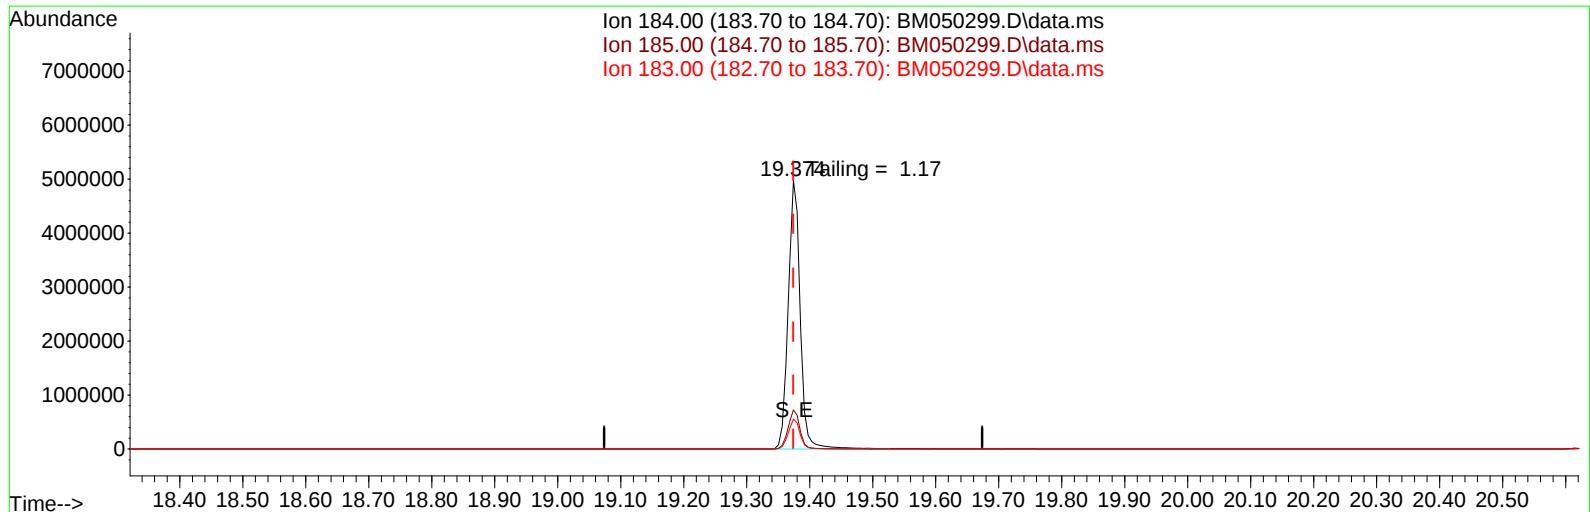

TIC: BM050299.D\data.ms

(77) Benzidine**19.374min (-0.000) 3527.81 ng****response 6639877**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.61
183.00	11.20	11.16
0.00	0.00	0.00