
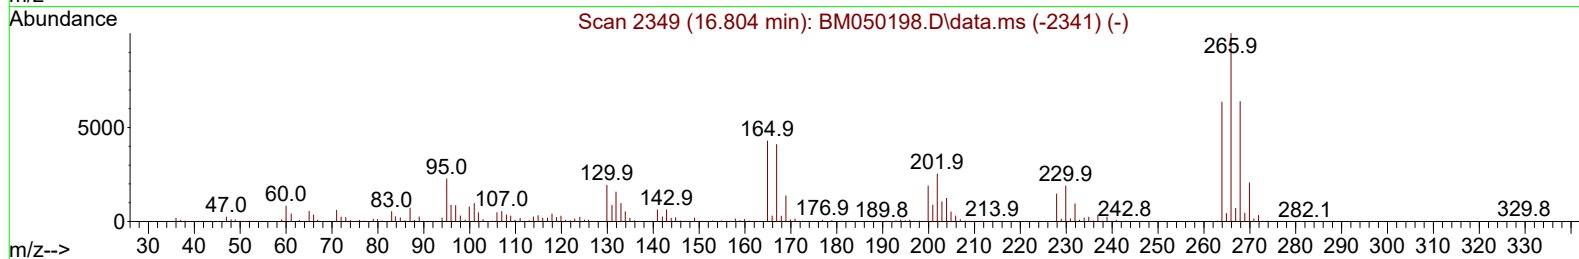
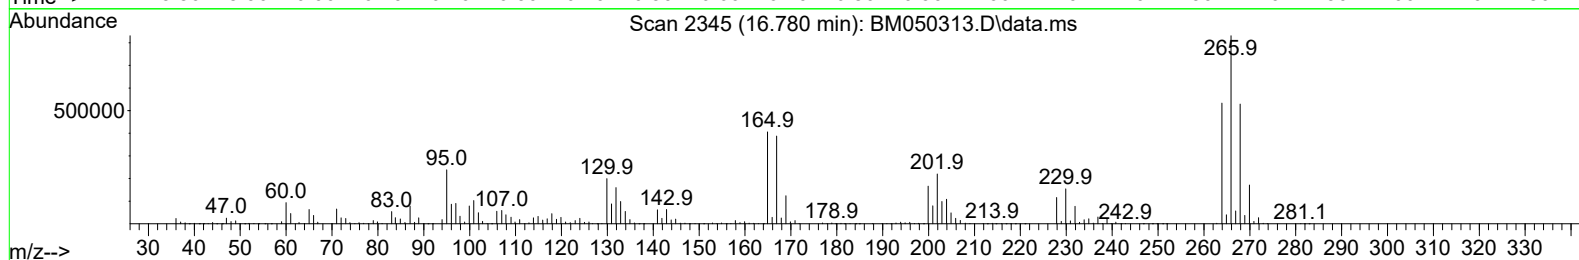


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061325\
Data File : BM050313.D
Acq On : 14 Jun 2025 00:22
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 14 03:45:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

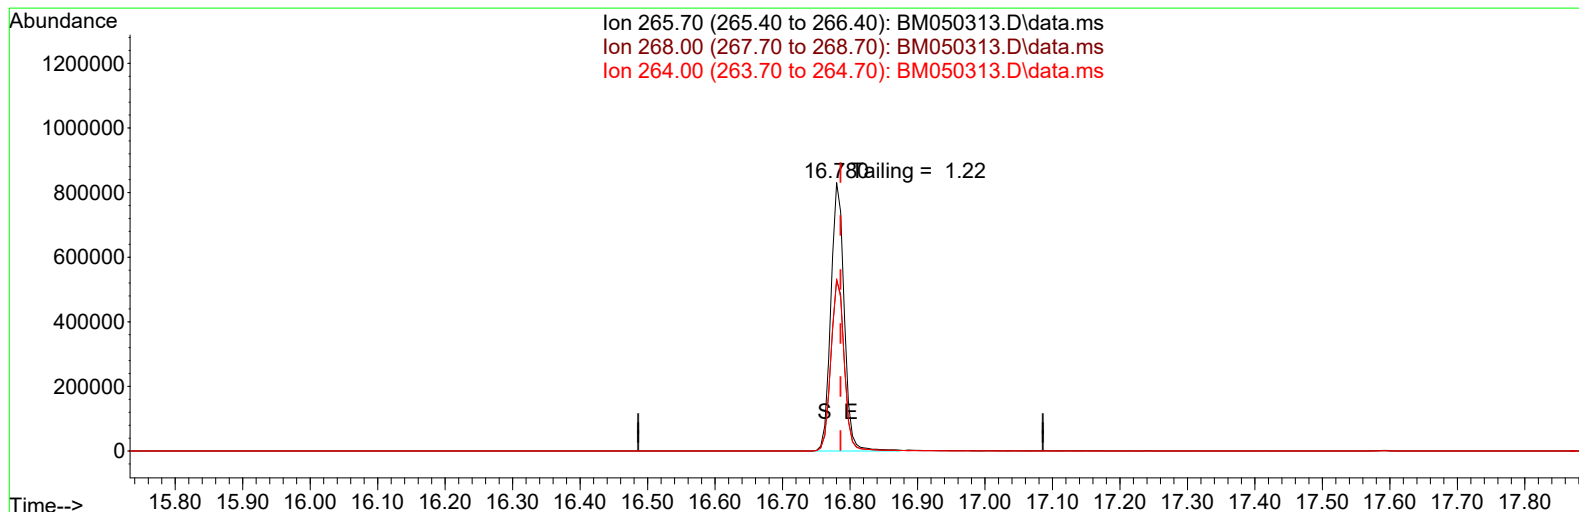

TIC: BM050313.D\data.ms

(70) Pentachlorophenol (C)




16.780min (-0.006) 595353.38 ng

response 1142952

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.70
264.00	63.50	64.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061325\
Data File : BM050313.D
Acq On : 14 Jun 2025 00:22
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 14 03:45:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

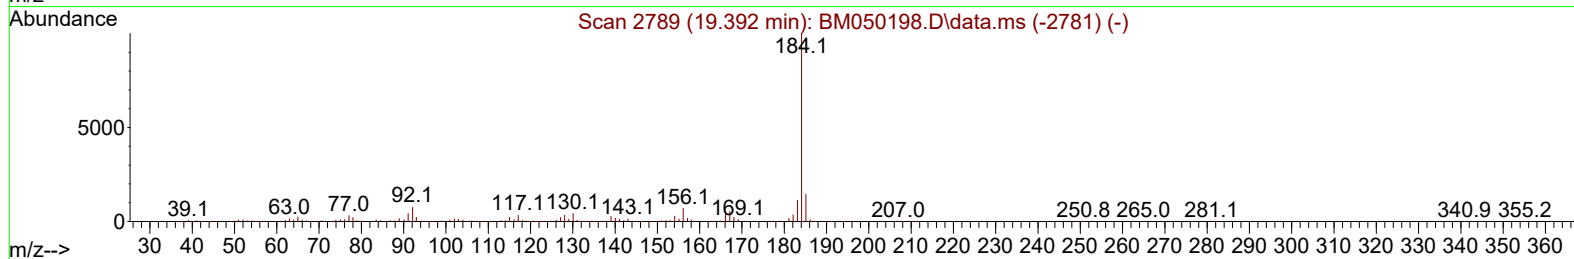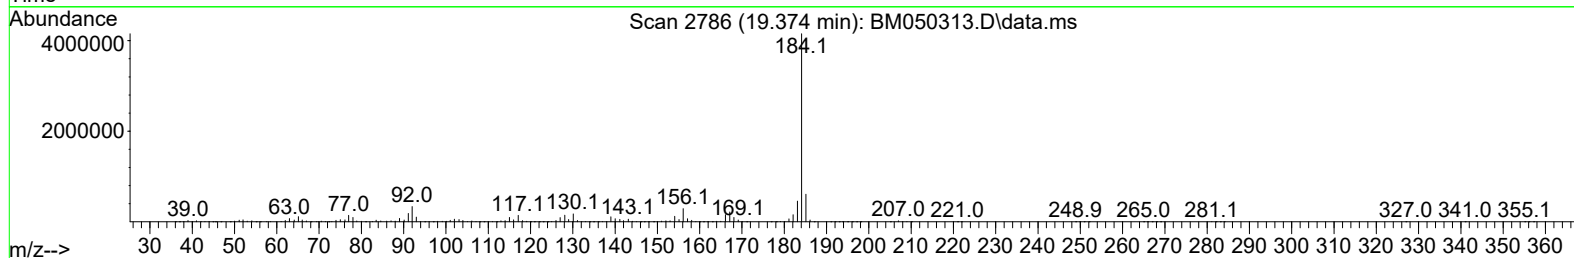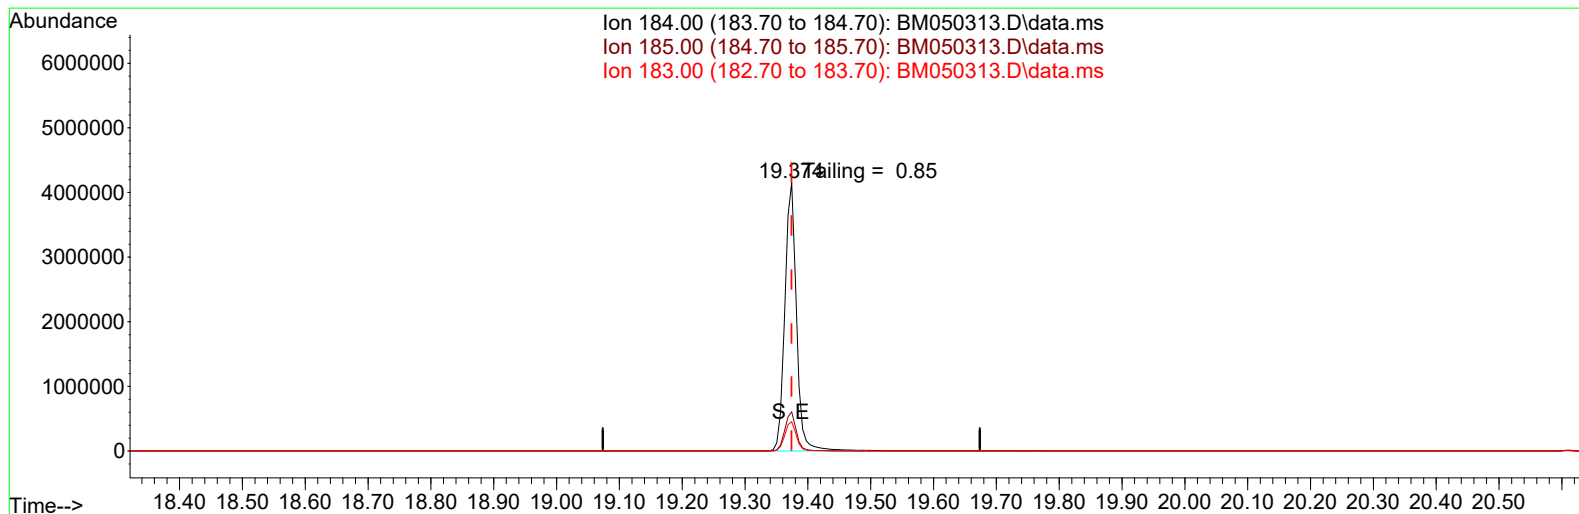

TIC: BM050313.D\data.ms

(77) Benzidine**19.374min (0.000) 119220.92 ng****response 5377552**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.63
183.00	11.20	10.95
0.00	0.00	0.00