
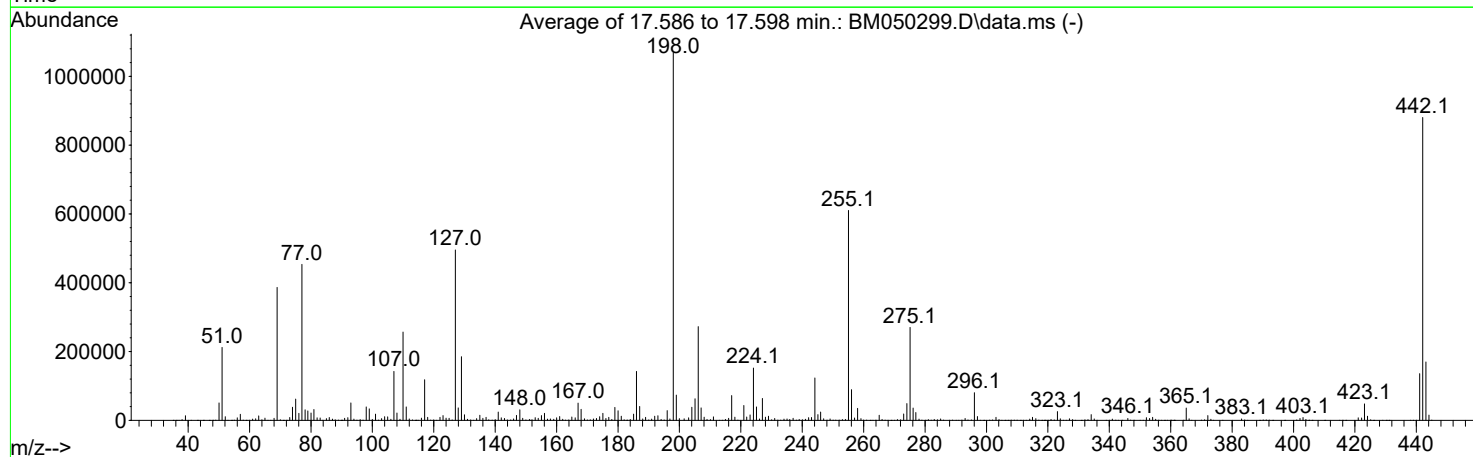


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061325\
Data File : BM050299.D
Acq On : 13 Jun 2025 13:06
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jun 09 11:54:38 2025

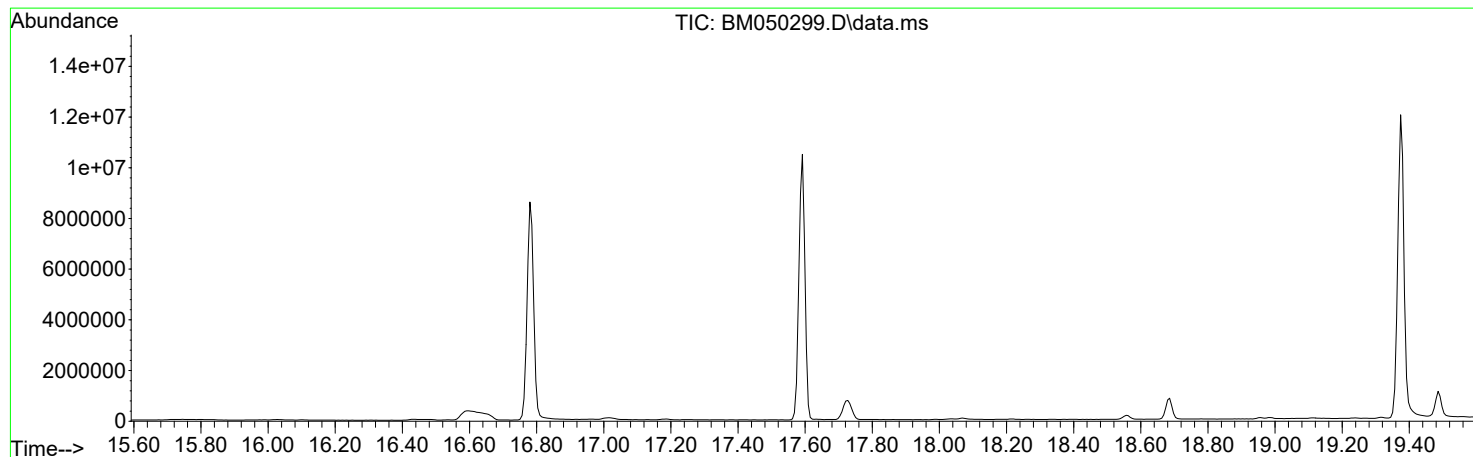

AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	19.8	211977	PASS
68	69	0.00	2	1.6	6013	PASS
69	198	0.00	100	36.2	386686	PASS
70	69	0.00	2	0.5	1832	PASS
127	198	10	80	46.3	495659	PASS
197	198	0.00	2	0.4	4144	PASS
198	198	100	100	100.0	1069440	PASS
199	198	5	9	6.9	73349	PASS
275	198	10	60	25.3	270187	PASS
365	198	1	100	3.4	35869	PASS
441	198	0.01	100	12.7	135752	PASS
442	442	50	100	100.0	880747	PASS
443	442	15	24	19.3	169835	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/13/2025	BNA_M	<u>BM050299.D</u>
Compound Name	Response	Retention Time
DDT	3370476	20.615
DDD	38022	20.227
DDE	5680	19.668
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
43702	3414178	1.28

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061325\
Data File : BM050299.D
Acq On : 13 Jun 2025 13:06
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jun 13 14:03:31 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

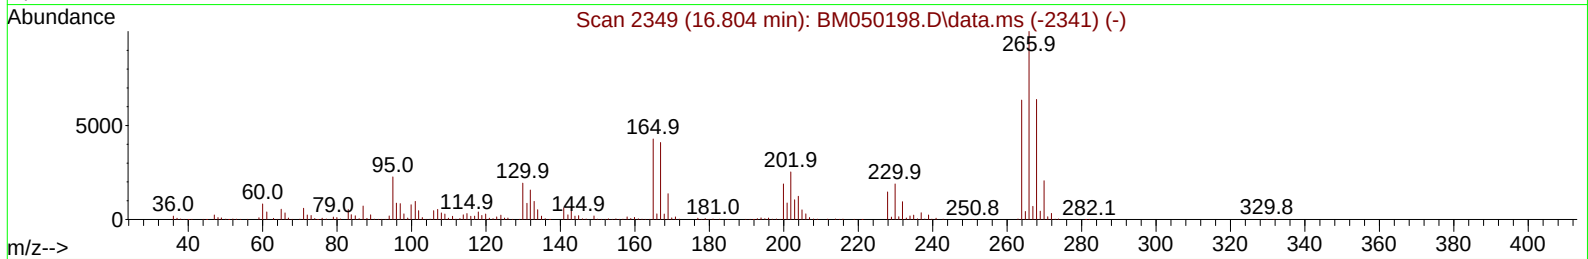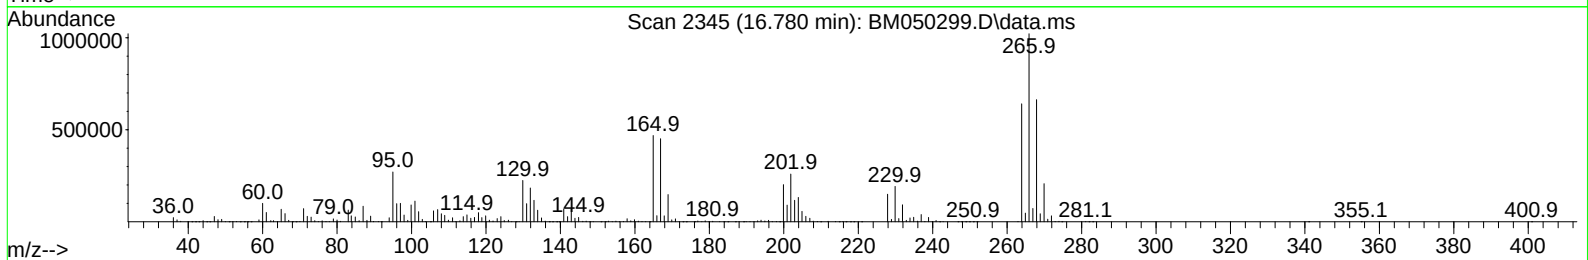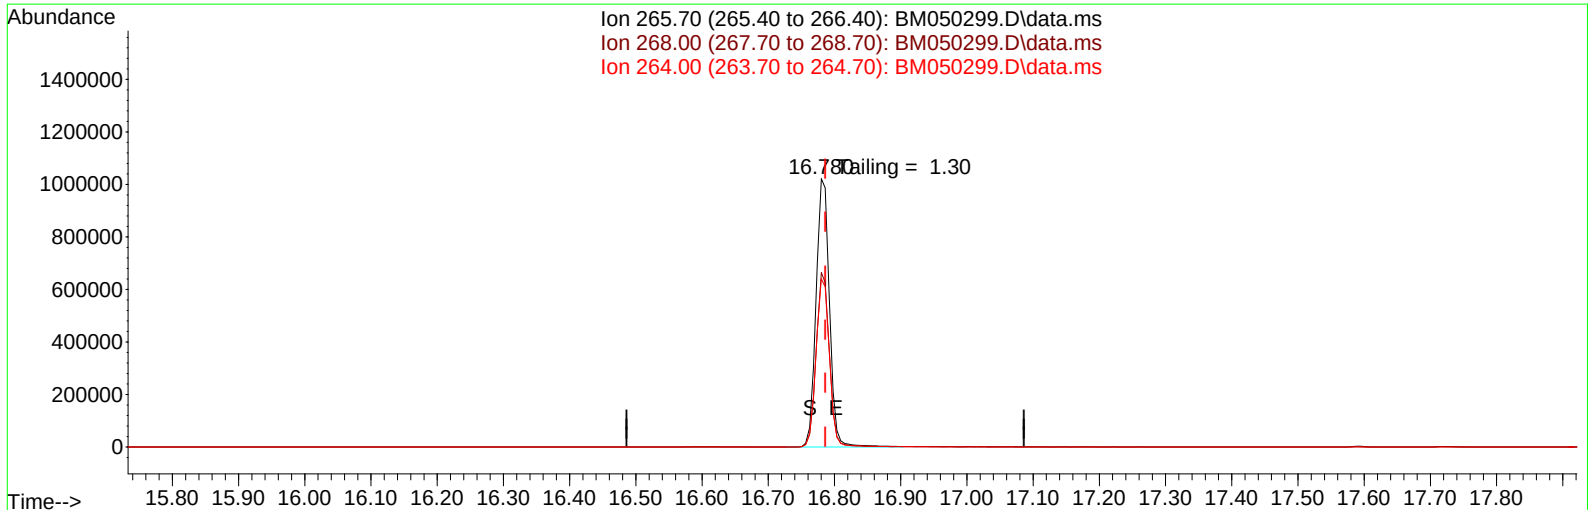

TIC: BM050299.D\data.ms

(70) Pentachlorophenol (C)

16.780min (-0.006) 1168905.43 ng




response 1439222

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.98
264.00	63.50	62.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061325\
Data File : BM050299.D
Acq On : 13 Jun 2025 13:06
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jun 13 14:03:31 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

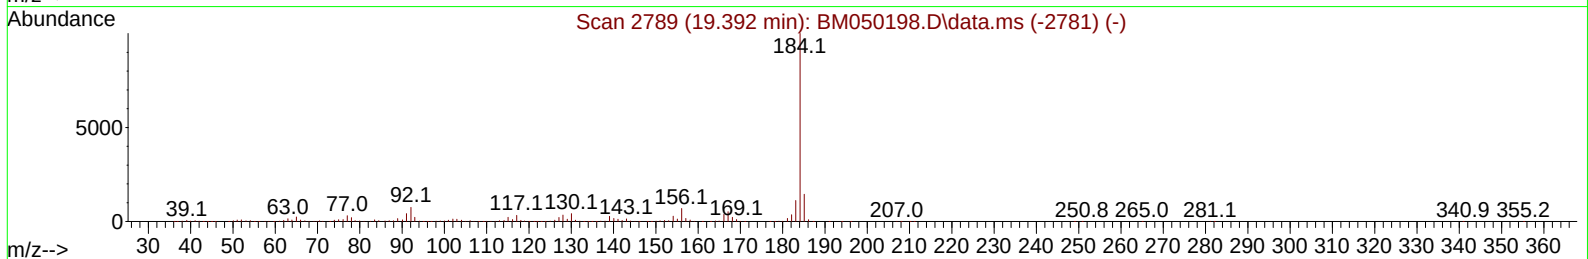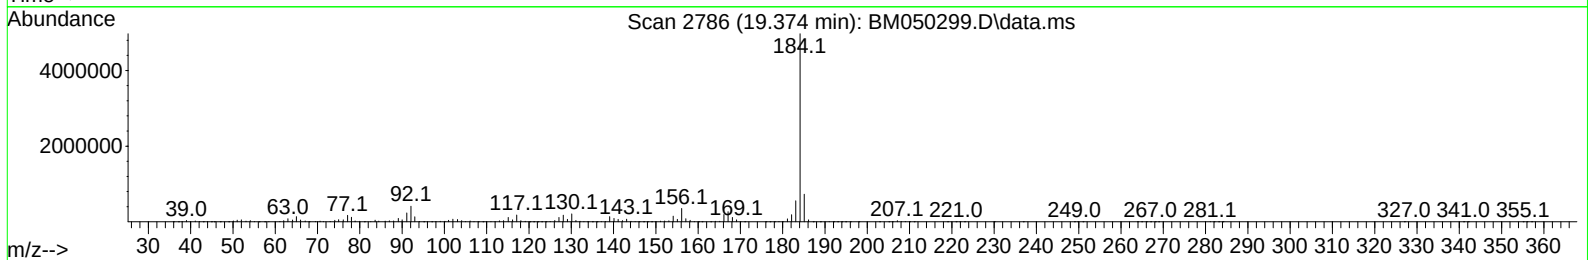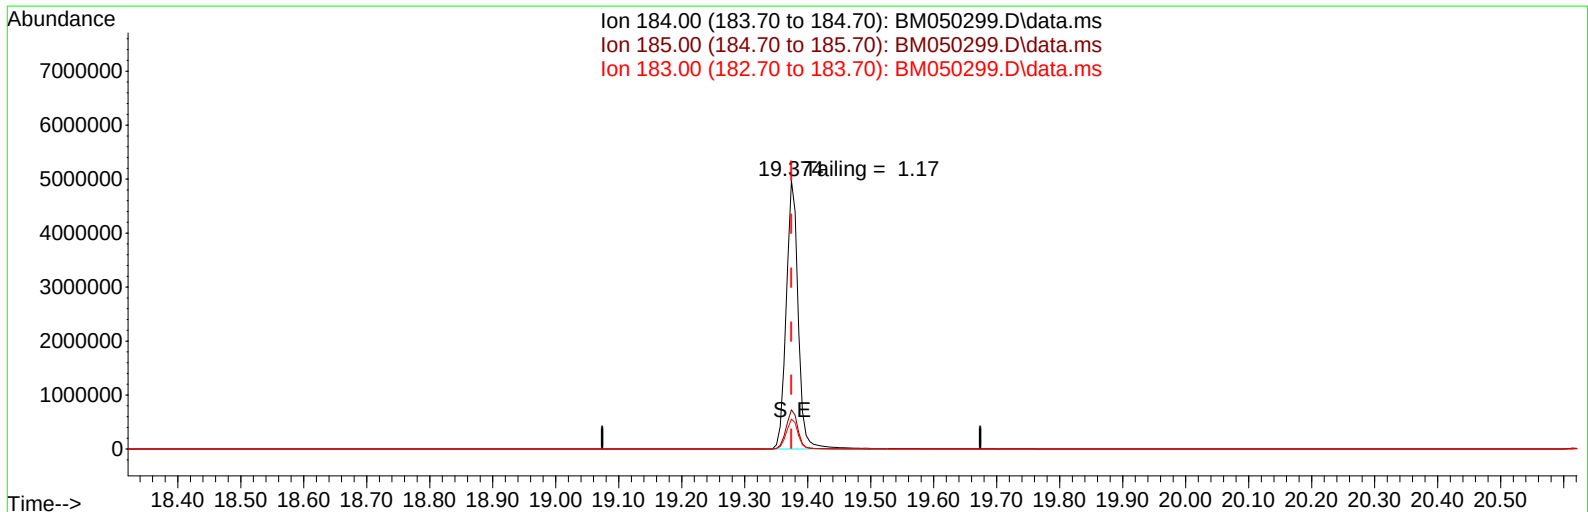

TIC: BM050299.D\data.ms

(77) Benzidine

19.374min (-0.000) 3527.81 ng

response 6639877

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.61
183.00	11.20	11.16
0.00	0.00	0.00