


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061325\
Data File : BM050313.D
Acq On : 14 Jun 2025 00:22
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jun 09 11:54:38 2025

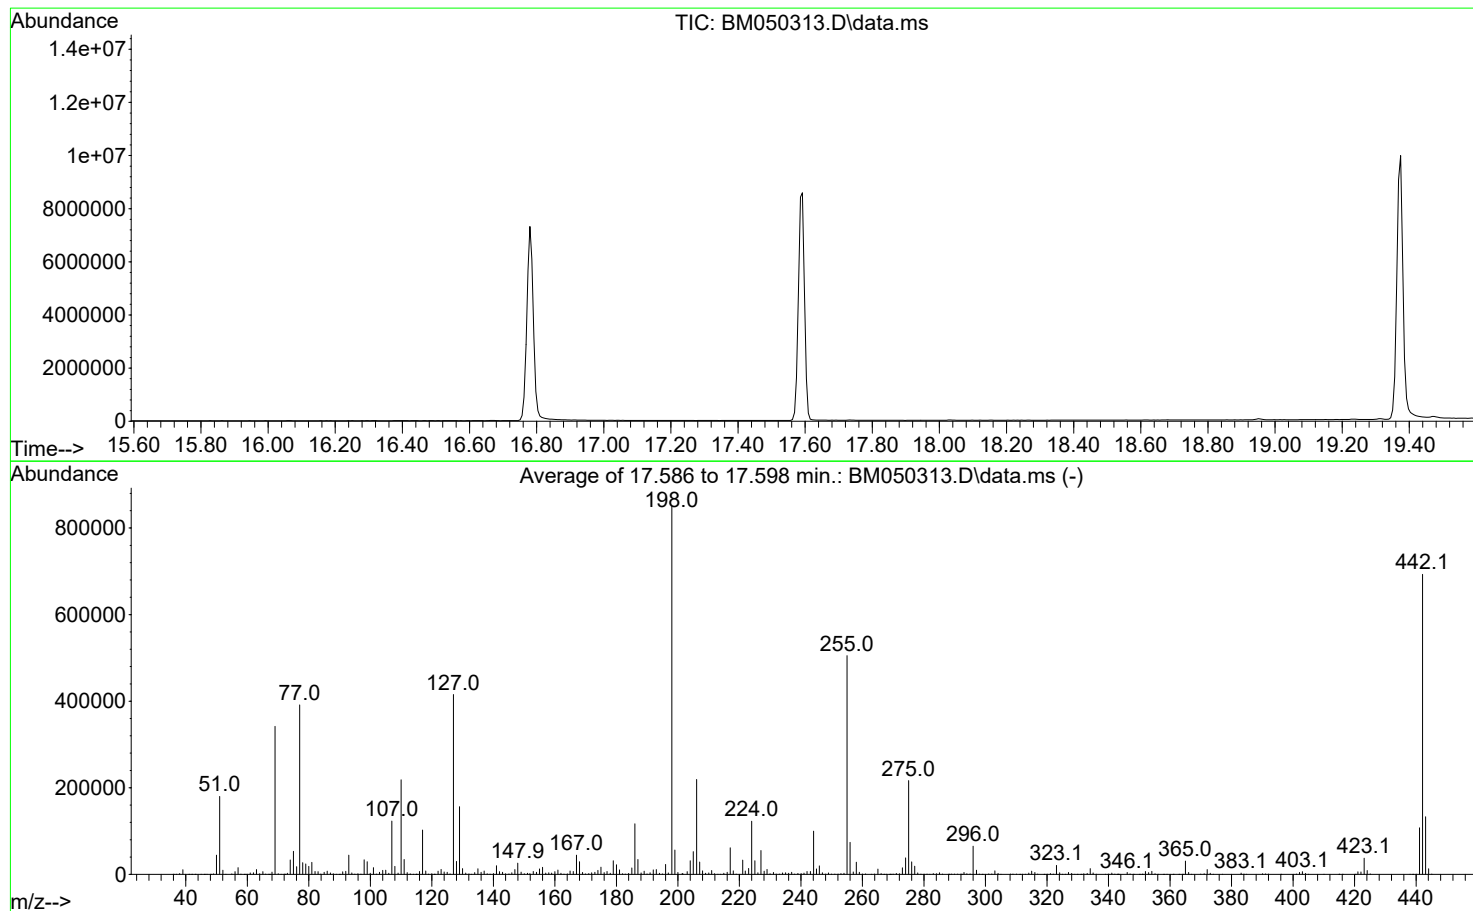

AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.2	180040	PASS
68	69	0.00	2	1.6	5301	PASS
69	198	0.00	100	40.2	341995	PASS
70	69	0.00	2	0.5	1663	PASS
127	198	10	80	48.9	415403	PASS
197	198	0.00	2	0.4	3487	PASS
198	198	100	100	100.0	849728	PASS
199	198	5	9	6.6	56200	PASS
275	198	10	60	25.5	216512	PASS
365	198	1	100	3.6	30629	PASS
441	198	0.01	100	12.7	107696	PASS
442	442	50	100	100.0	693056	PASS
443	442	15	24	19.2	132896	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/13/2025	BNA_M	<u>BM050313.D</u>
Compound Name	Response	Retention Time
DDT	3082392	20.609
DDD	22961	20.227
DDE	2634	19.662
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
25595	3107987	0.82

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061325\
Data File : BM050313.D
Acq On : 14 Jun 2025 00:22
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jun 14 03:45:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

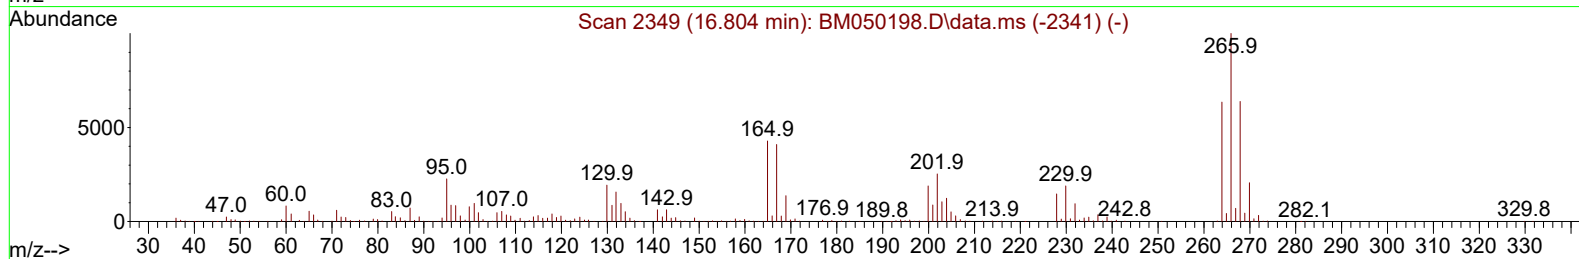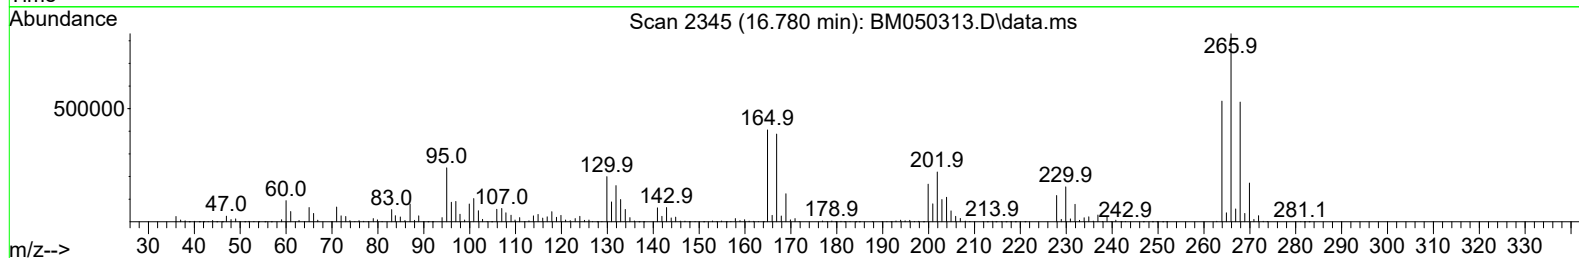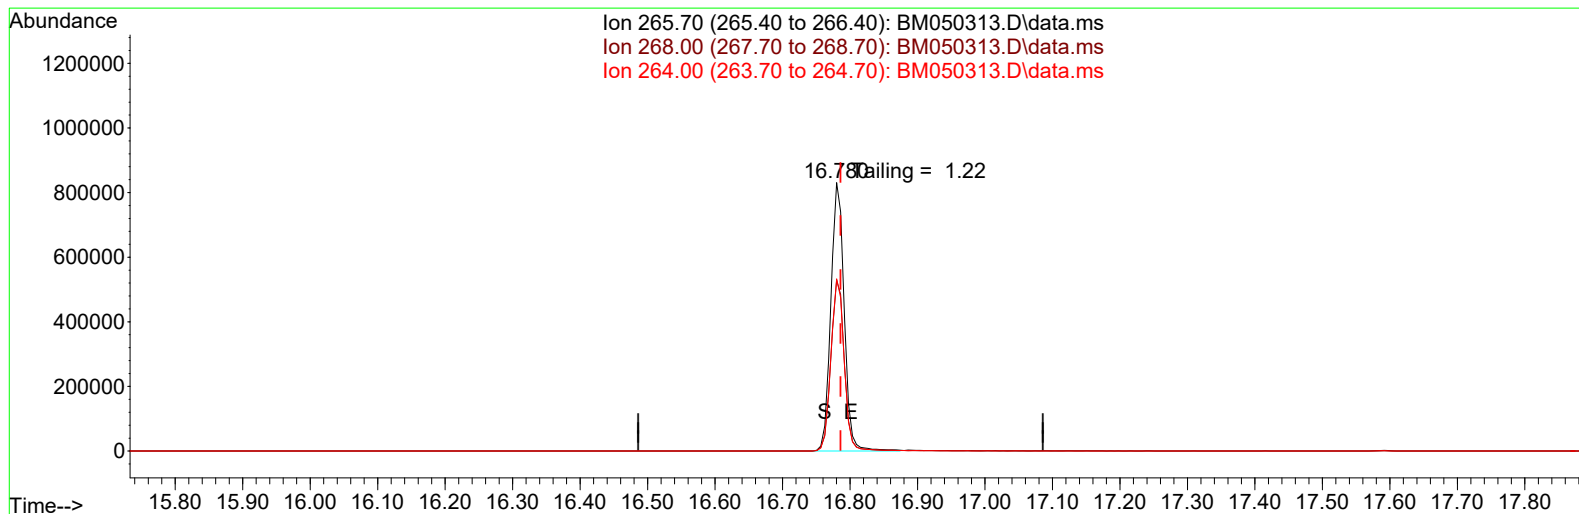

TIC: BM050313.D\data.ms

(70) Pentachlorophenol (C)

16.780min (-0.006) 595353.38 ng




response 1142952

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.70
264.00	63.50	64.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061325\
Data File : BM050313.D
Acq On : 14 Jun 2025 00:22
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jun 14 03:45:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

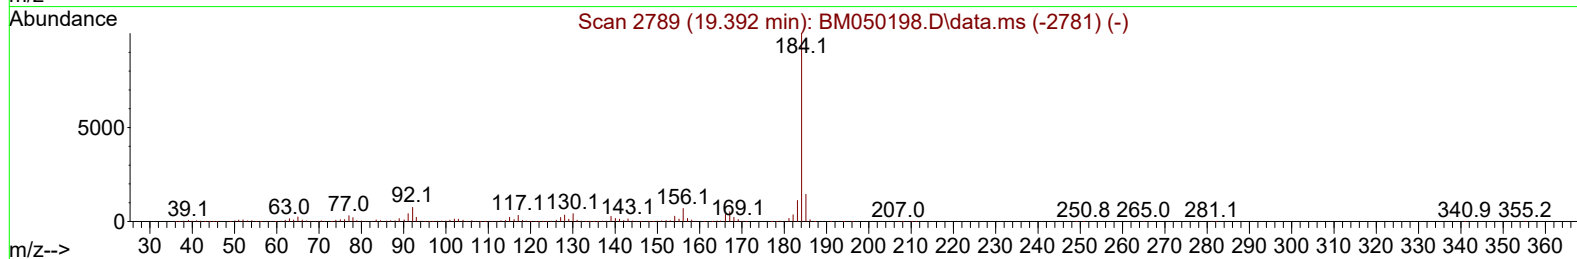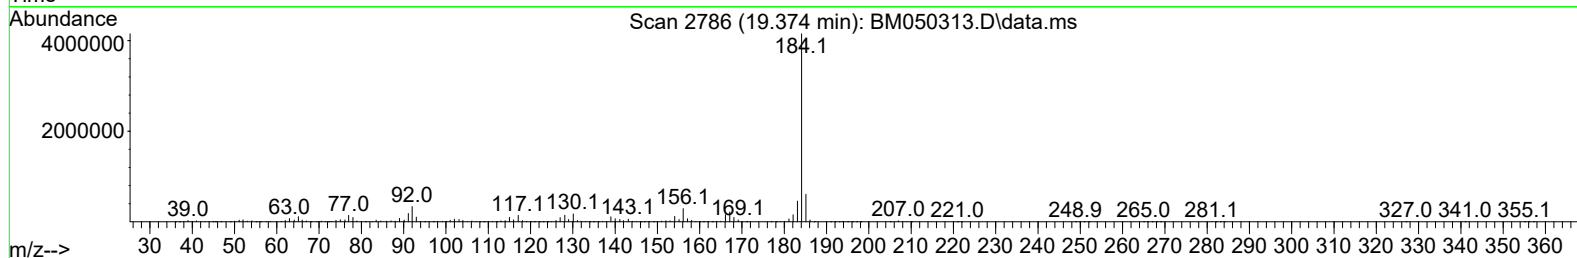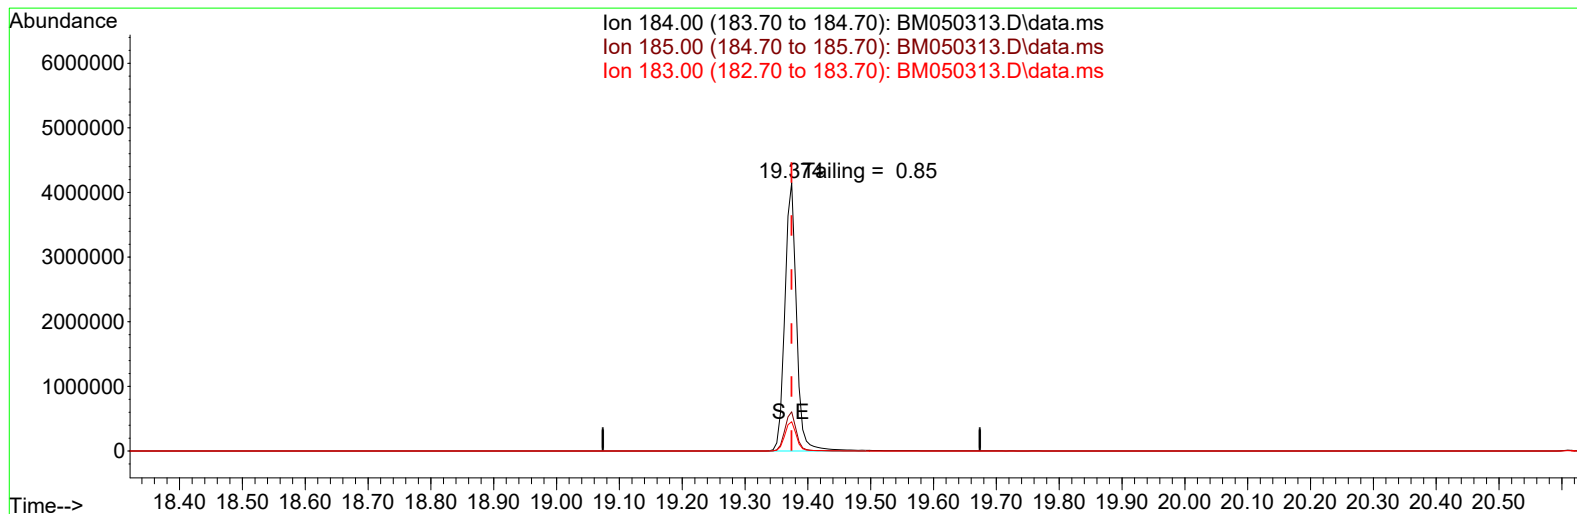

TIC: BM050313.D\data.ms

(77) Benzidine

19.374min (0.000) 119220.92 ng

response 5377552

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.63
183.00	11.20	10.95
0.00	0.00	0.00