

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061421\
 Data File : BM030432.D
 Acq On : 14 Jun 2021 12:08
 Operator : CG/JU
 Sample : PB137061BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB137061BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM030432.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.416	389	396	407	rBV	2936014	4195007	30.07%	7.290%
2	6.998	657	665	677	rBV	2751641	4306685	30.87%	7.484%
3	7.834	799	807	816	rBV	743229	1165050	8.35%	2.025%
4	8.151	853	861	874	rVB	3340279	5392617	38.65%	9.371%
5	8.986	995	1003	1014	rBV	2453036	4031812	28.90%	7.006%
6	10.622	1273	1281	1292	rBV	896301	1541178	11.05%	2.678%
7	13.080	1691	1699	1714	rBV	6425807	9396725	67.36%	16.329%
8	14.457	1926	1933	1947	rBV	1338312	2000052	14.34%	3.476%
9	15.939	2178	2185	2210	rBV	2908149	4263436	30.56%	7.409%
10	17.192	2391	2398	2409	rBV	1565425	2329160	16.70%	4.048%
11	18.086	2545	2550	2560	rBV2	56685	149156	1.07%	0.259%
12	19.803	2836	2842	2851	rBV	11275956	13950674	100.00%	24.243%
13	21.356	3100	3106	3115	rBV	1838826	2512271	18.01%	4.366%
14	23.627	3486	3492	3507	rVB2	1130712	2310899	16.56%	4.016%




Sum of corrected areas: 57544722

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061421\
Data File : BM030432.D
Acq On : 14 Jun 2021 12:08
Operator : CG/JU
Sample : PB137061BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB137061BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

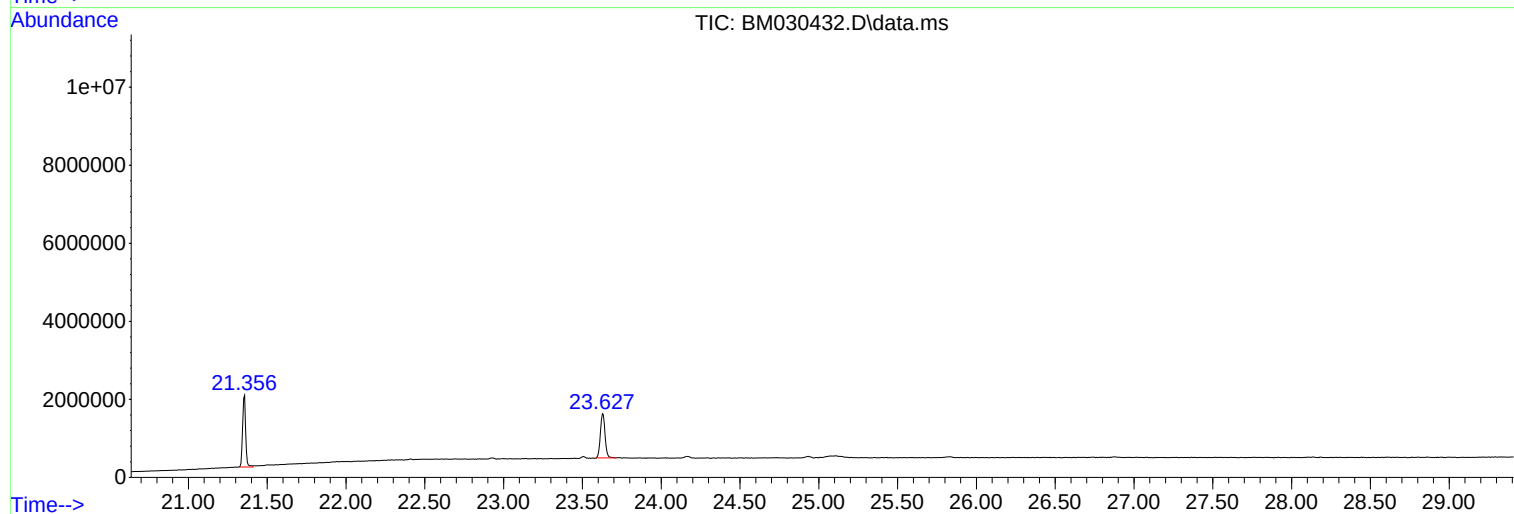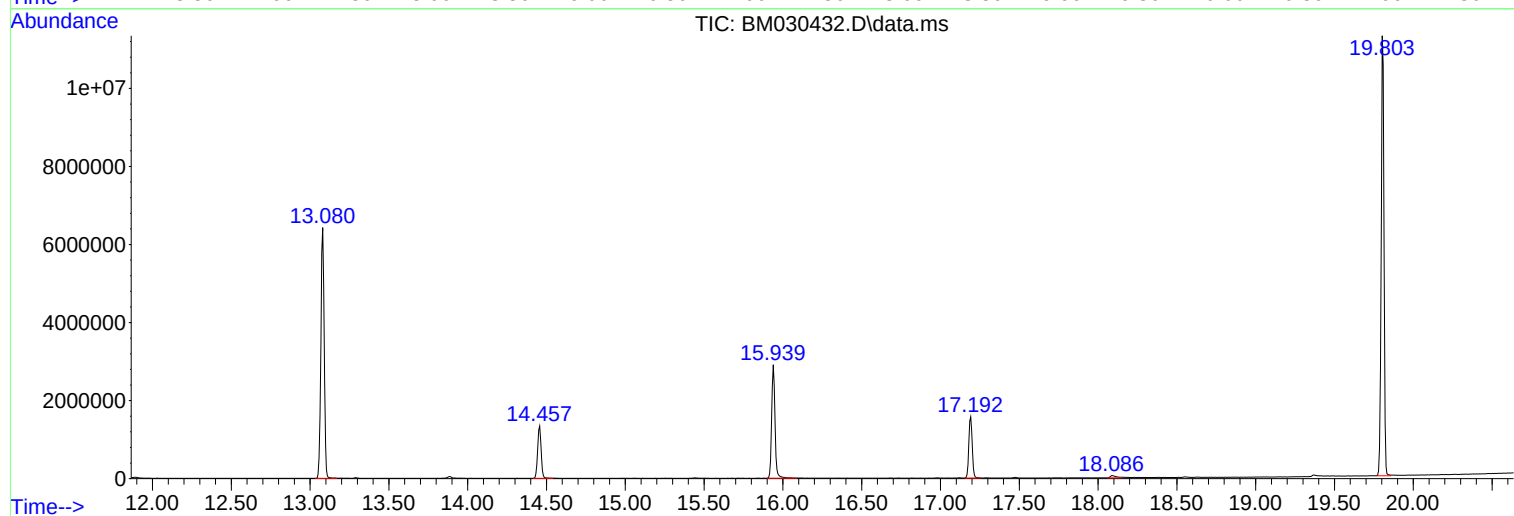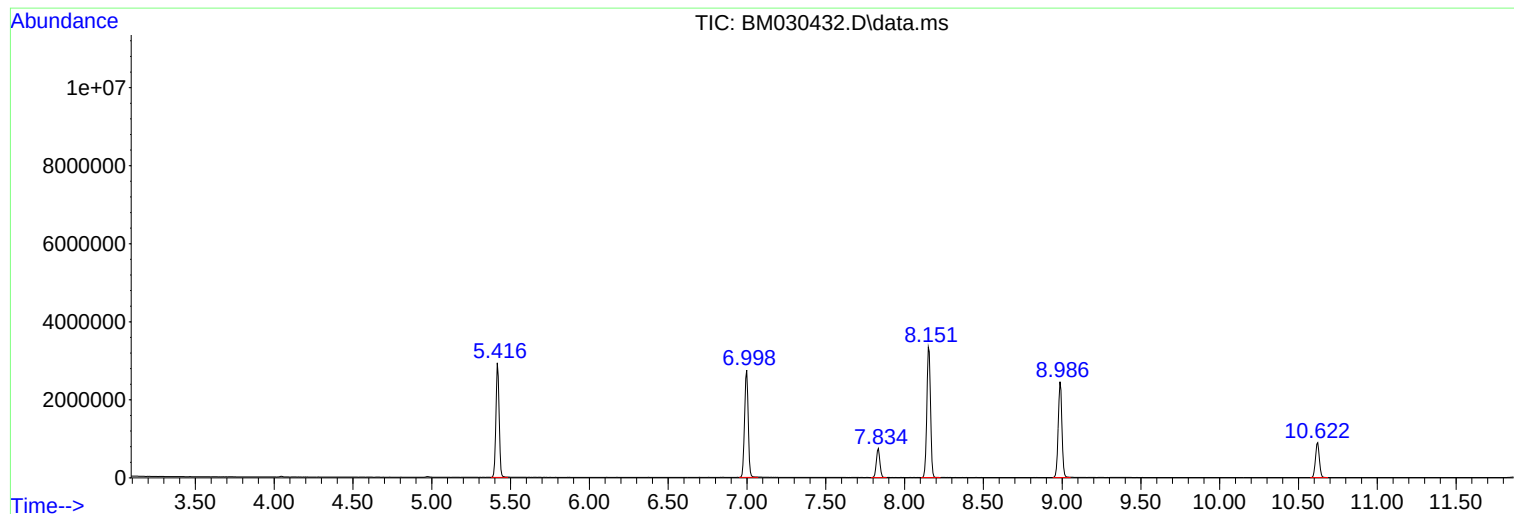

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061421\
Data File : BM030432.D
Acq On : 14 Jun 2021 12:08
Operator : CG/JU
Sample : PB137061BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB137061BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061421\
Data File : BM030432.D
Acq On : 14 Jun 2021 12:08
Operator : CG/JU
Sample : PB137061BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB137061BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------