

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061421\
 Data File : BM030435.D
 Acq On : 14 Jun 2021 13:58
 Operator : CG/JU
 Sample : PB137041BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB137041BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM030435.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.969	315	320	330	rBV	89990	136564	1.57%	0.290%
2	5.416	389	396	409	rBV	4181992	6016926	69.18%	12.774%
3	6.998	657	665	677	rBV	3896356	6047060	69.52%	12.838%
4	7.834	799	807	815	rVB	702869	1125257	12.94%	2.389%
5	8.987	995	1003	1018	rBV	2190961	3615743	41.57%	7.676%
6	10.622	1273	1281	1293	rBV	846166	1476933	16.98%	3.135%
7	13.080	1691	1699	1714	rBV	5515290	7960234	91.52%	16.899%
8	14.457	1926	1933	1947	rBV	1173221	1775314	20.41%	3.769%
9	15.939	2178	2185	2208	rBV	3465219	5165802	59.39%	10.967%
10	17.192	2391	2398	2409	rBV	1251432	1837386	21.12%	3.901%
11	19.803	2836	2842	2853	rBV	7248487	8698093	100.00%	18.466%
12	21.350	3101	3105	3115	rBV	1233147	1650102	18.97%	3.503%
13	23.627	3487	3492	3504	rVB2	797601	1599053	18.38%	3.395%




Sum of corrected areas: 47104467

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061421\
Data File : BM030435.D
Acq On : 14 Jun 2021 13:58
Operator : CG/JU
Sample : PB137041BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB137041BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

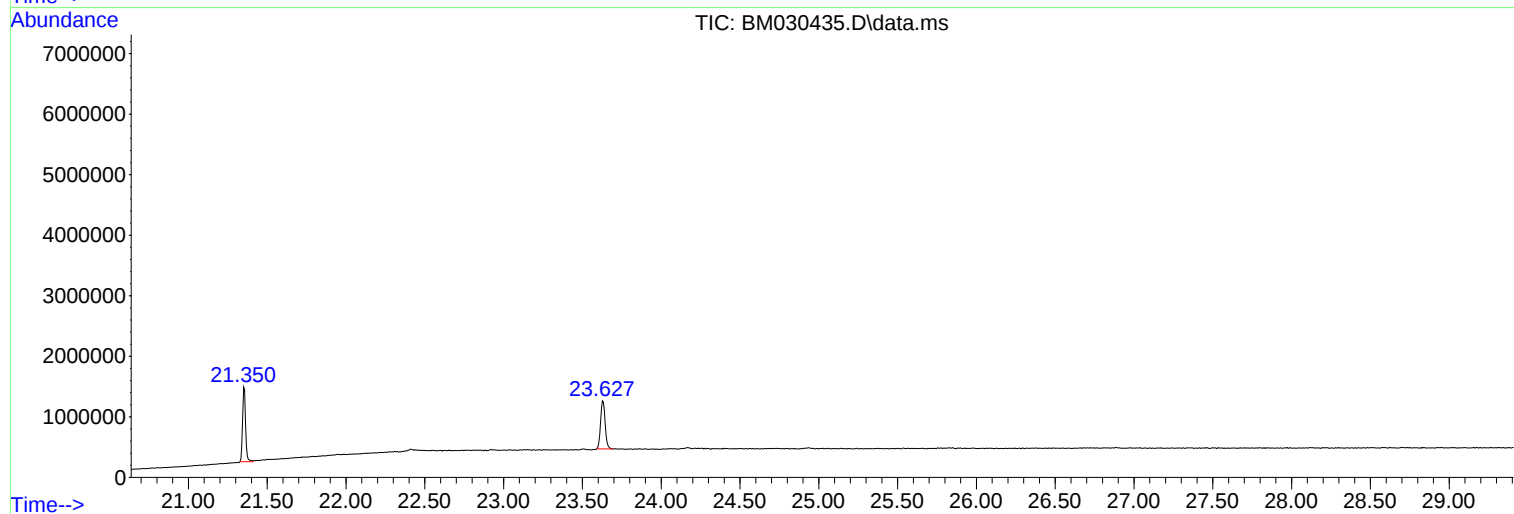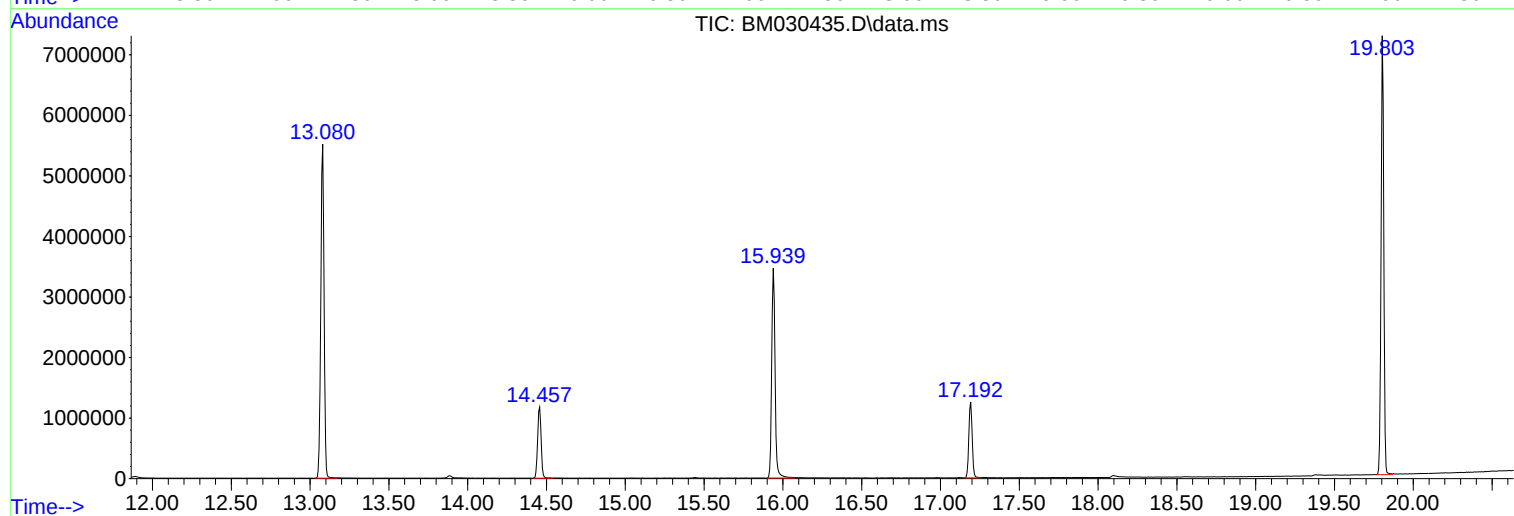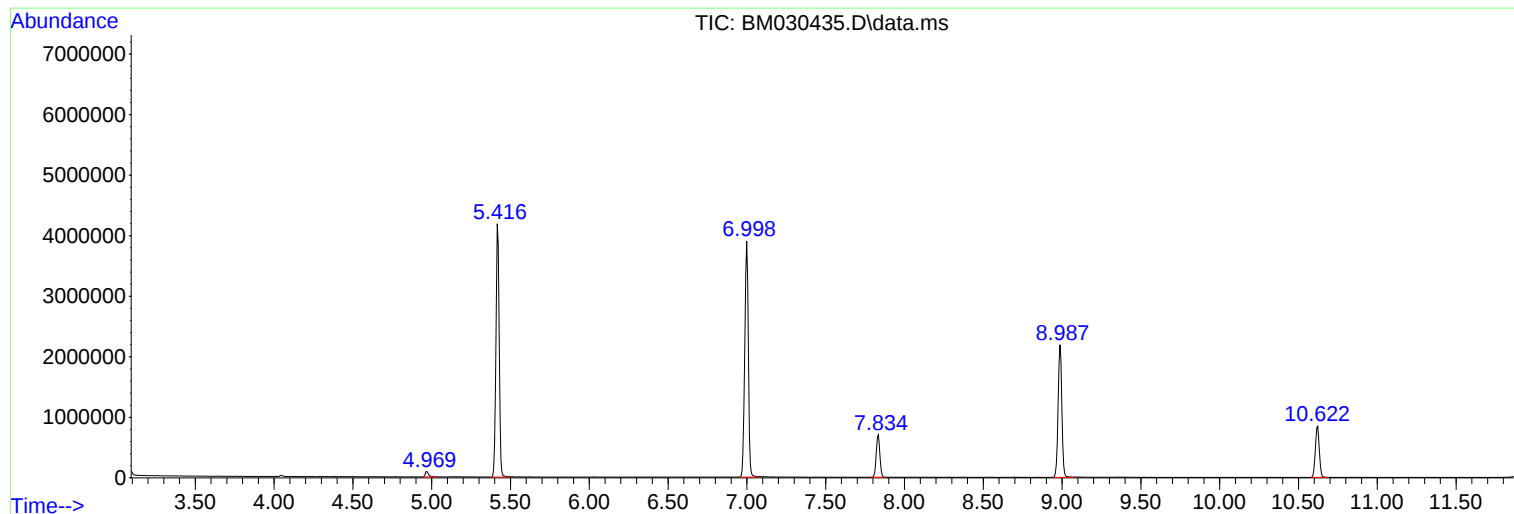

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061421\
Data File : BM030435.D
Acq On : 14 Jun 2021 13:58
Operator : CG/JU
Sample : PB137041BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB137041BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061421\
Data File : BM030435.D
Acq On : 14 Jun 2021 13:58
Operator : CG/JU
Sample : PB137041BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB137041BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------