


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061421\
 Data File : BM030430.D
 Acq On : 14 Jun 2021 10:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 11 14:10:50 2021

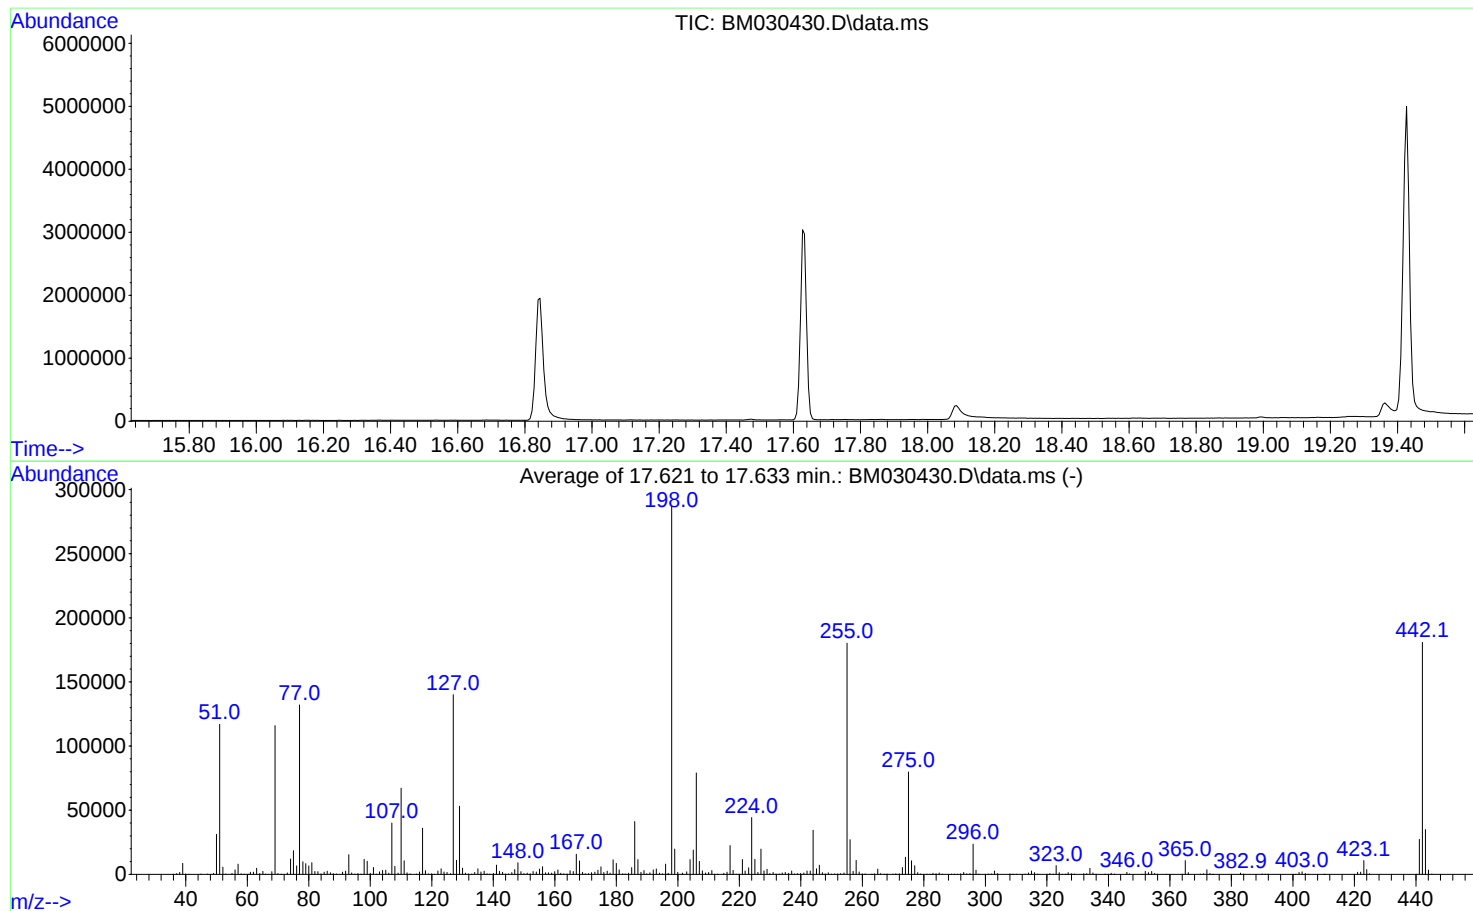




AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2465

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.8	116969	PASS
68	69	0.00	2	1.8	2102	PASS
69	198	0.00	100	40.5	116053	PASS
70	69	0.00	2	0.5	634	PASS
127	198	10	80	48.8	140075	PASS
197	198	0.00	2	0.2	524	PASS
198	198	100	100	100.0	286763	PASS
199	198	5	9	6.9	19686	PASS
275	198	10	60	27.8	79824	PASS
365	198	1	100	3.8	10758	PASS
441	198	0.01	100	9.5	27369	PASS
442	442	50	100	100.0	180923	PASS
443	442	15	24	19.3	34880	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061421\
Data File : BM030430.D
Acq On : 14 Jun 2021 10:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jun 14 11:24:11 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 11 14:10:50 2021
Response via : Initial Calibration

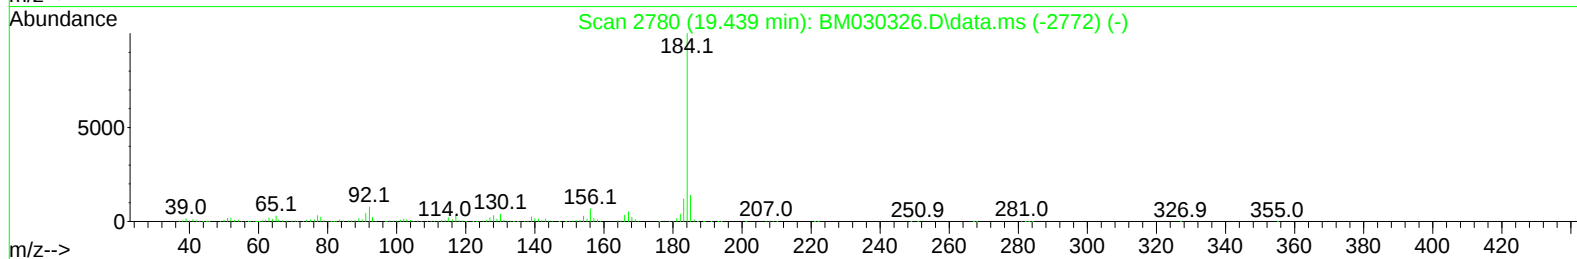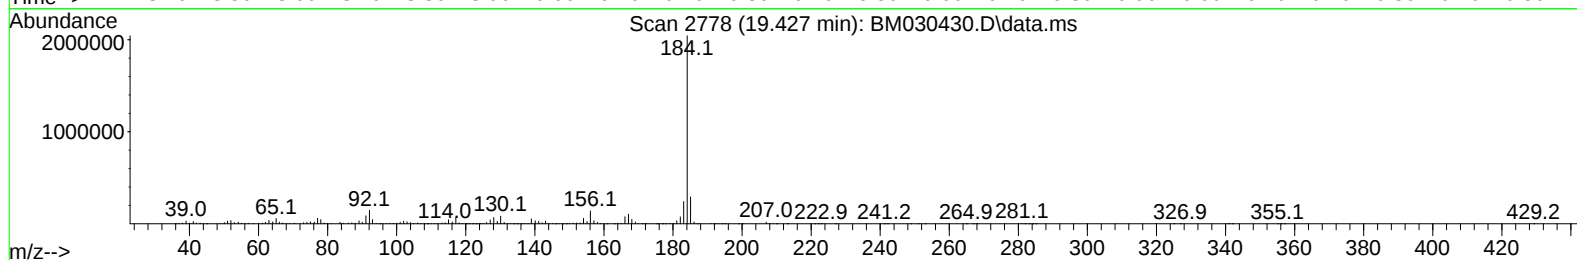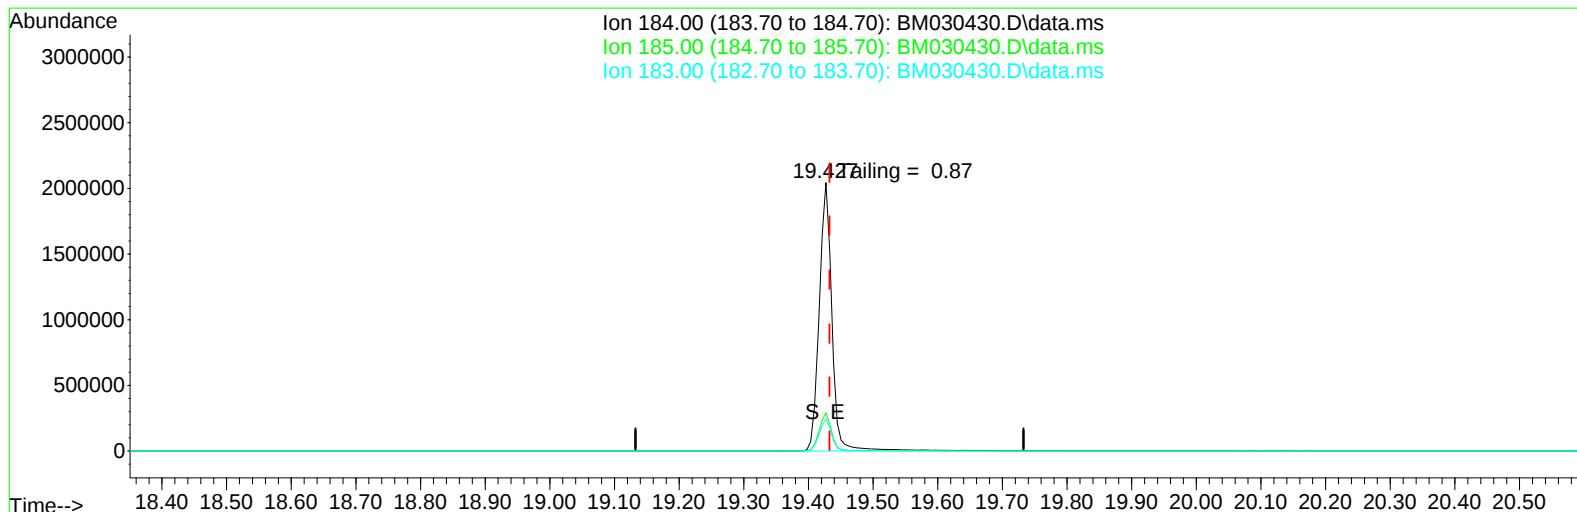

TIC: BM030430.D\data.ms




(77) Benzidine**19.427min (-0.006) 127785.61 ng****response 2790047**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	14.27
183.00	12.30	11.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061421\
Data File : BM030430.D
Acq On : 14 Jun 2021 10:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jun 14 11:24:11 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 11 14:10:50 2021
Response via : Initial Calibration

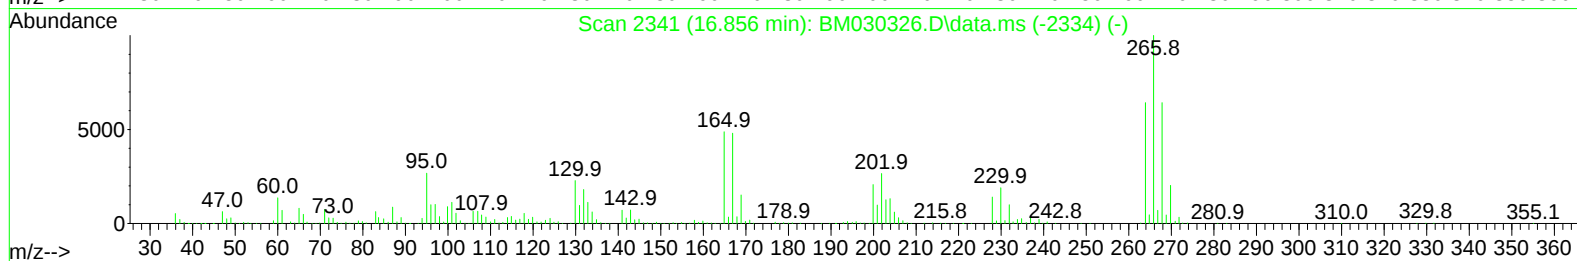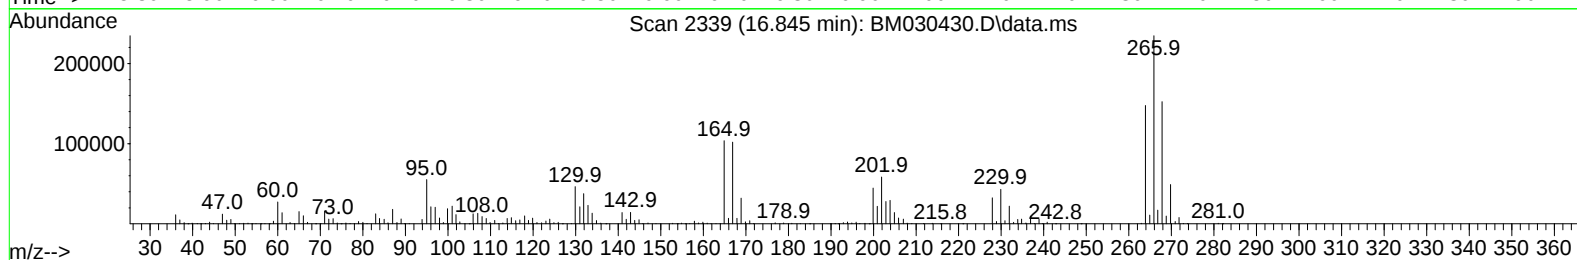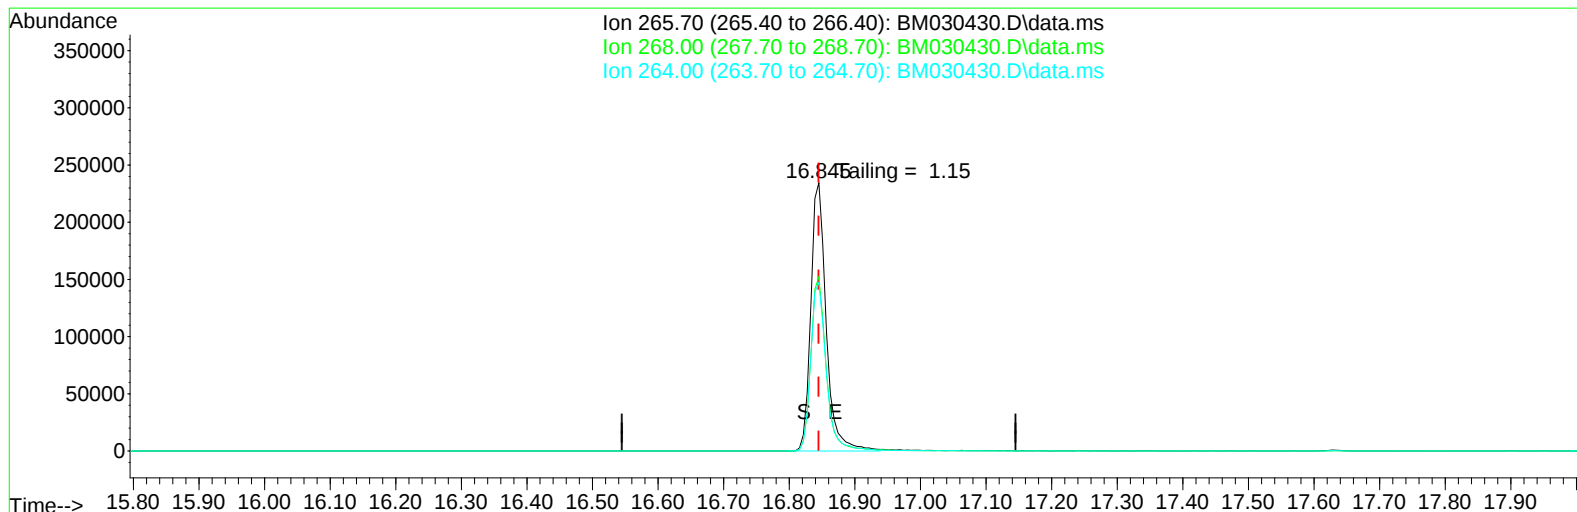

TIC: BM030430.D\data.ms

(70) Pentachlorophenol (C)

16.845min (+ 0.000) 765254.81 ng

response 384697

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.00	65.00
264.00	64.90	62.90
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/14/2021	BNA_M	<u>BM030430.D</u>
Compound Name	Response	Retention Time
DDT	1353843	20.65
DDD	11155	20.22
DDE	2432	19.7
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13587	1367430	0.99

Instrument :
BNA_M
ClientSampleId :
DFTPP