
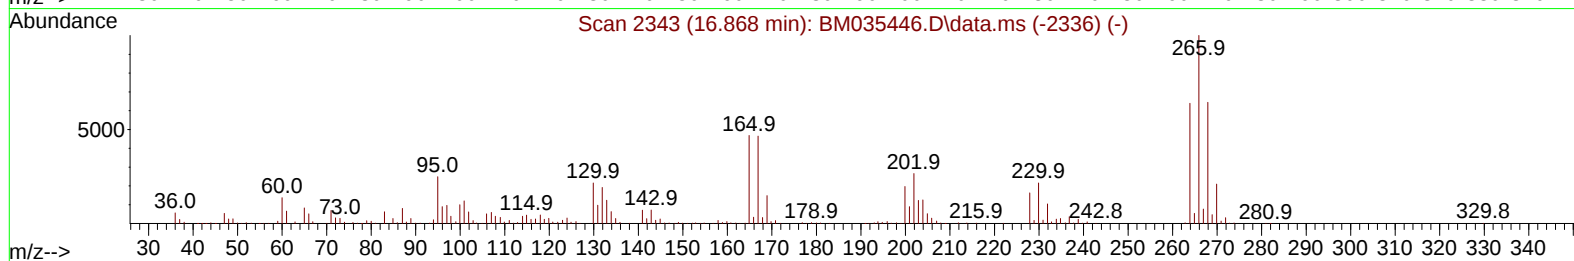
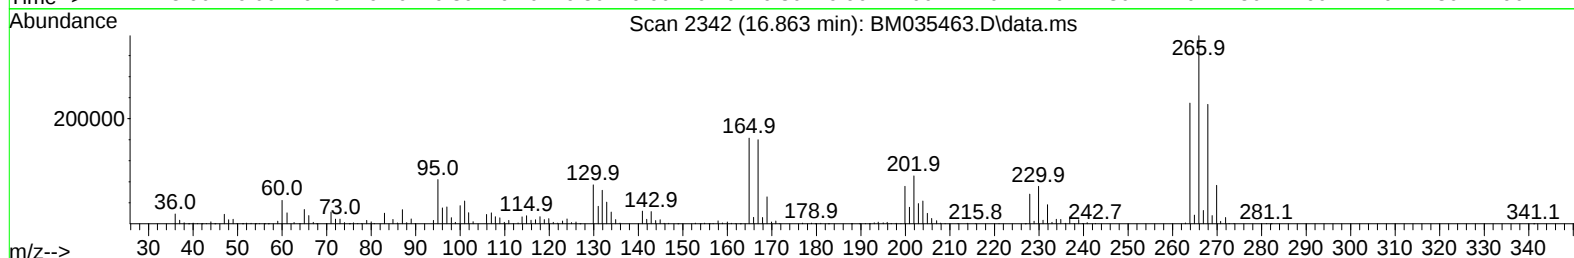


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061422\
 Data File : BM035463.D
 Acq On : 14 Jun 2022 12:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 15 04:31:32 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 10 16:05:33 2022
 Response via : Initial Calibration

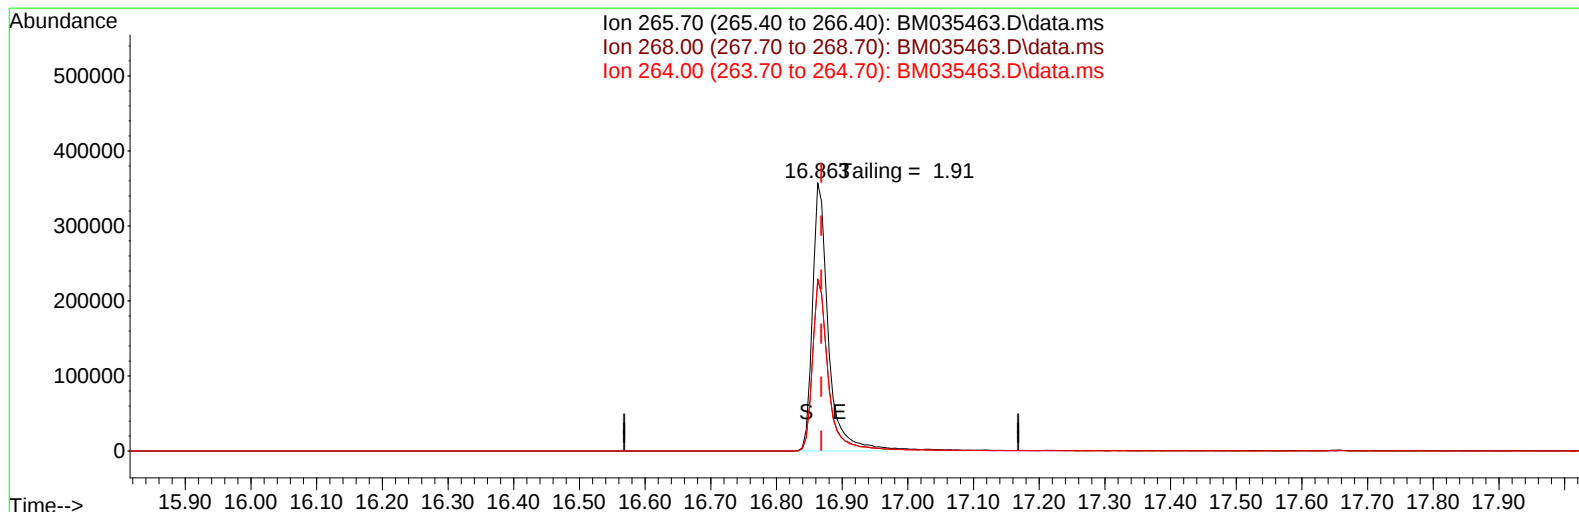

TIC: BM035463.D\data.ms

(70) Pentachlorophenol (C)




16.863min (-0.005) 0.00 ng

response 608750

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	63.51
264.00	63.30	64.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061422\
Data File : BM035463.D
Acq On : 14 Jun 2022 12:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 15 04:31:32 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 10 16:05:33 2022
Response via : Initial Calibration

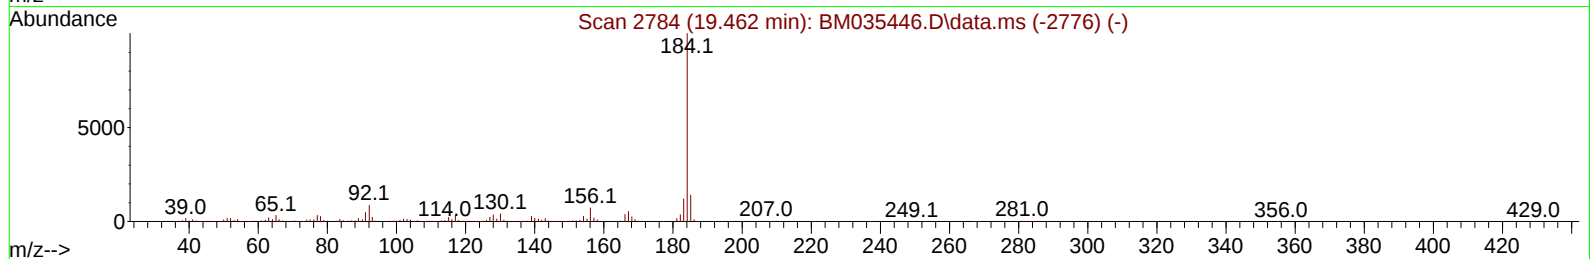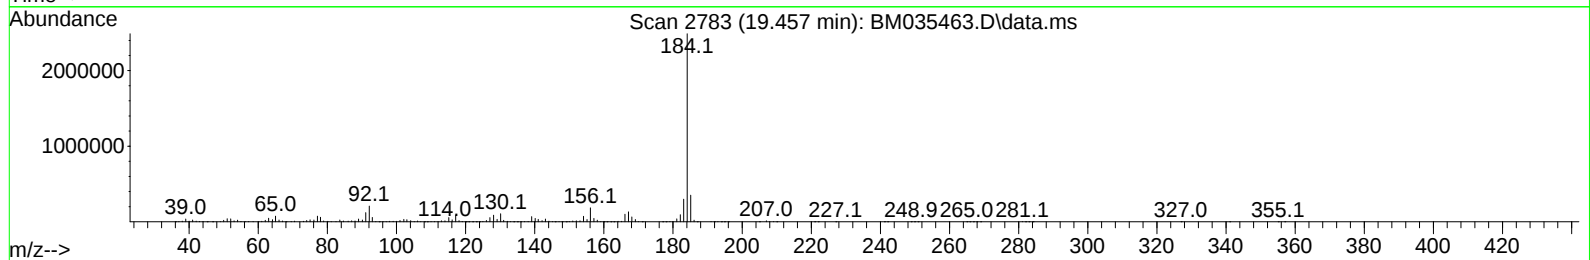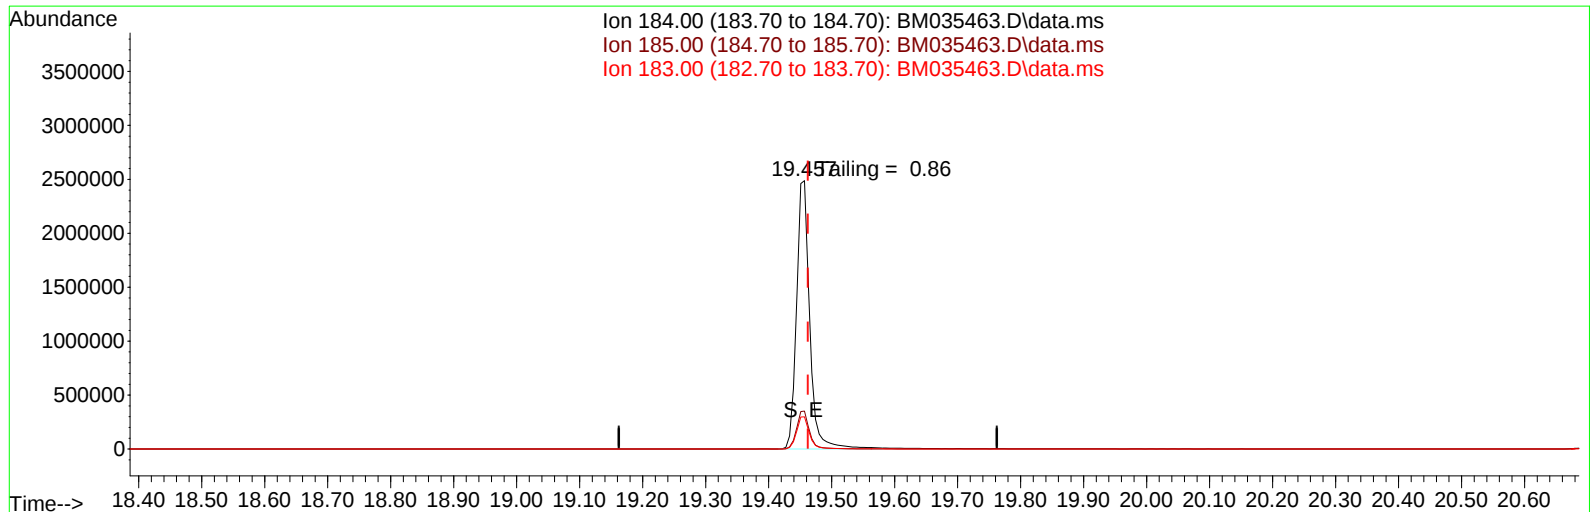

TIC: BM035463.D\data.ms

(77) Benzidine**19.457min (-0.005) 1664791.23 ng****response 3672428**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.15
183.00	11.90	12.01
0.00	0.00	0.00