


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061422\
 Data File : BM035463.D
 Acq On : 14 Jun 2022 12:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 10 16:05:33 2022

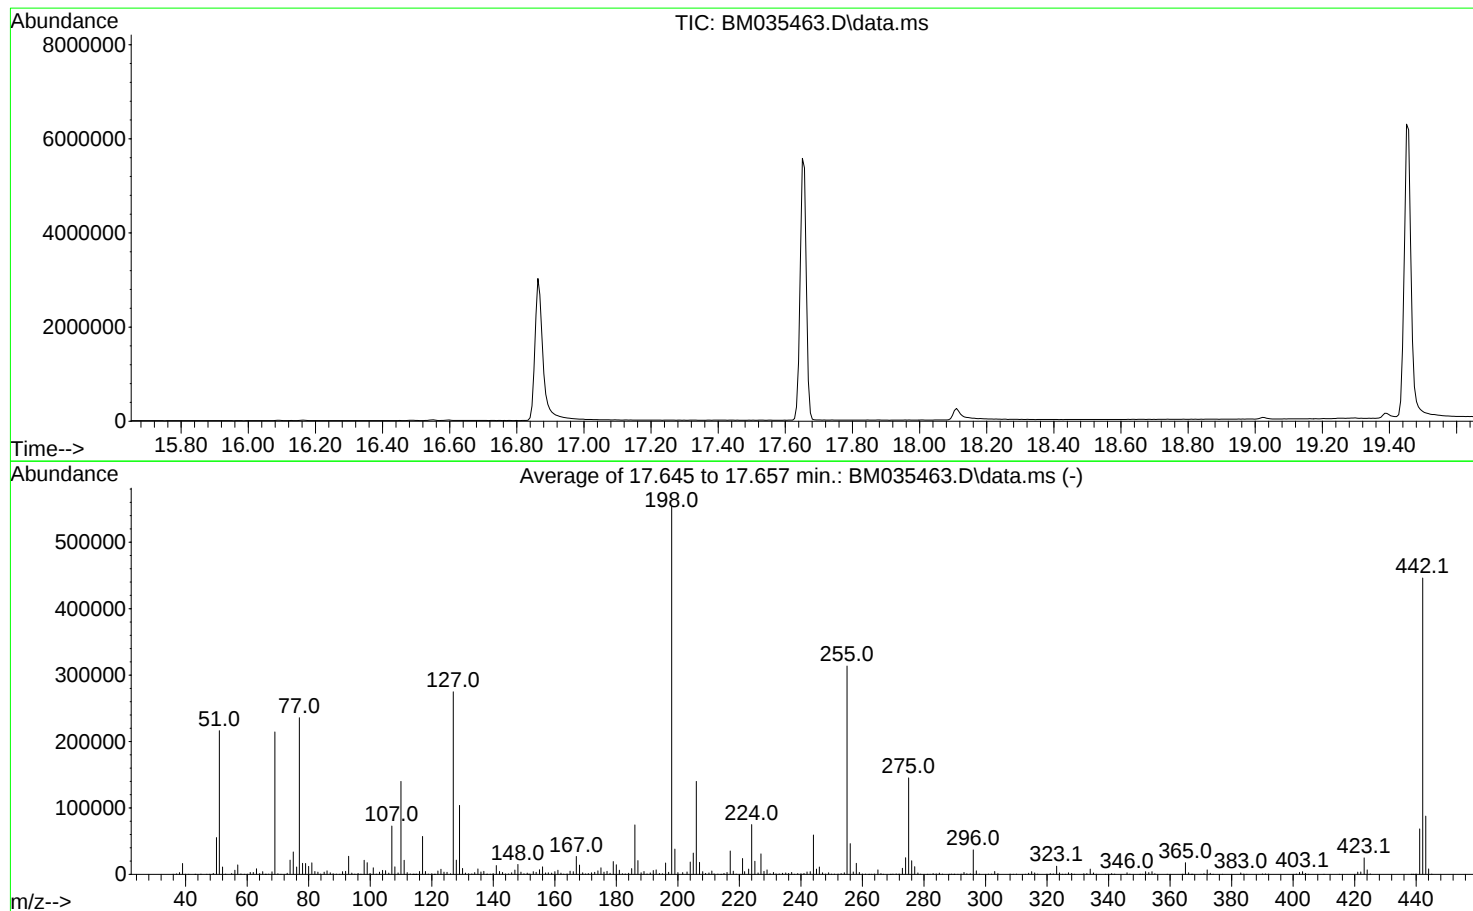




AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.1	216315	PASS
68	69	0.00	2	1.8	3929	PASS
69	198	0.00	100	38.7	214443	PASS
70	69	0.00	2	0.5	1096	PASS
127	198	10	80	49.6	274795	PASS
197	198	0.00	2	0.6	3178	PASS
198	198	100	100	100.0	553835	PASS
199	198	5	9	6.9	38016	PASS
275	198	10	60	26.2	145248	PASS
365	198	1	100	3.2	17506	PASS
441	198	0.01	100	12.3	68323	PASS
442	442	50	100	100.0	446144	PASS
443	442	15	24	19.6	87656	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061422\
Data File : BM035463.D
Acq On : 14 Jun 2022 12:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jun 15 04:31:32 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 10 16:05:33 2022
Response via : Initial Calibration

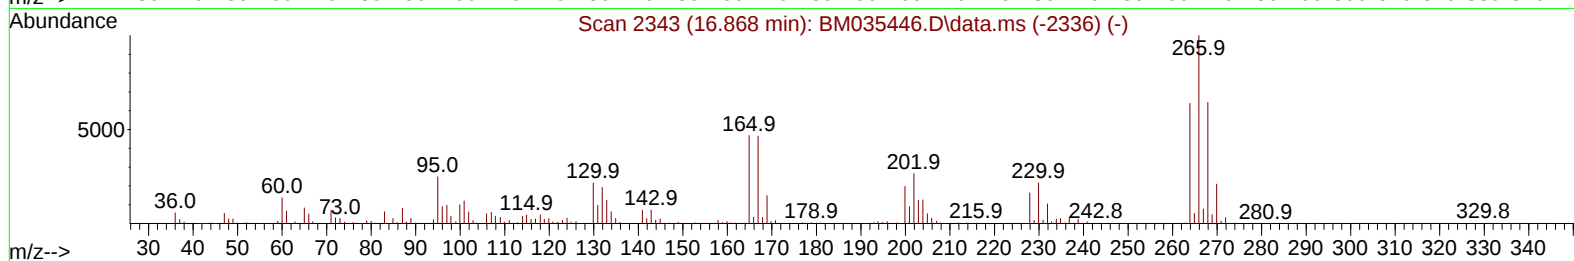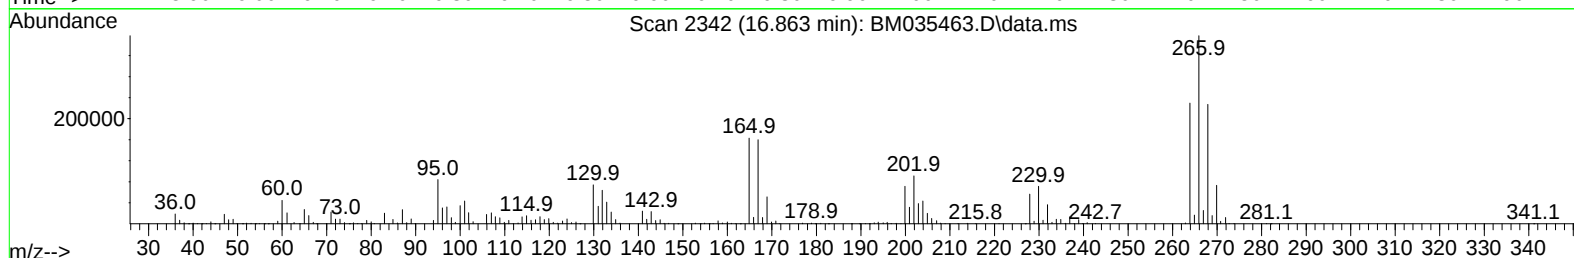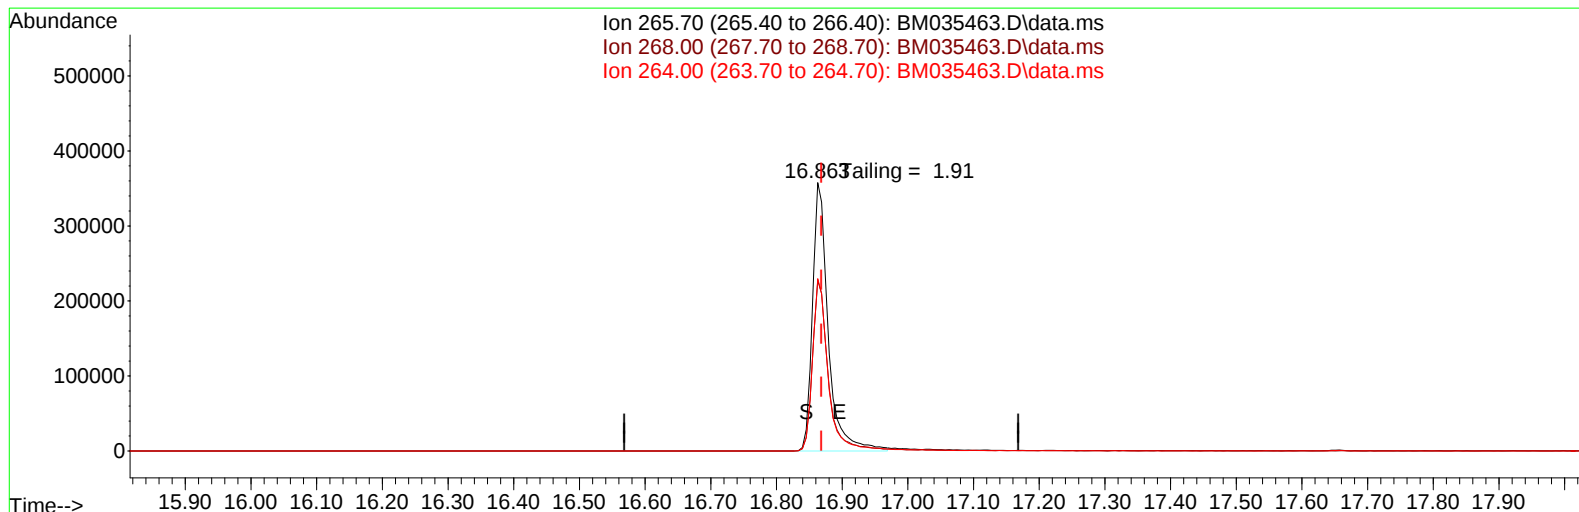

TIC: BM035463.D\data.ms

(70) Pentachlorophenol (C)

16.863min (-0.005) 0.00 ng




response 608750

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	63.51
264.00	63.30	64.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061422\
Data File : BM035463.D
Acq On : 14 Jun 2022 12:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jun 15 04:31:32 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 10 16:05:33 2022
Response via : Initial Calibration

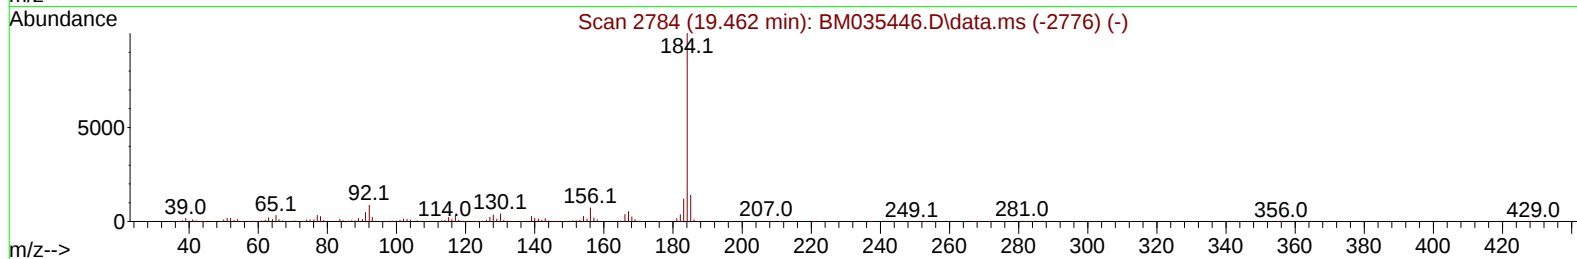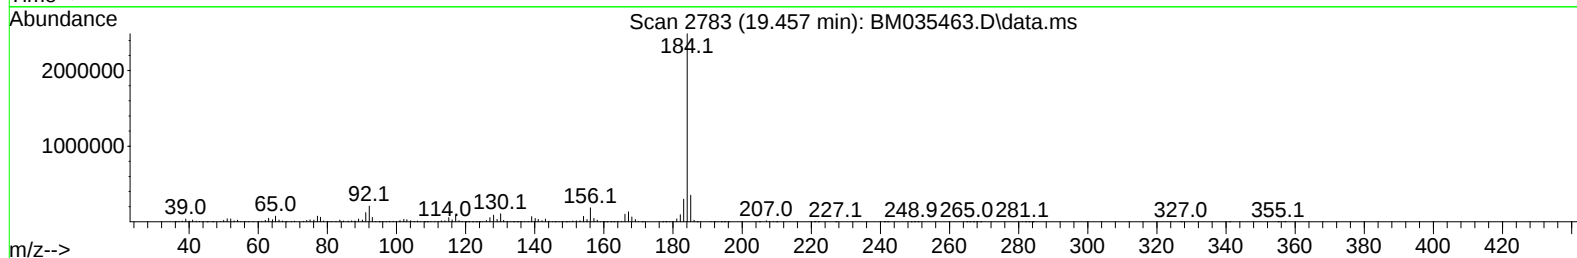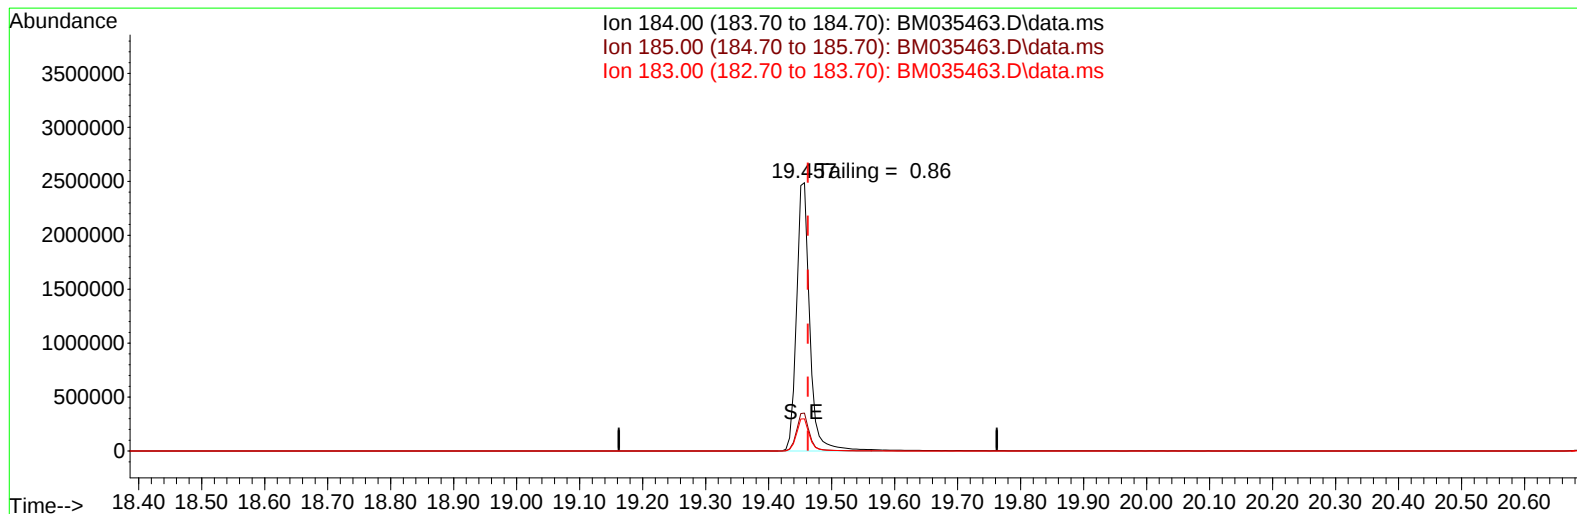

TIC: BM035463.D\data.ms

(77) Benzidine

19.457min (-0.005) 1664791.23 ng

response 3672428

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.15
183.00	11.90	12.01
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/14/2022	BNA_M	<u>BM035463.D</u>
Compound Name	Response	Retention Time
DDT	1838655	20.686
DDD	16221	20.298
DDE	4566	19.751
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
20787	1859442	1.12

Instrument :
BNA_M
ClientSampleId :
DFTPP