

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061424\
 Data File : BM046033.D
 Acq On : 14 Jun 2024 11:04
 Operator : MA/JU
 Sample : PB161357BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK357

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM046033.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.034	5	8	19	rBV	33020	53395	2.14%	0.170%
2	3.452	76	79	102	rBV	320941	746806	29.89%	2.373%
3	3.987	167	170	171	rBV3	2854	3237	0.13%	0.010%
4	4.140	193	196	200	rVB3	8326	8942	0.36%	0.028%
5	4.210	206	208	212	rBV5	2443	3283	0.13%	0.010%
6	4.587	270	272	274	rBV3	2454	2855	0.11%	0.009%
7	4.775	302	304	306	rBV3	2442	2745	0.11%	0.009%
8	5.222	378	380	383	rVB4	3054	3214	0.13%	0.010%
9	5.316	394	396	399	rVB3	3389	2784	0.11%	0.009%
10	6.069	523	524	528	rVB3	4276	3030	0.12%	0.010%
11	6.410	578	582	583	rBV4	2686	3075	0.12%	0.010%
12	6.563	605	608	611	rBV4	2781	3449	0.14%	0.011%
13	6.693	619	630	643	rBV	540461	1070820	42.86%	3.403%
14	6.798	643	648	665	rVB	391035	713989	28.58%	2.269%
15	6.998	675	682	696	rBV	600839	1031724	41.29%	3.278%
16	7.187	712	714	717	rVB3	3818	4657	0.19%	0.015%
17	7.216	717	719	722	rBV4	3278	4256	0.17%	0.014%
18	7.434	747	756	773	rBV	471556	786148	31.46%	2.498%
19	7.922	835	839	842	rBV5	2000	3153	0.13%	0.010%
20	8.204	879	887	902	rBV	601677	1179908	47.22%	3.749%
21	8.469	931	932	935	rBV3	3655	3159	0.13%	0.010%
22	8.598	947	954	970	rBV	584706	1047252	41.91%	3.328%
23	8.704	970	972	975	rVB3	2585	3162	0.13%	0.010%
24	9.051	1029	1031	1035	rVB5	2474	2955	0.12%	0.009%
25	9.104	1035	1040	1041	rBV4	1771	2779	0.11%	0.009%
26	9.310	1068	1075	1089	rBV	489218	906840	36.29%	2.882%
27	9.475	1101	1103	1107	rVB5	2337	2926	0.12%	0.009%
28	9.863	1161	1169	1191	rBV	540739	1207842	48.34%	3.838%
29	10.004	1191	1193	1196	rVB4	3317	3218	0.13%	0.010%
30	10.075	1204	1205	1207	rBV2	3438	3007	0.12%	0.010%
31	10.098	1207	1209	1214	rVB6	2389	3935	0.16%	0.013%
32	10.198	1219	1226	1236	rBV	628826	1069778	42.82%	3.399%
33	10.386	1249	1258	1279	rBV	488362	1190581	47.65%	3.783%
34	10.945	1350	1353	1355	rBV4	2296	3009	0.12%	0.010%
35	11.192	1393	1395	1398	rBV4	1785	2657	0.11%	0.008%
36	11.380	1423	1427	1429	rBV5	2161	2885	0.12%	0.009%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061424\
 Data File : BM046033.D
 Acq On : 14 Jun 2024 11:04
 Operator : MA/JU
 Sample : PB161357BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK357

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
 Title : SVOA CALIBRATION

37	11.416	1432	1433	1439	rVB6	2858	4255	0.17%	0.014%
38	11.663	1472	1475	1478	rVB4	1793	2517	0.10%	0.008%
39	11.833	1499	1504	1506	rBV5	6517	10624	0.43%	0.034%
40	11.880	1509	1512	1517	rVB7	2684	3639	0.15%	0.012%
41	12.233	1570	1572	1578	rBV4	1844	2512	0.10%	0.008%
42	13.057	1707	1712	1713	rVB5	2478	3259	0.13%	0.010%
43	13.533	1785	1793	1808	rBV	912365	1550079	62.04%	4.926%
44	13.633	1808	1810	1814	rVB5	2509	2678	0.11%	0.009%
45	13.769	1827	1833	1847	rBV	1143718	1827053	73.12%	5.806%
46	13.916	1857	1858	1863	rVB4	2333	2642	0.11%	0.008%
47	13.969	1863	1867	1868	rBV3	2285	2916	0.12%	0.009%
48	14.080	1878	1886	1898	rBV	849483	1283361	51.36%	4.078%
49	14.386	1933	1938	1967	rBV	350198	887067	35.50%	2.819%
50	14.692	1988	1990	1993	rBV4	2530	2932	0.12%	0.009%
51	15.080	2050	2056	2070	rBV	1392097	2077855	83.16%	6.603%
52	15.227	2074	2081	2095	rBV	425544	694384	27.79%	2.207%
53	15.321	2095	2097	2103	rVV7	11321	19530	0.78%	0.062%
54	15.392	2107	2109	2112	rVB4	3803	3346	0.13%	0.011%
55	15.657	2151	2154	2156	rBV4	2470	3059	0.12%	0.010%
56	15.827	2181	2183	2187	rBV5	2180	2779	0.11%	0.009%
57	16.157	2235	2239	2242	rBV3	3025	4448	0.18%	0.014%
58	16.186	2242	2244	2249	rVB6	1994	3673	0.15%	0.012%
59	16.615	2315	2317	2321	rVB5	3626	5537	0.22%	0.018%
60	16.663	2321	2325	2327	rBV4	2926	4478	0.18%	0.014%
61	16.827	2347	2353	2361	rBV	1101398	1444301	57.81%	4.590%
62	16.927	2363	2370	2383	rBV	1485229	2213437	88.59%	7.034%
63	17.427	2452	2455	2457	rBV3	2929	3082	0.12%	0.010%
64	17.486	2461	2465	2467	rBV5	1926	2889	0.12%	0.009%
65	17.774	2508	2514	2526	rBV6	31075	79138	3.17%	0.251%
66	18.045	2558	2560	2564	rBV5	3599	3289	0.13%	0.010%
67	18.309	2604	2605	2607	rBV2	3653	3069	0.12%	0.010%
68	18.345	2609	2611	2615	rVB5	5293	4997	0.20%	0.016%
69	18.792	2684	2687	2690	rVB4	16450	18904	0.76%	0.060%
70	18.868	2695	2700	2704	rBV	15204	23595	0.94%	0.075%
71	18.945	2711	2713	2716	rBV4	4892	5426	0.22%	0.017%
72	19.051	2727	2731	2733	rBV3	18863	23915	0.96%	0.076%
73	19.186	2751	2754	2755	rBV3	9987	10704	0.43%	0.034%
74	19.227	2755	2761	2771	rVB	1825836	2406140	96.30%	7.646%
75	21.045	3065	3070	3079	rBV	1037479	1436168	57.48%	4.564%
76	23.562	3491	3498	3507	rVB2	1169068	2498542	100.00%	7.940%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061424\
Data File : BM046033.D
Acq On : 14 Jun 2024 11:04
Operator : MA/JU
Sample : PB161357BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK357

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
Title : SVOA CALIBRATION

77	23.744	3521	3529	3539	rVB	713448	1799766	72.03%	5.719%
----	--------	------	------	------	-----	--------	---------	--------	--------


Sum of corrected areas: 31469440

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061424\
Data File : BM046033.D
Acq On : 14 Jun 2024 11:04
Operator : MA/JU
Sample : PB161357BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK357

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

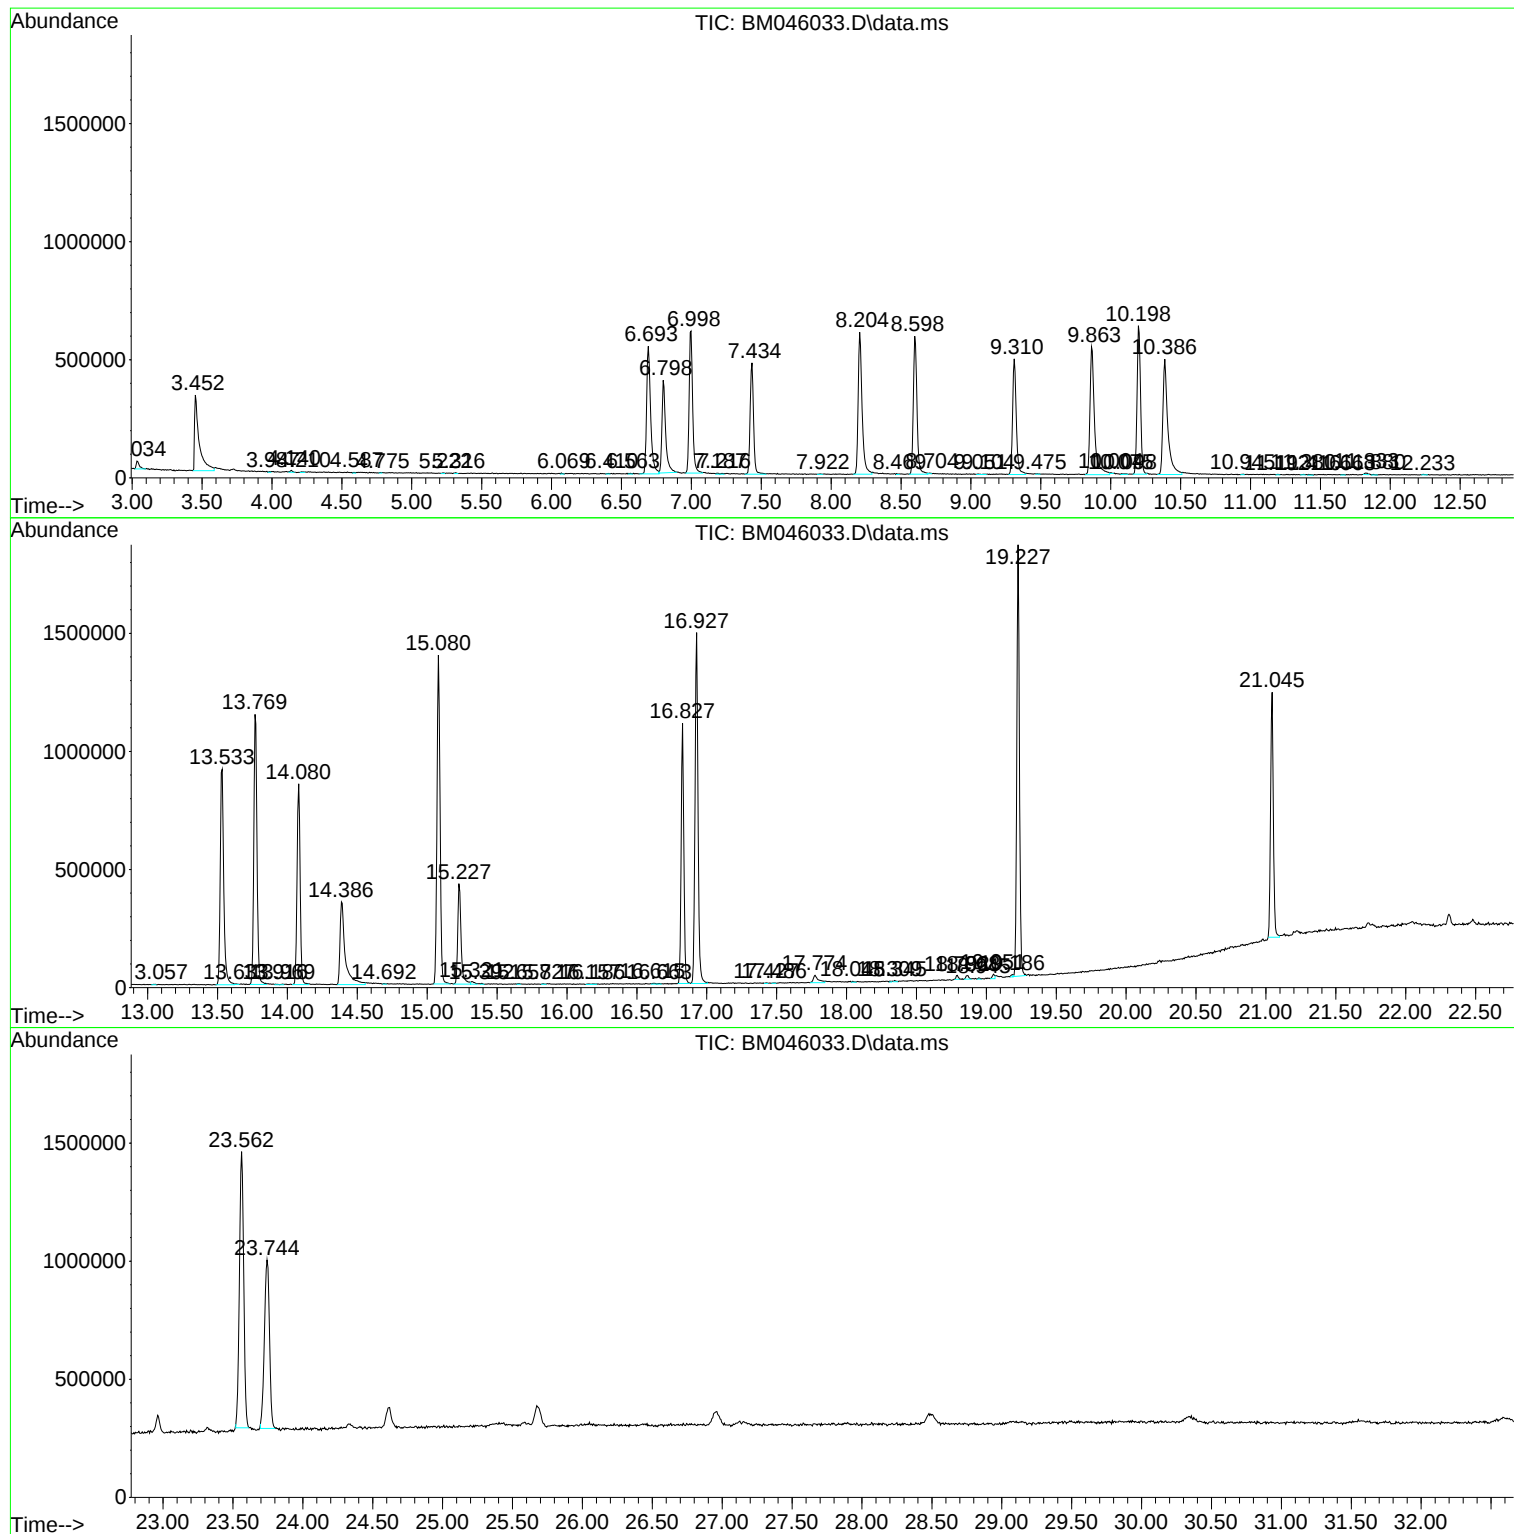

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061424\
Data File : BM046033.D
Acq On : 14 Jun 2024 11:04
Operator : MA/JU
Sample : PB161357BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK357

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061424\
Data File : BM046033.D
Acq On : 14 Jun 2024 11:04
Operator : MA/JU
Sample : PB161357BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK357

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------