

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061515\
 Data File : BM001701.D
 Acq On : 15 Jun 2015 14:56
 Operator : TP/IZ
 Sample : PB84015BL
 Misc : SBLK71
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK71

Quant Time: Jun 16 03:53:29 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061515.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 15 19:33:44 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	61451	20.00	ng/ul	0.00
18) Naphthalene-d8	10.46	136	230766	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.32	164	134566	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.07	188	300817	20.00	ng/ul	0.00
77) Chrysene-d12	21.26	240	363251	20.00	ng/ul	0.00
85) Perylene-d12	23.49	264	372322	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.15	96	7903	6.13	ng/uL	0.00
5) Phenol-d5	6.83	99	143202	30.34	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	82946	31.37	ng/ul	0.00
9) 2-Chlorophenol-d4	7.20	132	115469	30.94	ng/ul	0.00
13) 4-Methylphenol-d8	8.37	113	117382	30.98	ng/ul	0.00
19) Nitrobenzene-d5	8.83	128	52516	32.88	ng/ul	0.00
22) 2-Nitrophenol-d4	9.55	143	59620	34.13	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.07	165	115668	30.93	ng/ul	0.00
29) 4-Chloroaniline-d4	10.60	131	156464	41.13	ng/ul	0.00
43) Dimethylphthalate-d6	13.73	166	337721	33.84	ng/ul	0.00
46) Acenaphthylene-d8	14.01	160	417461	31.91	ng/ul	0.00
51) 4-Nitrophenol-d4	14.52	143	55553	30.18	ng/ul	0.00
57) Fluorene-d10	15.32	176	306668	33.12	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	54313	29.56	ng/ul	0.00
70) Anthracene-d10	17.16	188	476321	33.99	ng/ul	0.00
78) Pyrene-d10	19.46	212	548690	35.66	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.34	264	587983	35.83	ng/ul	0.00


Target Compounds					Qvalue
45) 2,6-Dinitrotoluene	13.73	165	2664	1.30 ng/ul#	32


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061515\
Data File : BM001701.D
Acq On : 15 Jun 2015 14:56
Operator : TP/IZ
Sample : PB84015BL
Misc : SBLK71
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK71

Quant Time: Jun 16 03:53:29 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061515.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 15 19:33:44 2015
Response via : Initial Calibration

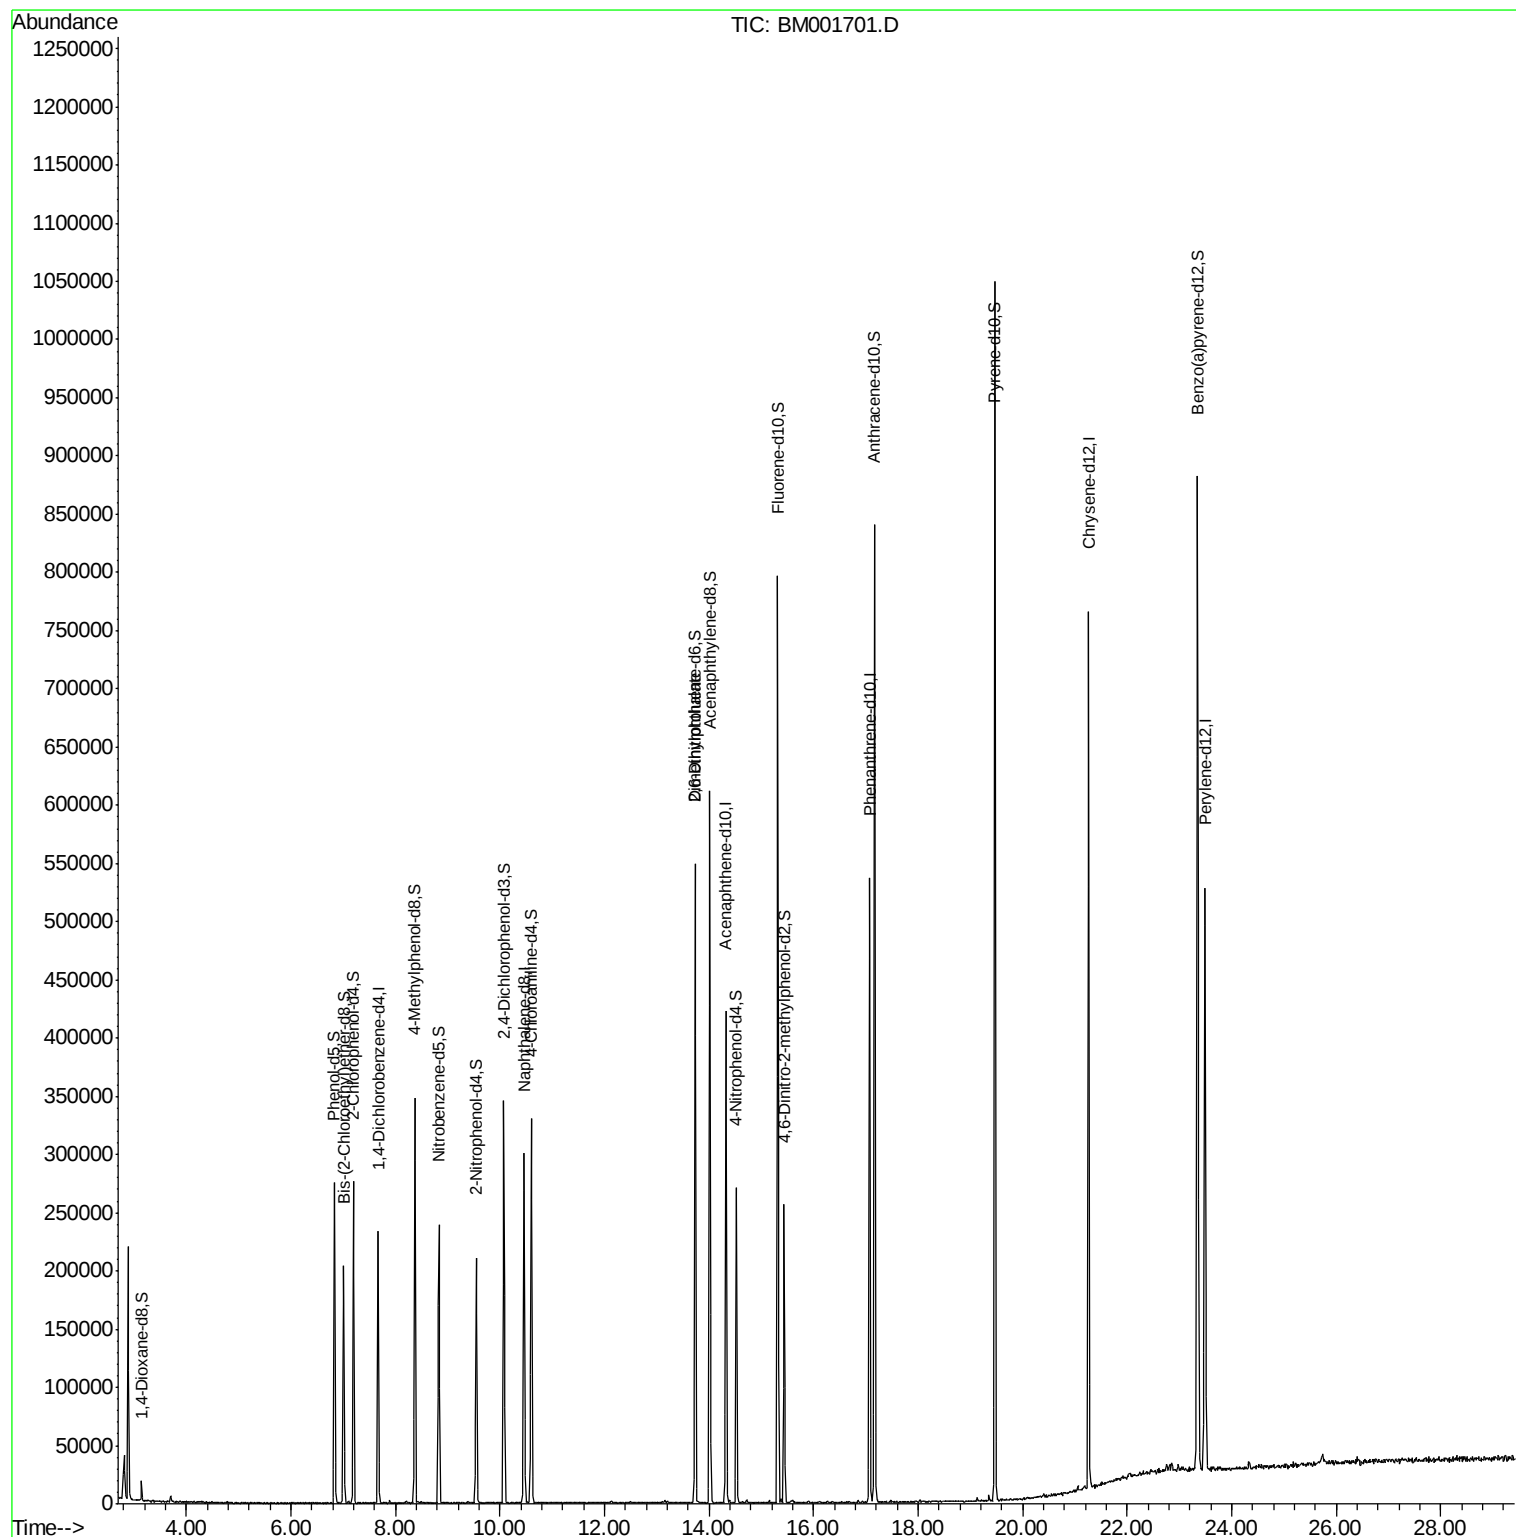


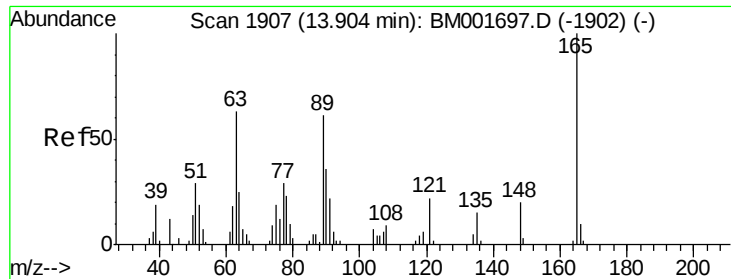

#45
 2,6-Dinitrotoluene
 Concen: 1.30 ng/ul
 RT: 13.73 min Scan# 1878
 Delta R.T. -0.17 min
 Lab File: BM001701.D
 Acq: 15 Jun 2015 14:56

Instrument :
 BNA_M
 ClientSampleId :
 SBLK71

Tgt Ion:165 Resp: 2664
 Ion Ratio Lower Upper
 165 100
 89 0.0 49.1 73.7#
 121 37.8 17.4 26.2#

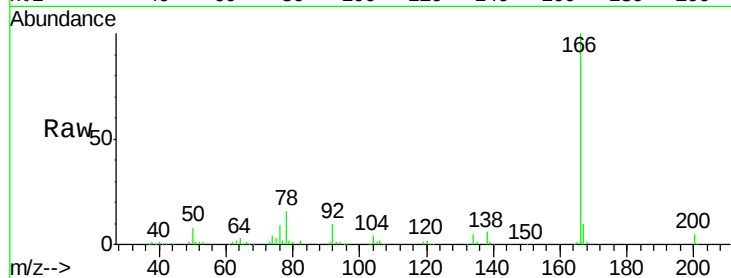

Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 89.00 (88.70 to 89.70): BM0
 Ion 121.00 (120.70 to 121.70): E

