


Data Path : Z:\HPCHEM1\BNA_M\Data\BM061515\
 Data File : BM001694.D
 Acq On : 15 Jun 2015 09:55
 Operator : TP/IZ
 Sample : DFTPP59
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP59

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM031115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Mar 28 05:37:34 2015

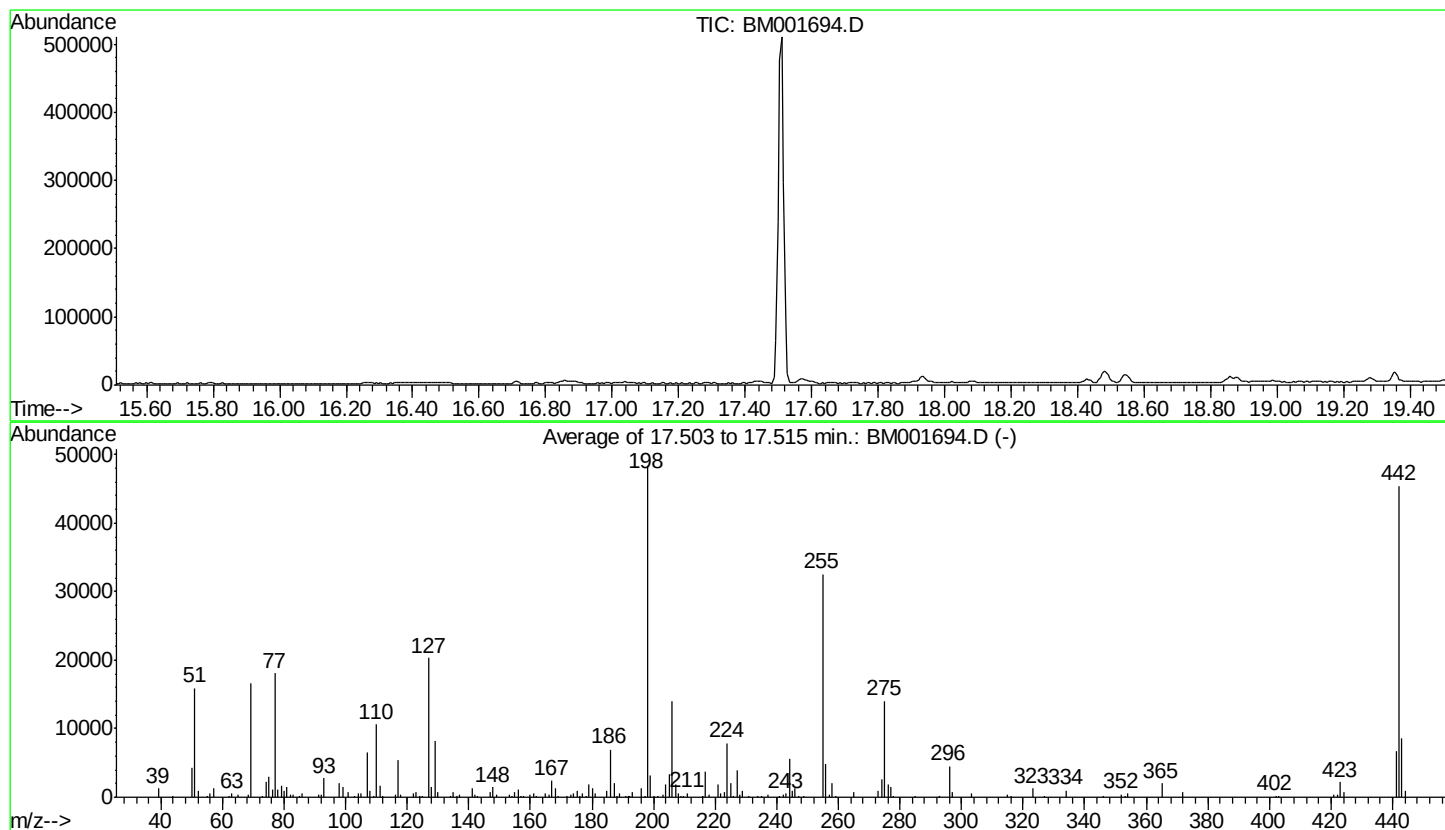

AutoFind: Scans 2519, 2520, 2521; Background Corrected with Scan 2513


Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.9	15931	PASS
68	69	0.00	2	1.9	322	PASS
69	198	0.00	100	34.6	16720	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.0	20344	PASS
197	198	0.00	2	0.3	148	PASS
198	198	100	100	100.0	48389	PASS
199	198	5	9	6.5	3133	PASS
275	198	10	60	29.0	14013	PASS
365	198	1	100	4.2	2025	PASS
441	442	0.01	24	15.0	6821	PASS
442	198	50	100	93.9	45416	PASS
443	442	15	24	19.1	8680	PASS

Data Path : Z:\HPCHEM1\BNA_M\Data\BM061515\
 Data File : BM001694.D
 Acq On : 15 Jun 2015 09:55
 Operator : TP/IZ
 Sample : DFTPP59
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP59

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM031115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Mar 28 05:37:34 2015

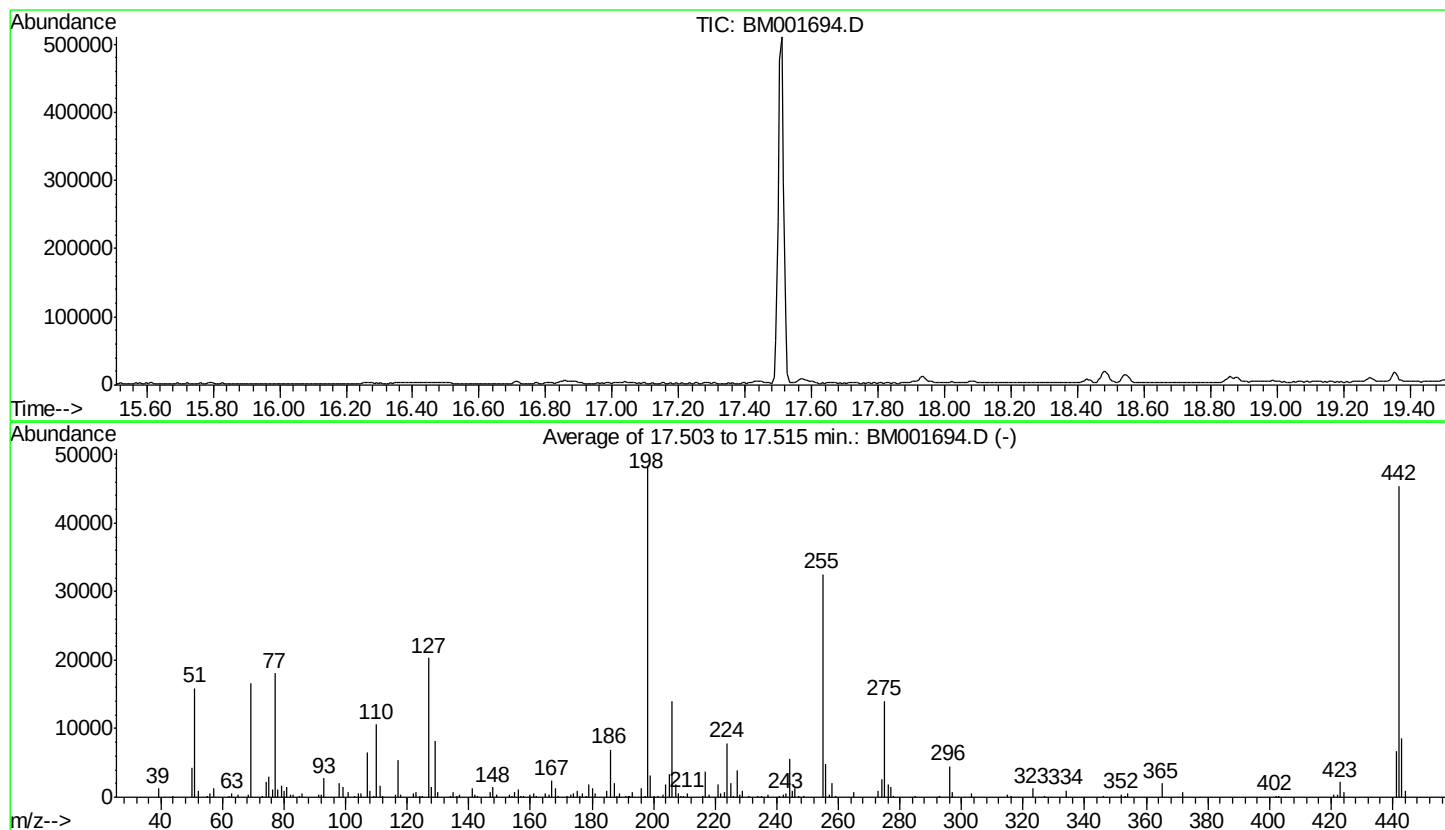

AutoFind: Scans 2519, 2520, 2521; Background Corrected with Scan 2513

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.9	15931	PASS
68	69	0.00	2	1.9	322	PASS
69	198	0.00	100	34.6	16720	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.0	20344	PASS
197	198	0.00	2	0.3	148	PASS
198	198	100	100	100.0	48389	PASS
199	198	5	9	6.5	3133	PASS
275	198	10	60	29.0	14013	PASS
365	198	1	100	4.2	2025	PASS
441	442	0.01	24	15.0	6821	PASS
442	198	50	100	93.9	45416	PASS
443	442	15	24	19.1	8680	PASS

m/z	Abundance
39.10	1548.0
40.00	853.0
44.00	1278.0
50.00	5418.0
51.10	20744.0
52.00	1182.0
56.00	598.0
57.00	1526.0
62.00	452.0
63.00	776.0
65.00	345.0
68.10	461.0
69.00	20664.0
73.00	707.0
74.00	2652.0
75.00	3723.0
76.10	1389.0
77.10	22816.0
78.00	1436.0
79.00	2050.0
80.00	1365.0
81.00	1769.0
82.00	679.0
83.10	382.0
85.10	323.0
86.00	645.0
91.10	421.0
92.00	683.0
93.00	3417.0
98.00	2329.0
99.00	1861.0
100.90	898.0
102.90	414.0
104.10	552.0
104.90	747.0
107.00	7615.0
108.00	1207.0
110.00	12694.0
111.00	2001.0
116.10	771.0
117.00	6560.0
118.00	583.0
122.10	589.0
122.90	719.0
124.00	338.0
127.00	24208.0
128.00	1954.0
129.00	9585.0
129.90	689.0
134.00	381.0
135.00	1044.0
135.90	536.0
137.00	492.0
141.00	1385.0
142.10	543.0
142.80	351.0
147.10	819.0
148.00	1792.0
149.10	536.0
153.00	522.0
154.00	405.0
154.90	937.0
156.00	1215.0
157.00	315.0
157.80	351.0
160.00	486.0
160.90	542.0
161.90	336.0
165.00	641.0
165.90	420.0
167.00	2758.0
168.00	1710.0
171.80	301.0
173.00	494.0
174.00	673.0
175.00	1084.0
176.00	389.0
177.10	514.0
177.90	330.0
179.00	2587.0
180.00	1481.0
181.00	619.0
184.90	1208.0
186.00	7955.0
187.00	2269.0
187.90	339.0
189.00	638.0
191.90	654.0
193.00	847.0
196.00	1557.0
198.00	54856.0

Instrument :
BNA_M
ClientSampleId :
DFTPP59

199.00	3681.0
201.30	353.0
203.00	444.0
204.00	2045.0
205.00	3822.0
206.00	15599.0
207.00	2641.0
207.90	701.0
209.80	302.0
211.10	563.0
215.80	300.0
217.00	4070.0
218.00	663.0
221.00	2275.0
221.90	595.0
223.00	820.0
224.00	8469.0
225.00	2551.0
227.00	4348.0
228.00	466.0
229.00	1001.0
231.00	338.0
233.90	303.0
234.90	330.0
237.00	583.0
240.90	338.0
242.00	502.0
243.00	563.0
244.00	5998.0
245.00	832.0
246.00	1404.0
246.90	350.0
255.00	34744.0
256.00	4866.0
256.90	497.0
257.90	2088.0
259.00	405.0
265.00	944.0
273.00	830.0
274.00	2726.0
275.00	14309.0
276.00	1933.0
277.00	1598.0
278.00	314.0
292.80	328.0
296.00	4612.0
297.00	755.0
303.00	562.0
315.00	447.0
323.10	1400.0
334.10	970.0
352.10	473.0
353.00	303.0
354.10	632.0
365.00	1683.0
372.00	689.0
421.00	360.0
422.00	374.0
423.00	1915.0
424.10	694.0
441.10	5738.0
442.10	39584.0
443.00	7988.0
444.00	1029.0

Instrument :
BNA_M
ClientSampleId :
DFTPP59

m/z	Abundance
39.00	1589.0
40.00	811.0
44.00	1129.0
50.10	4869.0
51.10	18232.0
52.00	1174.0
55.10	333.0
55.90	520.0
57.00	1377.0
63.00	713.0
65.00	532.0
68.20	507.0
69.00	19864.0
73.00	596.0
74.00	2418.0
75.00	3327.0
76.00	1159.0
77.00	20880.0
78.10	1338.0
79.00	1834.0
79.90	1217.0
81.00	1708.0
81.90	395.0
83.00	504.0
85.00	371.0
85.90	493.0
91.00	467.0
92.00	619.0
93.00	3199.0
98.00	2480.0
99.00	1580.0
101.00	1059.0
103.00	309.0
104.00	729.0
105.00	750.0
107.00	7828.0
108.00	1106.0
109.00	355.0
110.00	12390.0
111.00	2182.0
112.00	339.0
116.00	537.0
117.00	6493.0
118.00	445.0
122.00	833.0
123.00	873.0
123.90	412.0
124.90	370.0
127.00	23552.0
128.00	1703.0
129.00	9834.0
130.00	926.0
135.00	794.0
136.00	309.0
136.90	483.0
141.00	1698.0
142.00	449.0
147.00	887.0
147.90	1603.0
148.90	348.0
153.00	551.0
153.90	363.0
155.00	1072.0
156.00	1259.0
159.90	427.0
161.00	664.0
164.90	628.0
166.00	460.0
167.00	2604.0
168.00	1369.0
169.00	341.0
172.90	393.0
174.00	494.0
175.00	958.0
176.90	756.0
178.90	2042.0
180.00	1817.0
181.00	804.0
185.00	1114.0
186.00	7539.0
187.10	2450.0
188.00	390.0
188.90	517.0
191.00	563.0
192.10	716.0
193.00	1000.0
196.00	1756.0
197.10	444.0
198.00	56088.0
198.90	3432.0
200.00	425.0

Instrument :
BNA_M
ClientSampleId :
DFTPP59

202.90	576.0
204.00	2178.0
205.10	3729.0
206.00	16520.0
207.00	2804.0
208.00	810.0
208.90	333.0
211.00	802.0
216.10	370.0
216.90	4782.0
218.00	578.0
220.90	2012.0
221.70	859.0
223.00	1023.0
224.00	9727.0
225.00	2309.0
225.90	457.0
227.00	4464.0
228.00	646.0
229.00	1056.0
234.00	350.0
235.00	494.0
237.10	361.0
241.90	404.0
243.10	572.0
244.10	6550.0
245.00	1102.0
245.90	1454.0
246.90	364.0
248.90	306.0
255.00	39256.0
256.00	5966.0
257.00	590.0
258.00	2457.0
258.90	388.0
265.00	929.0
273.00	1131.0
274.00	3043.0
275.00	17280.0
276.00	2378.0
276.90	1798.0
285.00	341.0
293.00	401.0
296.00	5391.0
297.00	853.0
303.00	571.0
315.00	529.0
315.90	303.0
323.00	1365.0
326.90	490.0
334.00	1209.0
346.10	391.0
352.10	552.0
353.10	321.0
354.00	651.0
365.00	2523.0
372.00	903.0
402.10	338.0
402.90	339.0
421.00	454.0
422.00	553.0
423.10	2301.0
424.00	817.0
441.10	8678.0
442.10	55688.0
443.00	10735.0
444.00	1100.0

Instrument :
BNA_M
ClientSampleId :
DFTPP59

m/z	Abundance
39.00	587.0
40.00	794.0
44.00	1505.0
50.10	2373.0
51.10	8818.0
52.00	361.0
56.00	358.0
57.10	928.0
69.00	9634.0
73.10	486.0
74.00	1557.0
75.00	1798.0
76.00	611.0
77.10	10641.0
78.00	820.0
79.00	1015.0
79.90	495.0
81.00	1017.0
83.00	320.0
86.10	367.0
93.00	1654.0
98.00	1238.0
99.00	947.0
101.00	505.0
103.90	316.0
104.90	383.0
107.00	4157.0
107.90	617.0
110.00	6632.0
111.00	1004.0
117.00	3383.0
118.00	349.0
123.00	394.0
127.00	13272.0
128.00	1051.0
129.00	5481.0
130.00	404.0
134.90	660.0
136.90	372.0
140.90	679.0
147.00	663.0
147.90	856.0
156.00	677.0
161.00	486.0
164.90	367.0
167.00	1678.0
168.00	848.0
173.90	469.0
175.00	650.0
176.90	425.0
179.00	1213.0
180.00	799.0
181.00	461.0
185.00	556.0
186.00	5244.0
187.00	1535.0
188.90	358.0
193.00	446.0
196.00	903.0
198.00	34224.0
198.90	2287.0
204.00	1428.0
205.10	2474.0
206.00	9696.0
207.10	1945.0
208.00	416.0
211.00	420.0
217.00	2642.0
220.90	1457.0
221.90	329.0
223.00	627.0
224.00	5506.0
225.00	1570.0
227.00	2734.0
228.00	309.0
229.00	628.0
242.90	300.0
244.10	4245.0
245.10	674.0
245.90	1002.0
255.00	23792.0
256.00	3523.0
258.00	1651.0
265.10	483.0
273.00	649.0
274.00	2179.0
275.00	10452.0
276.00	1293.0
277.00	1182.0
296.10	3618.0
297.00	508.0

Instrument :
BNA_M
ClientSampleId :
DFTPP59

303.10	420.0
314.90	359.0
323.10	1028.0
326.90	320.0
334.00	881.0
351.90	376.0
354.00	313.0
365.00	1871.0
372.00	642.0
401.90	349.0
402.80	301.0
421.00	387.0
423.10	2427.0
424.10	598.0
441.10	6047.0
442.10	40976.0
443.10	7319.0
444.10	653.0

Instrument :
BNA_M
ClientSampleId :
DFTPP59

Scan 2513 (17.468 min): BM001694.D
DFTPP59

m/z	Abundance
40.00	819.0
44.00	1135.0
73.00	449.0
207.00	668.0

Instrument :
BNA_M
ClientSampleId :
DFTPP59