


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061516\
 Data File : BM005784.D
 Acq On : 14 Jun 2016 14:24
 Operator : UM/SJ
 Sample : DFTPP57
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP57

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM041416.M
 Title : SVOA CALIBRATION
 Last Update : Sat Apr 23 01:00:10 2016

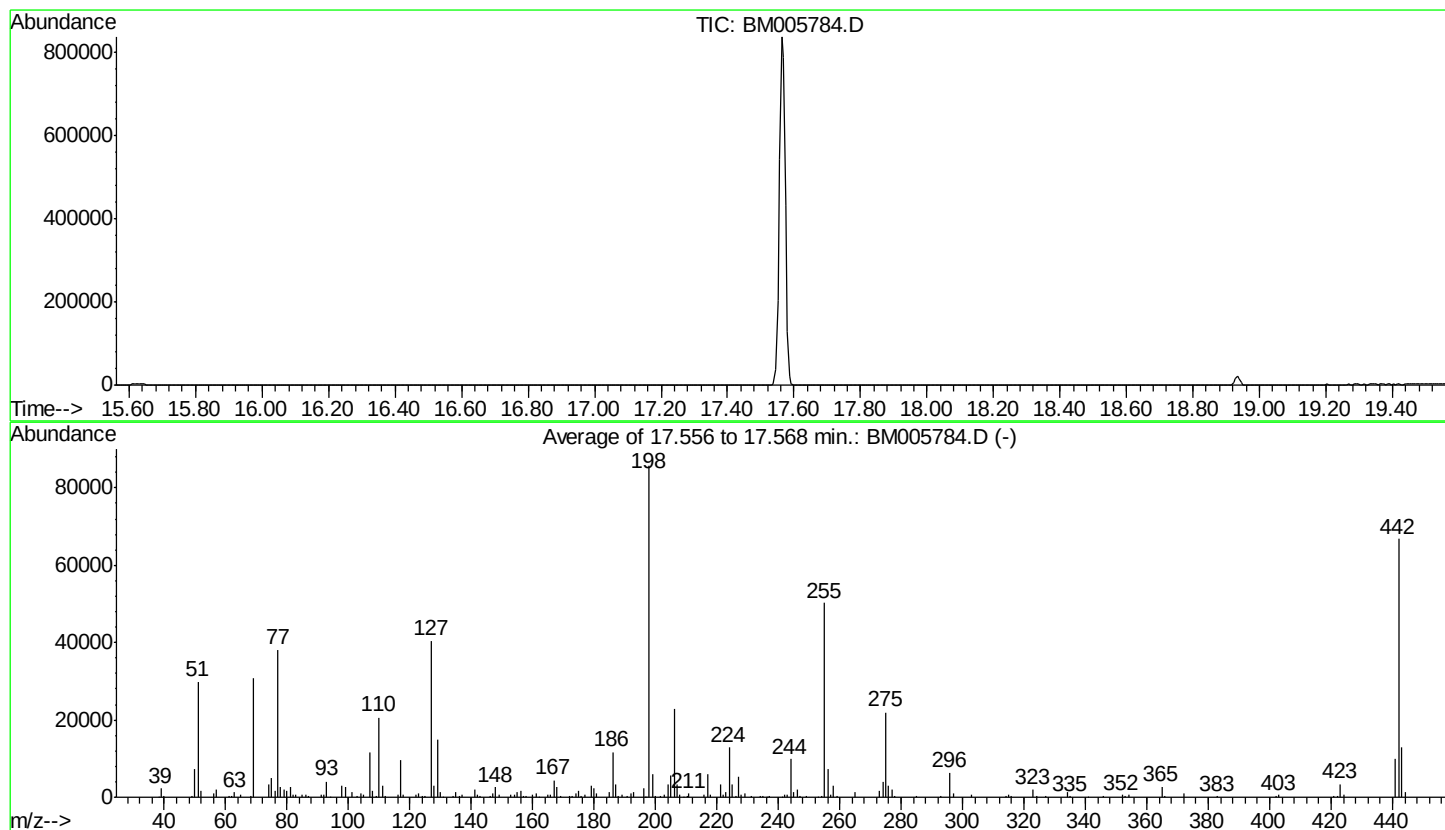

AutoFind: Scans 2545, 2546, 2547; Background Corrected with Scan 2540

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.7	29802	PASS
68	69	0.00	2	1.5	455	PASS
69	198	0.00	100	35.9	30770	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.2	40522	PASS
197	198	0.00	2	0.2	148	PASS
198	198	100	100	100.0	85770	PASS
199	198	5	9	6.9	5937	PASS
275	198	10	60	25.6	21972	PASS
365	198	1	100	3.1	2701	PASS
441	443	0.01	100	78.4	10032	PASS
442	198	50	100	77.9	66816	PASS
443	442	15	24	19.1	12793	PASS

m/z	Abundance
39.00	1937.0
40.00	324.0
50.00	6533.0
51.00	25464.0
52.00	1397.0
56.00	801.0
57.00	1729.0
60.90	338.0
62.00	389.0
63.00	945.0
65.00	581.0
68.00	442.0
69.00	26408.0
74.00	2894.0
75.00	4473.0
76.00	1519.0
77.00	33184.0
78.00	2396.0
79.00	1834.0
80.00	1512.0
81.00	2262.0
82.00	552.0
83.00	533.0
85.00	422.0
85.90	710.0
87.00	322.0
90.90	418.0
91.90	576.0
93.00	3535.0
98.00	2615.0
99.00	2350.0
100.90	1136.0
103.00	436.0
104.00	760.0
105.00	612.0
107.00	9723.0
108.00	1449.0
110.00	17224.0
111.00	2493.0
115.90	469.0
117.00	7644.0
117.90	568.0
121.90	544.0
123.00	921.0
123.90	465.0
124.90	412.0
127.00	32456.0
128.00	2629.0
129.00	12361.0
129.90	1167.0
133.90	388.0
135.00	1061.0
136.00	370.0
137.00	642.0
140.90	1468.0
142.00	484.0
143.00	414.0
146.90	867.0
147.90	2097.0
149.00	480.0
152.90	523.0
153.90	427.0
155.00	981.0
156.00	1391.0
160.00	539.0
161.00	679.0
164.90	632.0
166.00	513.0
167.00	3447.0
168.00	2469.0
168.90	341.0
171.90	311.0
172.90	370.0
174.00	676.0
175.00	1307.0
175.90	302.0
177.00	589.0
179.00	2350.0
180.00	1934.0
180.90	755.0
185.00	1170.0
186.00	9303.0
187.00	2612.0
188.90	564.0
190.90	336.0
191.90	702.0
193.00	940.0
196.00	1660.0
197.90	64528.0
198.90	4804.0
200.00	360.0

Instrument :
BNA_M
ClientSampleId :
DFTPP57

201.60	310.0
202.90	465.0
204.00	2459.0
205.00	3897.0
206.00	17208.0
207.00	2530.0
208.00	617.0
210.30	359.0
211.00	555.0
215.90	436.0
217.00	4555.0
217.90	651.0
221.10	2450.0
221.90	546.0
223.00	855.0
224.00	9230.0
225.00	2259.0
227.00	3901.0
228.00	560.0
228.90	702.0
231.00	347.0
236.90	335.0
242.00	512.0
243.00	398.0
244.00	6972.0
245.00	1092.0
246.00	1386.0
246.90	306.0
254.00	310.0
255.00	35200.0
256.00	5268.0
257.00	386.0
258.00	2289.0
258.90	330.0
265.00	865.0
273.00	1105.0
274.00	2876.0
275.00	15460.0
276.00	2053.0
276.90	1319.0
278.00	320.0
296.00	4589.0
297.00	658.0
303.00	383.0
314.90	452.0
323.00	1252.0
334.00	902.0
352.00	386.0
352.90	309.0
354.00	372.0
365.00	1724.0
372.00	551.0
402.90	342.0
422.00	401.0
423.00	2038.0
424.00	545.0
441.00	5911.0
442.00	39288.0
443.00	8015.0
444.00	714.0

Instrument :
BNA_M
ClientSampleId :
DFTPP57

m/z	Abundance
38.00	343.0
39.00	2457.0
39.90	314.0
44.00	351.0
49.00	403.0
50.00	8444.0
51.00	35608.0
52.00	1727.0
55.90	1028.0
57.00	2483.0
61.00	512.0
61.90	488.0
62.90	1371.0
65.00	879.0
68.00	532.0
69.00	36176.0
74.00	3801.0
75.00	5914.0
76.00	2155.0
77.00	44384.0
78.00	3125.0
79.00	2516.0
80.00	2274.0
81.00	2923.0
82.00	717.0
83.00	688.0
85.00	738.0
85.90	807.0
87.10	410.0
91.00	685.0
92.00	826.0
93.00	4599.0
94.00	319.0
98.00	3563.0
99.00	3018.0
101.00	1847.0
103.00	572.0
103.90	1047.0
105.00	902.0
107.00	13785.0
108.00	2128.0
109.00	318.0
110.00	23976.0
111.00	3729.0
111.90	507.0
116.00	643.0
117.00	11339.0
118.00	922.0
122.00	781.0
123.00	1258.0
123.90	555.0
125.00	524.0
127.00	47416.0
128.00	3566.0
129.00	16944.0
130.00	1703.0
130.90	314.0
134.00	546.0
135.00	1332.0
135.90	541.0
137.00	835.0
141.00	2337.0
141.90	887.0
143.00	465.0
146.00	550.0
146.90	1331.0
148.00	2887.0
149.00	623.0
152.90	812.0
153.90	660.0
155.00	1491.0
156.00	2057.0
156.90	408.0
157.80	377.0
159.90	719.0
161.00	1122.0
162.00	331.0
164.90	1012.0
165.90	672.0
167.00	5066.0
168.00	3144.0
169.00	516.0
171.90	485.0
172.90	525.0
174.00	992.0
175.00	2169.0
176.00	459.0
176.90	894.0
179.00	3624.0
180.00	2492.0
181.00	1246.0

Instrument :

BNA_M

ClientSampleId :

DFTPP57

185.00	1507.0
186.00	13763.0
187.00	3932.0
188.00	437.0
189.00	850.0
191.00	455.0
192.00	1166.0
193.00	1580.0
196.00	2909.0
196.80	444.0
198.00	99928.0
198.90	6772.0
199.90	502.0
201.50	395.0
203.00	696.0
204.00	3852.0
205.00	6502.0
206.00	26000.0
207.00	3806.0
208.00	842.0
208.90	357.0
210.20	344.0
210.90	1013.0
216.00	519.0
217.00	7124.0
218.00	842.0
221.00	3635.0
221.80	1020.0
223.00	1620.0
224.00	14608.0
225.00	4041.0
226.00	386.0
227.00	6023.0
228.00	995.0
228.90	1330.0
231.00	567.0
234.10	387.0
235.00	464.0
236.90	575.0
241.00	309.0
241.90	746.0
243.10	809.0
244.00	11794.0
245.00	1580.0
246.00	2308.0
247.00	414.0
249.00	360.0
255.00	58456.0
256.00	8681.0
257.00	607.0
258.00	3416.0
259.00	566.0
265.00	1530.0
273.00	1603.0
274.00	4534.0
275.00	25128.0
276.00	3247.0
277.00	2035.0
277.90	424.0
285.00	365.0
293.00	500.0
296.00	7205.0
296.90	953.0
303.10	857.0
313.90	323.0
315.00	858.0
316.00	511.0
323.00	2490.0
324.00	461.0
326.90	503.0
334.00	1318.0
335.00	411.0
345.90	497.0
352.10	647.0
353.00	396.0
354.00	713.0
365.00	3089.0
365.90	556.0
372.00	1103.0
383.00	307.0
402.00	440.0
403.00	609.0
421.00	528.0
422.00	493.0
423.10	3808.0
424.00	839.0
441.10	10920.0
442.10	73152.0
443.00	13748.0
444.10	1358.0

Instrument :
BNA_M
ClientSampleId :
DFTPP57

m/z	Abundance
39.00	2203.0
40.00	372.0
49.00	374.0
50.00	6890.0
51.00	28336.0
52.00	1509.0
56.00	875.0
57.00	1980.0
61.00	390.0
61.90	462.0
63.00	1218.0
65.00	552.0
68.00	392.0
69.00	29728.0
74.00	2995.0
75.00	4914.0
76.00	1634.0
77.00	36984.0
78.00	2415.0
79.00	2064.0
80.00	1545.0
81.00	2455.0
81.90	613.0
83.00	578.0
85.00	654.0
86.00	731.0
87.00	333.0
91.00	668.0
91.90	592.0
93.00	4093.0
98.00	2967.0
99.00	2633.0
101.00	1388.0
103.00	408.0
104.00	947.0
105.00	972.0
107.00	11487.0
108.00	1674.0
109.00	350.0
110.00	20496.0
111.00	3216.0
112.00	343.0
116.00	678.0
117.00	9474.0
118.00	662.0
121.90	706.0
123.00	1241.0
123.90	484.0
124.90	521.0
127.00	41696.0
128.00	3115.0
129.00	15315.0
129.90	1278.0
133.90	349.0
135.00	1303.0
136.00	566.0
136.90	702.0
141.00	2038.0
141.90	676.0
143.00	533.0
146.00	388.0
146.90	978.0
148.00	2522.0
148.90	503.0
153.00	657.0
153.90	522.0
155.00	1207.0
156.00	1681.0
157.00	349.0
157.90	354.0
160.00	627.0
161.00	1126.0
165.00	784.0
166.00	695.0
167.00	4668.0
168.00	2490.0
168.90	361.0
171.90	324.0
172.90	568.0
174.00	910.0
175.00	1811.0
176.00	389.0
176.90	823.0
179.00	3340.0
180.00	2083.0
181.00	1254.0
185.00	1671.0
186.00	12191.0
187.00	3657.0
188.00	395.0
189.00	656.0

Instrument :
BNA_M
ClientSampleId :
DFTPP57

190.90	309.0
192.00	1170.0
193.00	1254.0
196.00	2404.0
197.00	441.0
198.00	92856.0
199.00	6237.0
199.90	529.0
201.50	472.0
203.00	643.0
204.00	3592.0
205.00	6122.0
206.00	25400.0
207.00	3155.0
208.00	791.0
210.20	454.0
211.00	1202.0
216.00	610.0
217.00	6653.0
218.00	853.0
221.00	3594.0
221.90	819.0
223.00	1448.0
224.00	14474.0
225.00	3389.0
226.00	374.0
227.00	5853.0
227.90	853.0
229.00	1222.0
231.00	575.0
233.90	400.0
234.90	412.0
236.00	319.0
237.00	382.0
242.00	898.0
243.00	865.0
244.00	10897.0
245.00	1402.0
246.00	2298.0
246.90	390.0
249.00	410.0
253.00	307.0
254.00	435.0
255.00	57096.0
256.00	8169.0
257.00	563.0
258.00	3200.0
258.90	431.0
265.00	1389.0
273.00	1908.0
274.00	4494.0
275.00	25328.0
276.00	3388.0
277.00	2275.0
277.90	444.0
285.00	413.0
293.00	447.0
296.00	7551.0
297.00	1067.0
303.00	874.0
314.00	369.0
315.00	843.0
315.90	422.0
323.10	2175.0
324.10	511.0
327.00	446.0
334.00	1524.0
335.00	309.0
341.00	300.0
346.00	565.0
352.00	677.0
353.00	449.0
354.00	683.0
365.00	3291.0
366.00	510.0
372.00	1265.0
382.90	395.0
402.00	564.0
403.00	734.0
421.00	803.0
422.00	607.0
423.00	4147.0
424.00	1068.0
441.00	13265.0
442.00	88008.0
443.10	16616.0
444.00	1570.0

Instrument :
BNA_M
ClientSampleId :
DFTPP57

m/z	Abundance
44.00	326.0

Instrument :
BNA_M
ClientSampleId :
DFTPP57