

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061520\
 Data File : BM026390.D
 Acq On : 15 Jun 2020 14:19
 Operator : JU/CG
 Sample : PB129539BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jun 15 16:14:43 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM060520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 15 12:22:53 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.40	152	102137	20.00	ng	0.00
21) Naphthalene-d8	10.16	136	403634	20.00	ng	0.00
39) Acenaphthene-d10	14.06	164	247350	20.00	ng	0.00
64) Phenanthrene-d10	16.82	188	544754	20.00	ng	0.00
76) Chrysene-d12	21.02	240	568437	20.00	ng	0.00
86) Perylene-d12	23.11	264	603375	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.04	112	801222	138.70	ng	0.00
7) Phenol-d6	6.61	99	1086133	129.84	ng	0.00
23) Nitrobenzene-d5	8.55	82	759823	92.43	ng	0.00
42) 2,4,6-Tribromophenol	15.56	330	438151	146.23	ng	0.00
45) 2-Fluorobiphenyl	12.67	172	1534136	94.15	ng	0.00
79) Terphenyl-d14	19.47	244	2735046	93.40	ng	0.00


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061520\
Data File : BM026390.D
Acq On : 15 Jun 2020 14:19
Operator : JU/CG
Sample : PB129539BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jun 15 16:14:43 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 15 12:22:53 2020
Response via : Initial Calibration

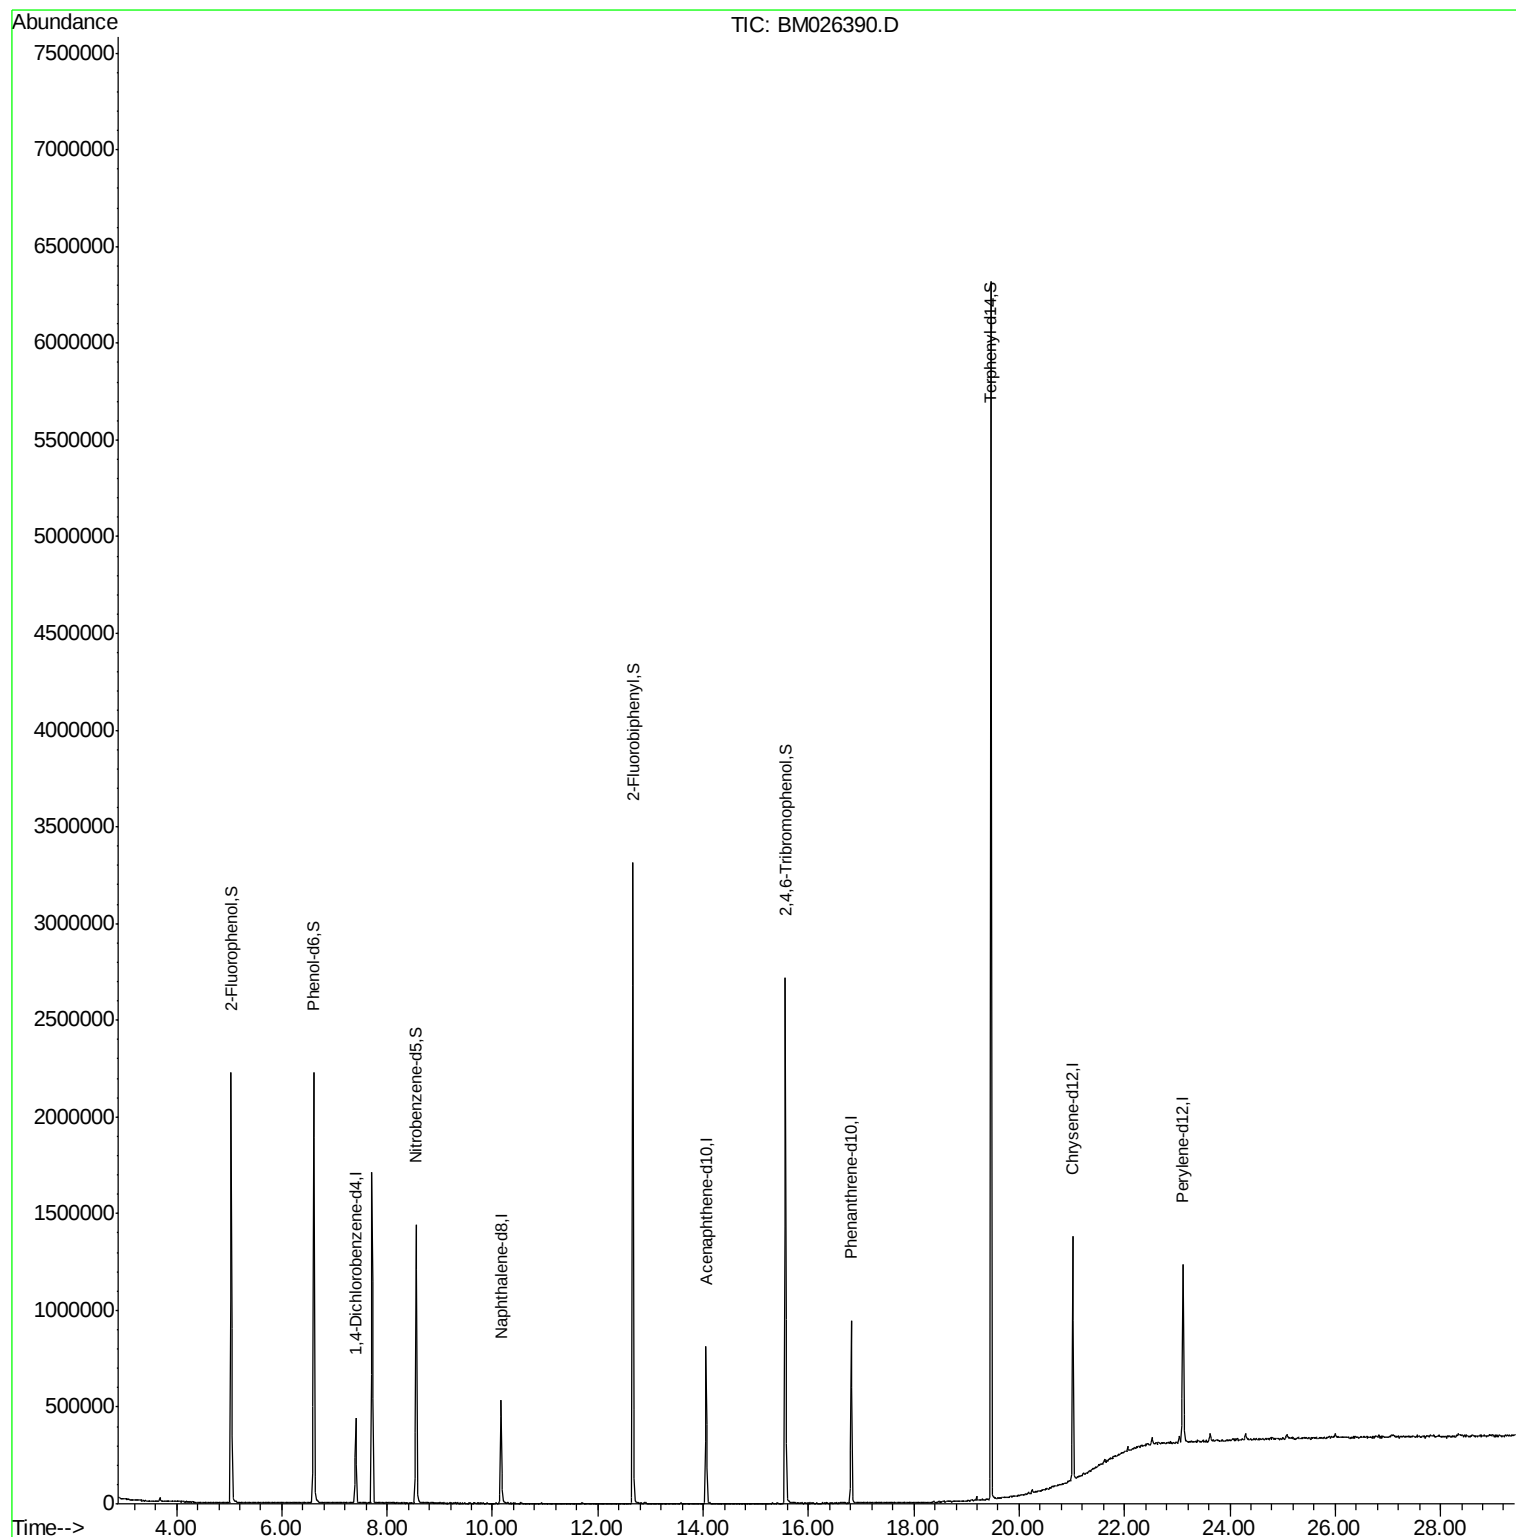




#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.40 min Scan# 768
Delta R.T. 0.00 min
Lab File: BM026390.D
Acq: 15 Jun 2020 14:19

Instrument :
BNA_M
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
152	100		
150	157.2	127.8	191.6
115	62.7	51.5	77.3



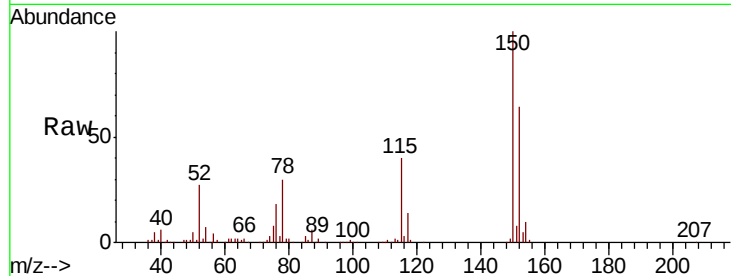


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

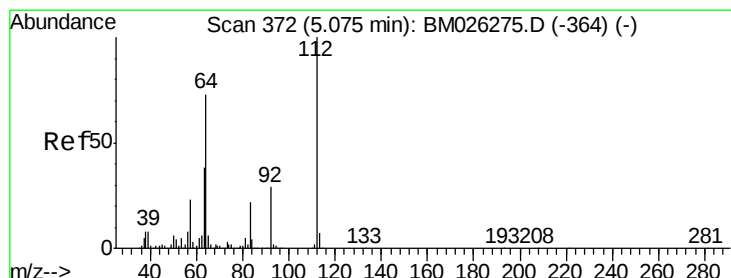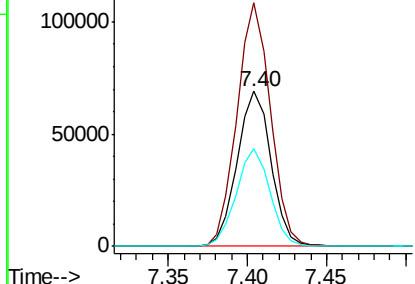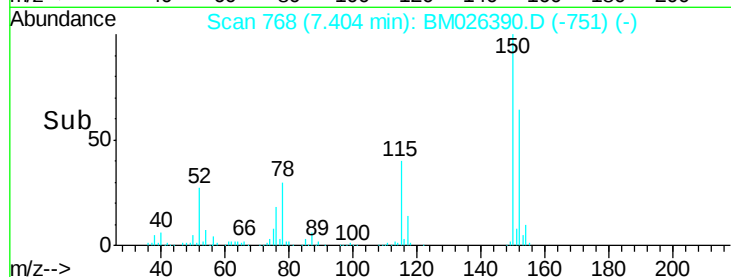

#5

2-Fluorophenol
Concen: 138.695 ng
RT: 5.04 min Scan# 366
Delta R.T. 0.00 min
Lab File: BM026390.D
Acq: 15 Jun 2020 14:19

Tgt Ion	Ratio	Lower	Upper
112	100		
64	68.7	56.0	84.0
63	35.6	29.0	43.6


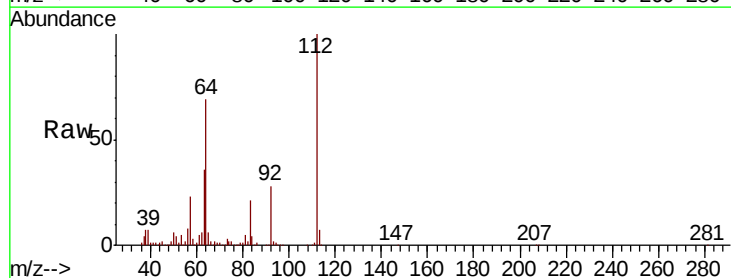



Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BM0

Ion 63.00 (62.70 to 63.70): BM0

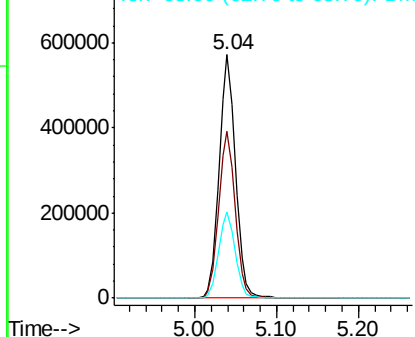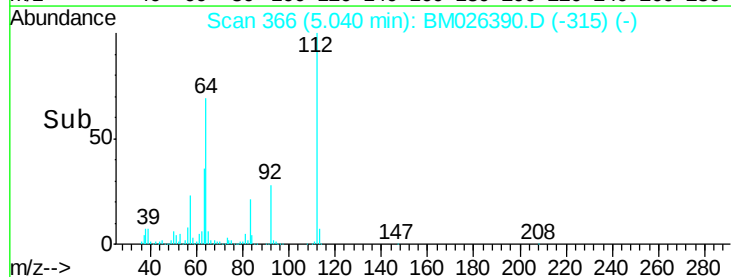

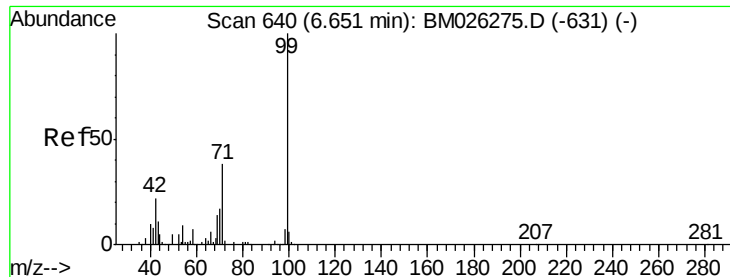

#7

Phenol-d6

Concen: 129.839 ng

RT: 6.61 min Scan# 633

Delta R.T. 0.00 min

Lab File: BM026390.D

Acq: 15 Jun 2020 14:19


Instrument :

BNA_M

ClientSampled :

Tot Ion: 99 Resp: 1086133

Ion	Ratio	Lower	Upper
99	100		
42	22.5	17.8	26.6
71	38.2	31.0	46.4



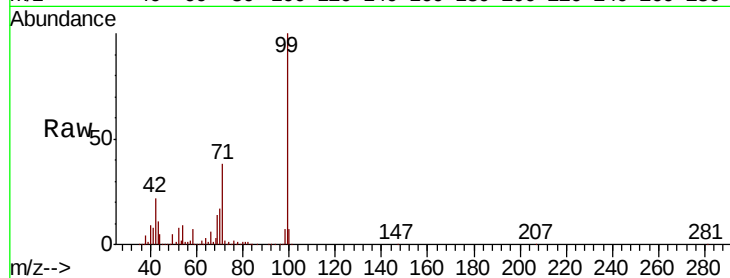


Abundance

Ion 99.00 (98.70 to 99.70): BM0

Ion 42.00 (41.70 to 42.70): BM0

Ion 71.00 (70.70 to 71.70): BM0

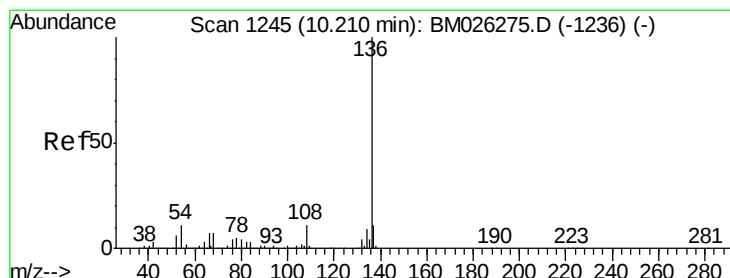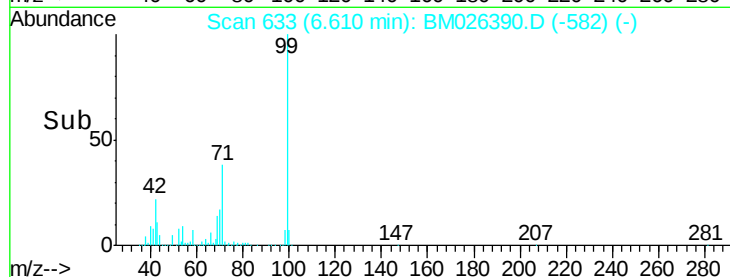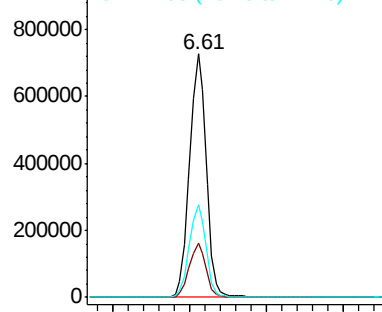

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.16 min Scan# 1237


Delta R.T. 0.00 min

Lab File: BM026390.D

Acq: 15 Jun 2020 14:19

Tgt Ion: 136 Resp: 403634

Ion	Ratio	Lower	Upper
136	100		
137	10.9	8.5	12.7
54	11.1	9.0	13.6
68	7.6	5.6	8.4

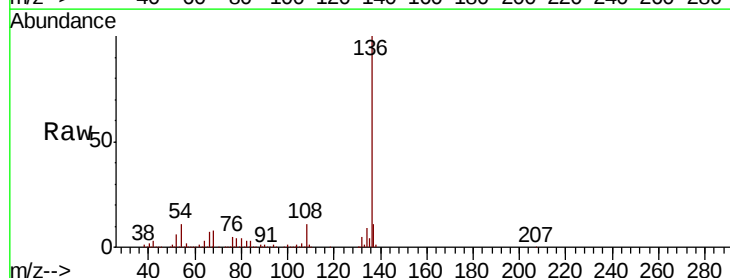



Abundance


Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BM0

Ion 68.00 (67.70 to 68.70): BM0



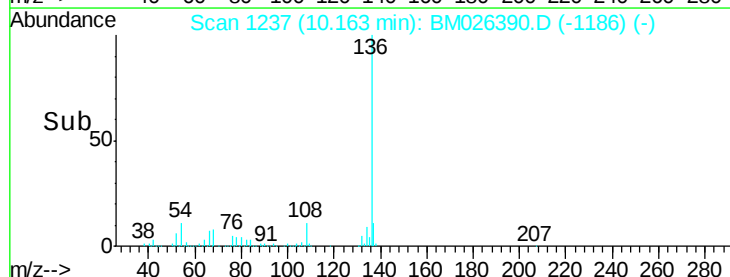
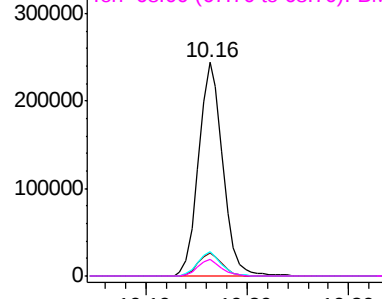


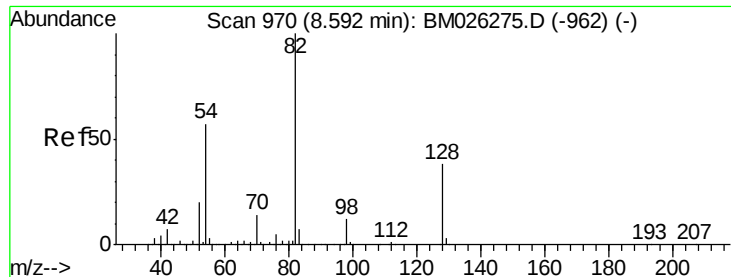

#23
Nitrobenzene-d5
Concen: 92.428 ng
RT: 8.55 min Scan# 963
Delta R.T. 0.00 min
Lab File: BM026390.D
Acq: 15 Jun 2020 14:19




Instrument :
BNA_M
ClientSampleId :


Tot Ion	82	Resp	759823
Ion Ratio	Lower	Upper	
82	100		
128	39.2	31.0	46.6
54	57.2	45.4	68.2

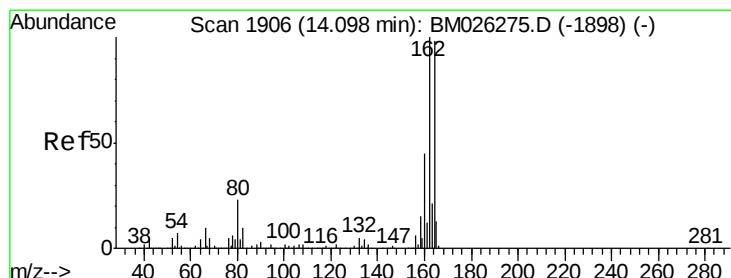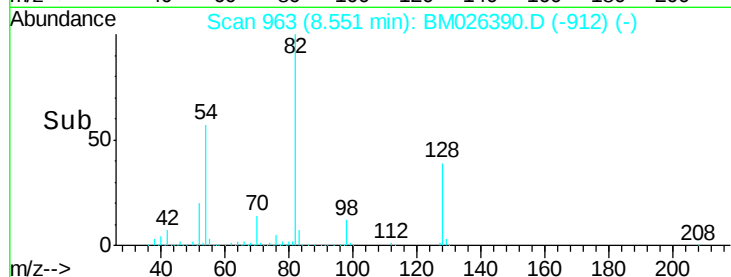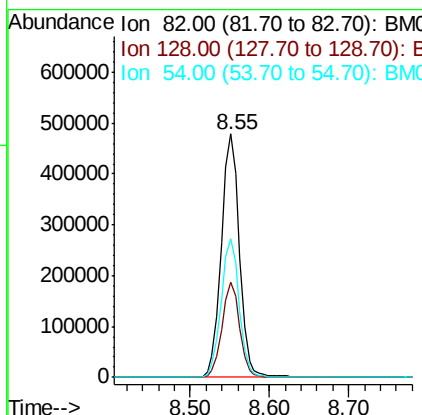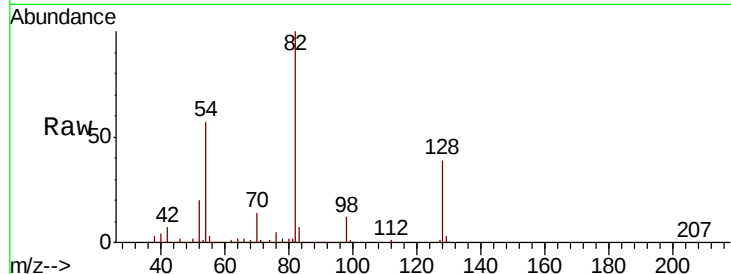

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.06 min Scan# 1899
Delta R.T. 0.00 min
Lab File: BM026390.D
Acq: 15 Jun 2020 14:19

Tgt Ion	164	Resp	247350
Ion Ratio	Lower	Upper	
164	100		
162	103.0	77.7	116.5
160	43.6	34.2	51.2

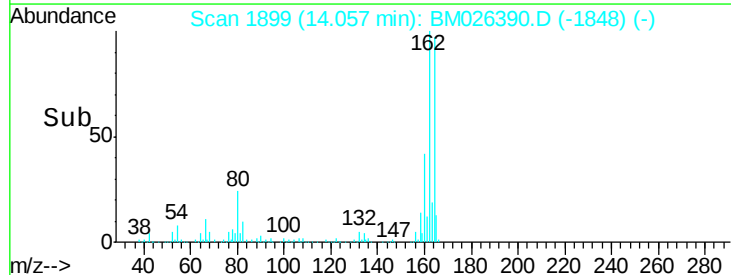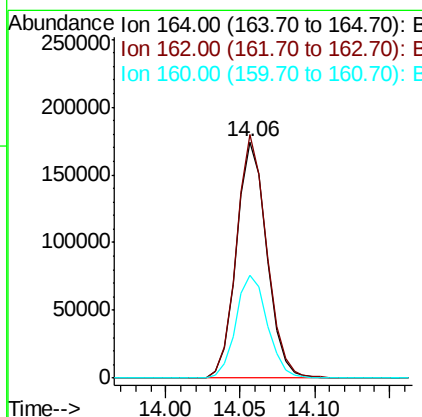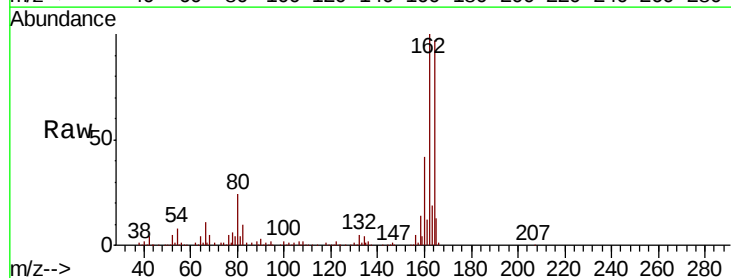


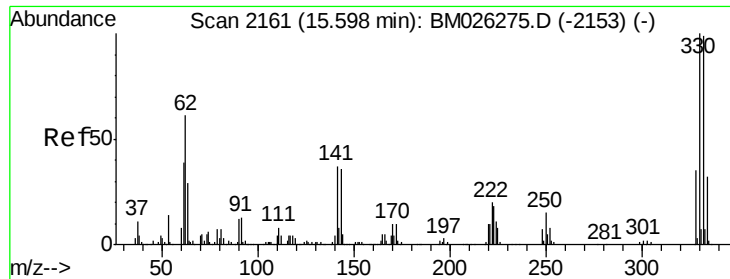




#42
 2,4,6-Tribromophenol
 Concen: 146.232 ng
 RT: 15.56 min Scan# 2155
 Delta R.T. 0.00 min
 Lab File: BM026390.D
 Acq: 15 Jun 2020 14:19

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion:330 Resp: 438151
 Ion Ratio Lower Upper
 330 100
 332 96.5 77.7 116.5
 141 37.7 29.7 44.5

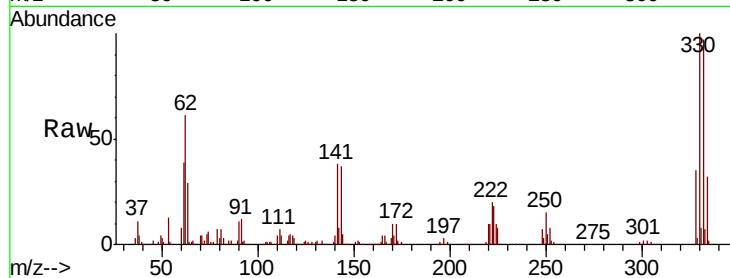


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

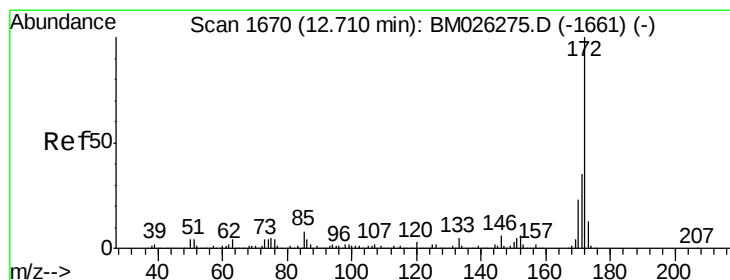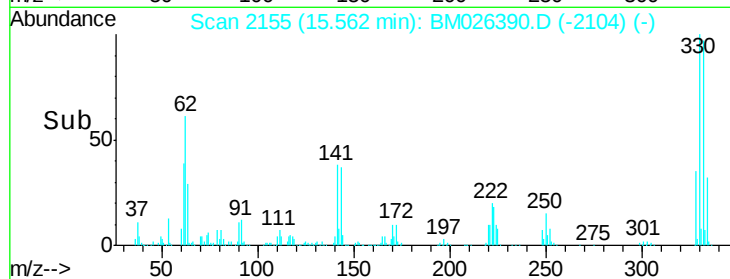
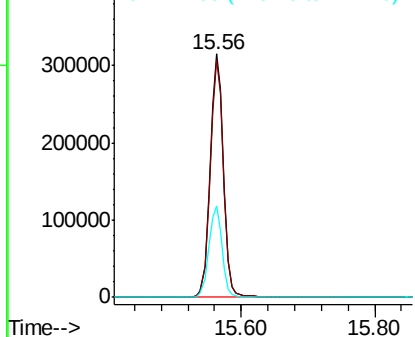



#45
 2-Fluorobiphenyl
 Concen: 94.149 ng
 RT: 12.67 min Scan# 1663
 Delta R.T. 0.00 min
 Lab File: BM026390.D
 Acq: 15 Jun 2020 14:19

Tgt Ion:172 Resp: 1534136
 Ion Ratio Lower Upper
 172 100
 171 34.7 27.8 41.8
 170 22.7 18.2 27.4

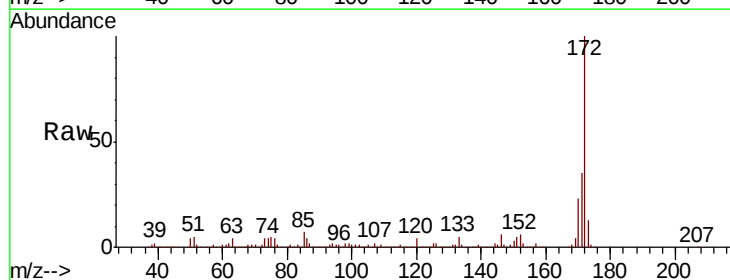

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

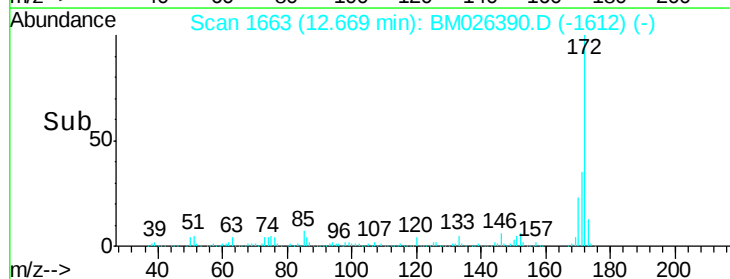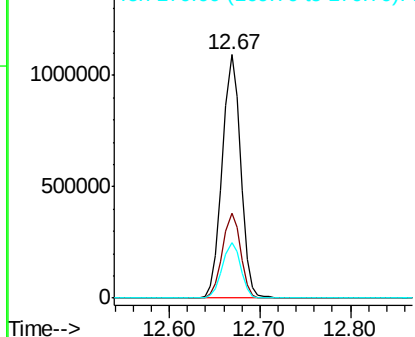

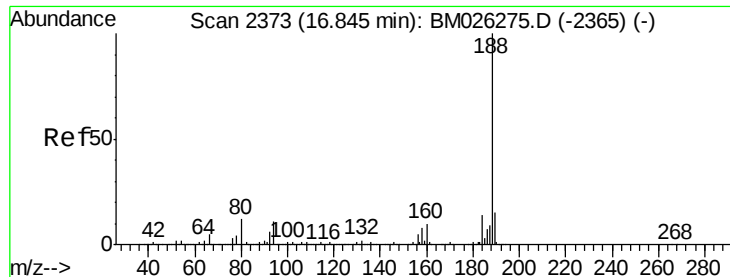

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 16.82 min Scan# 2368

Delta R.T. 0.00 min

Lab File: BM026390.D

Acq: 15 Jun 2020 14:19

Instrument :

BNA_M

ClientSampled :


Tot Ion:188 Resp: 544754

Ion Ratio Lower Upper

188 100

94 9.6 7.8 11.6

80 11.4 9.5 14.3

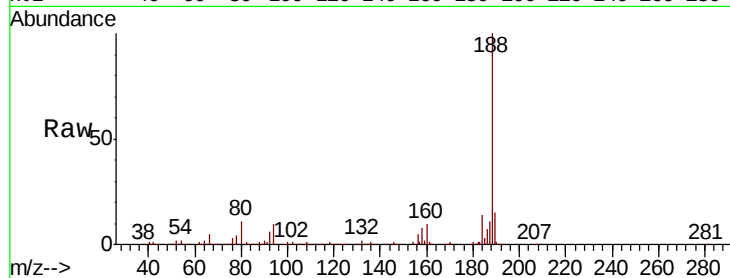

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BM

Ion 80.00 (79.70 to 80.70): BM

500000

400000

300000

200000

100000



0

16.82

16.80

16.90

Time-->

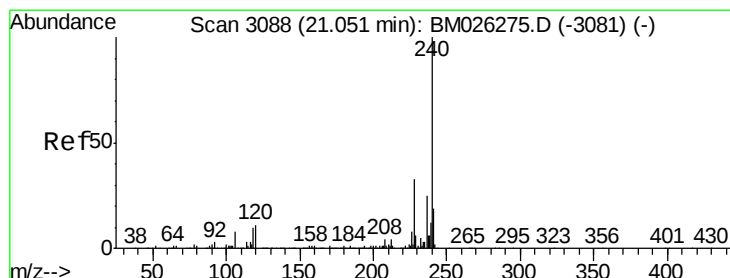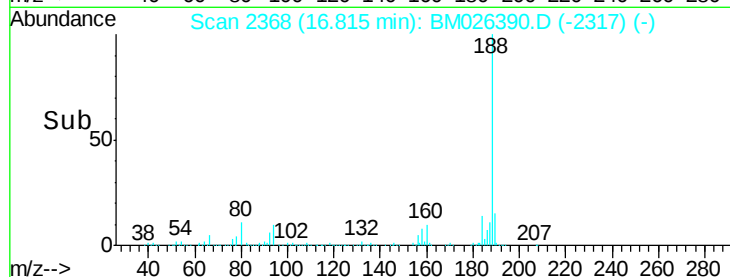

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.02 min Scan# 3083

Delta R.T. 0.00 min

Lab File: BM026390.D

Acq: 15 Jun 2020 14:19


Tgt Ion:240 Resp: 568437

Ion Ratio Lower Upper

240 100

120 9.5 9.3 13.9

236 25.3 19.4 29.0

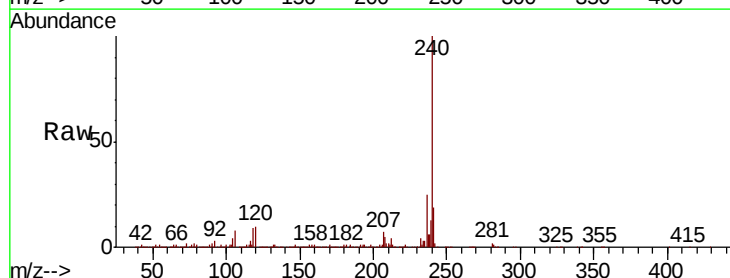

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

600000

500000

400000

300000

200000

100000


0


21.02

21.00

21.10

Time-->




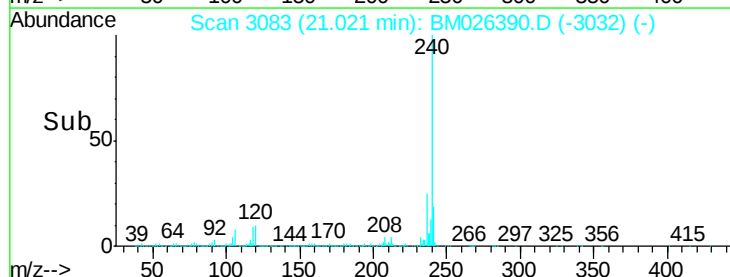


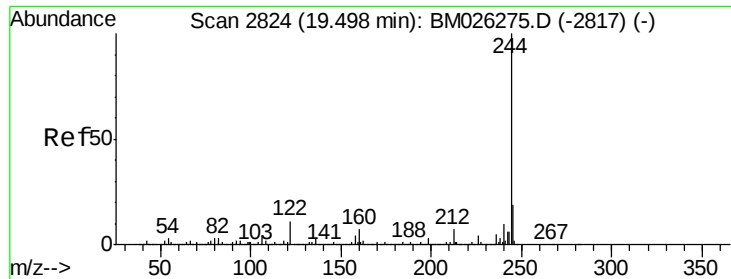

#79
 Terphenyl-d14
 Concen: 93.400 ng
 RT: 19.47 min Scan# 2819
 Delta R.T. 0.00 min
 Lab File: BM026390.D
 Acq: 15 Jun 2020 14:19

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion:244 Resp: 2735046
 Ion Ratio Lower Upper
 244 100
 212 7.2 5.9 8.9
 122 10.5 8.6 13.0

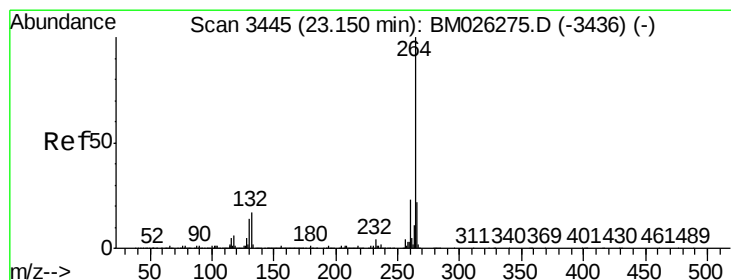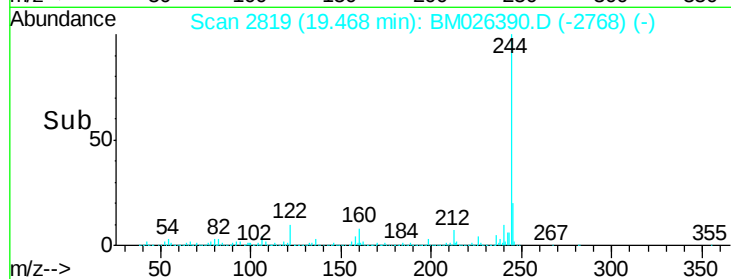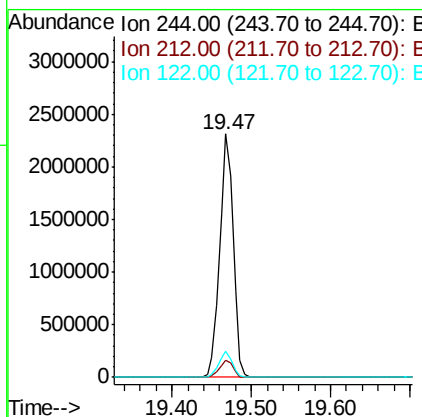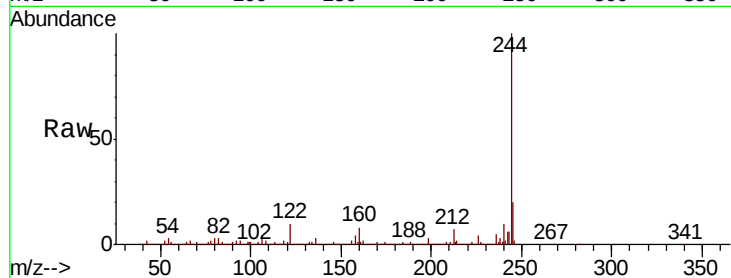

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.11 min Scan# 3438
 Delta R.T. -0.01 min
 Lab File: BM026390.D
 Acq: 15 Jun 2020 14:19

Tgt Ion:264 Resp: 603375
 Ion Ratio Lower Upper
 264 100
 260 23.0 18.6 28.0
 265 21.6 17.8 26.6

